
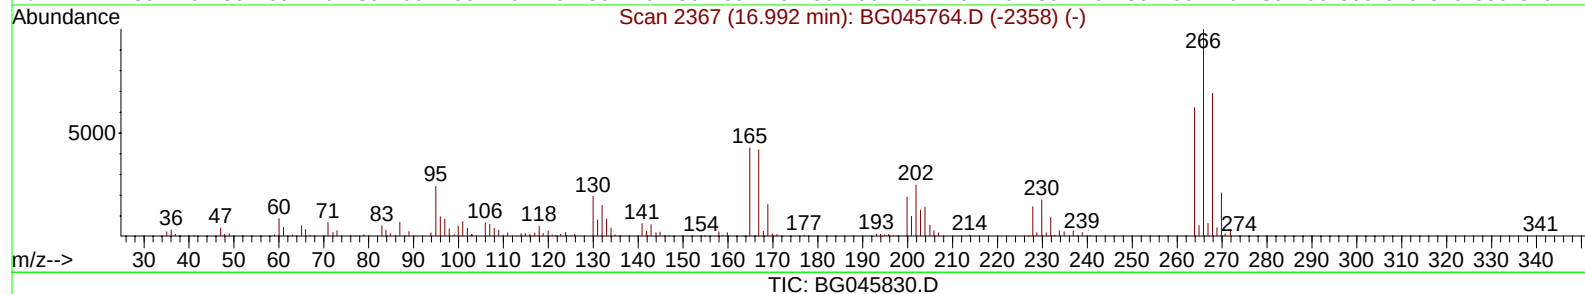
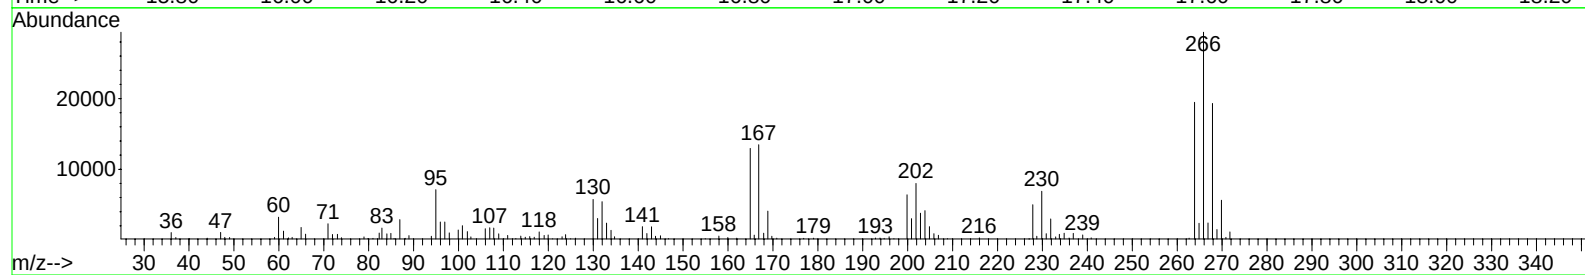


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062320\
Data File : BG045830.D
Acq On : 23 Jun 2020 8:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 16:51:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 18:34:19 2020
Response via : Initial Calibration

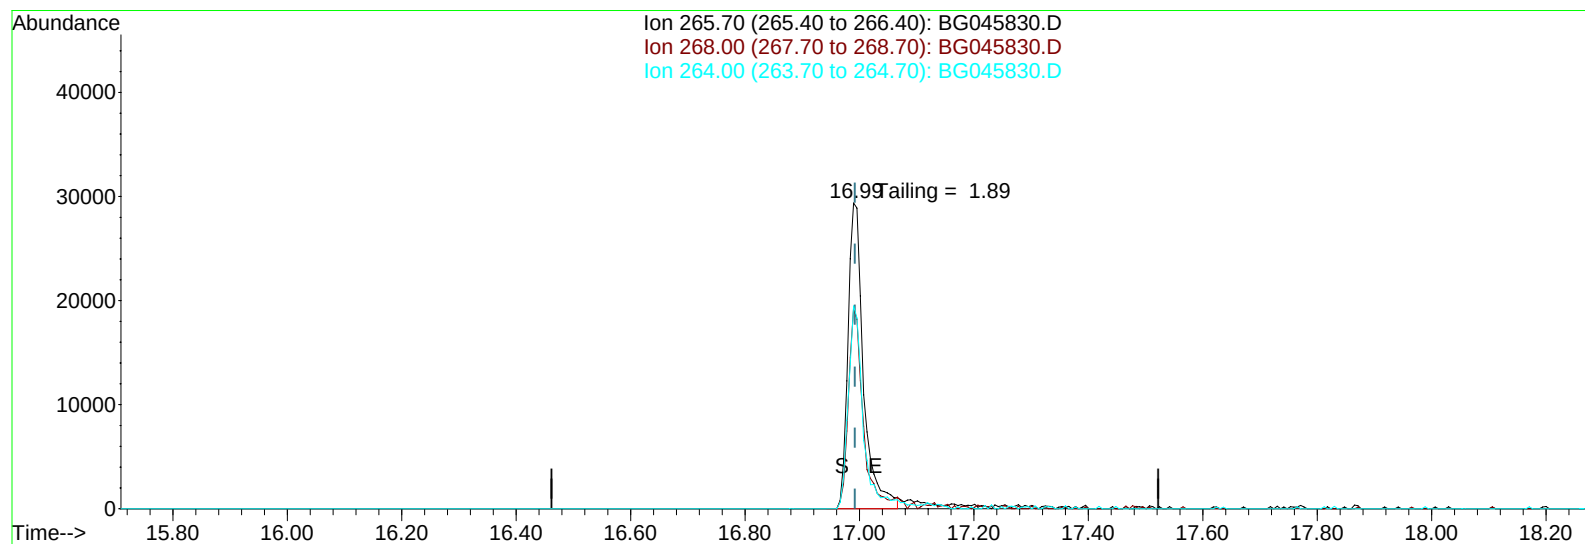

(70) Pentachlorophenol (C)




16.990min (-0.002) 33468.20ng

response 56041

Ion	Exp%	Act%
265.70	100	100
268.00	69.20	65.74
264.00	62.20	66.29
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062320\
 Data File : BG045830.D
 Acq On : 23 Jun 2020 8:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 16:51:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 15 18:34:19 2020
 Response via : Initial Calibration

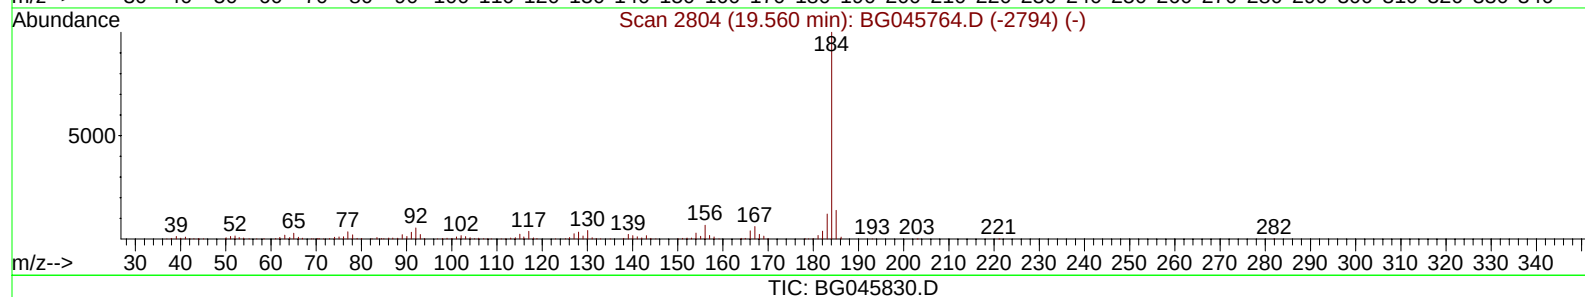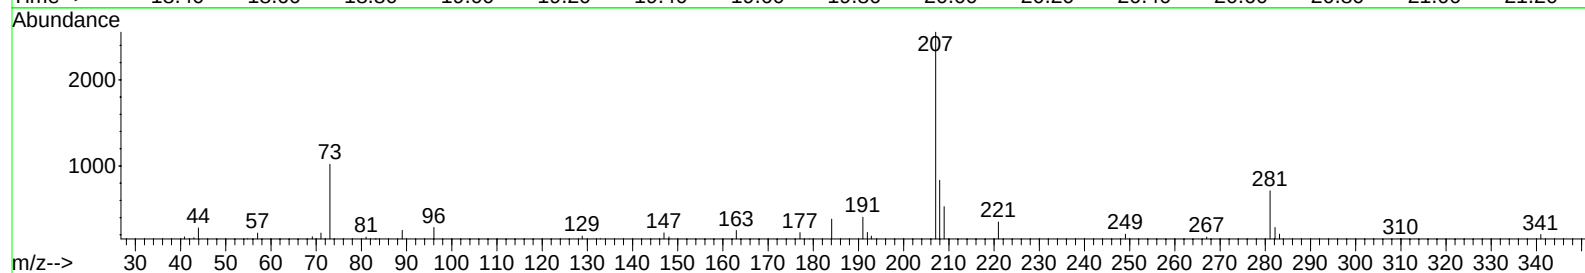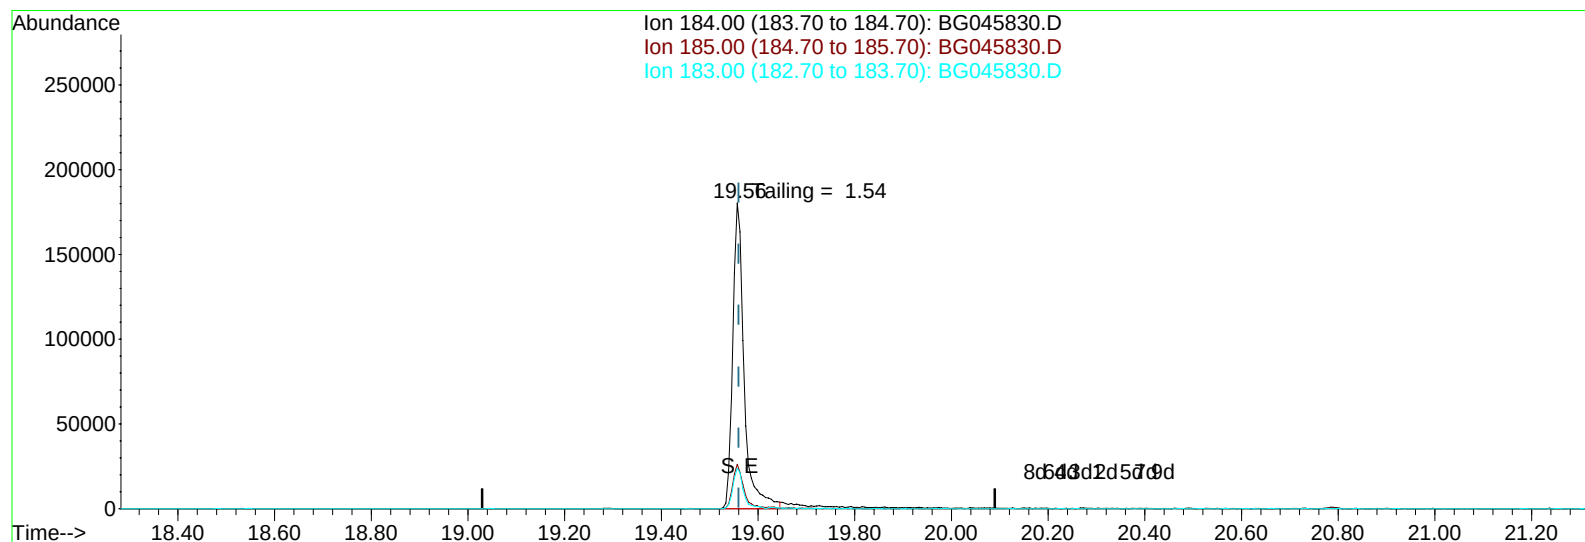

(77) Benzidine

20.303min (+0.743) 137.45ng

response 268

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	0.00#
183.00	12.10	0.00#
0.00	0.00	0.00