

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062320\
 Data File : BG045835.D
 Acq On : 23 Jun 2020 11:36
 Operator : CG/JU
 Sample : L3033-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SS043MW100-200615

Quant Time: Jun 24 02:27:52 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 15 18:34:19 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	53246	20.00	ng	0.00
21) Naphthalene-d8	10.72	136	212971	20.00	ng	0.00
39) Acenaphthene-d10	14.57	164	147255	20.00	ng	0.00
64) Phenanthrene-d10	17.32	188	319822	20.00	ng	0.00
76) Chrysene-d12	21.57	240	316802	20.00	ng	0.00
86) Perylene-d12	24.70	264	335828	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.53	112	134391	42.64	ng	-0.01
7) Phenol-d6	7.14	99	120469	25.13	ng	-0.02
23) Nitrobenzene-d5	9.08	82	359480	77.11	ng	0.00
42) 2,4,6-Tribromophenol	16.06	330	273213	122.89	ng	0.00
45) 2-Fluorobiphenyl	13.19	172	852346	85.06	ng	0.00
79) Terphenyl-d14	19.94	244	1383188	88.48	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.38	88	3812	2.640	ng	91
50) Dimethylphthalate	14.02	163	133550	11.577	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062320\
Data File : BG045835.D
Acq On : 23 Jun 2020 11:36
Operator : CG/JU
Sample : L3033-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SS043MW100-200615

Quant Time: Jun 24 02:27:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 18:34:19 2020
Response via : Initial Calibration

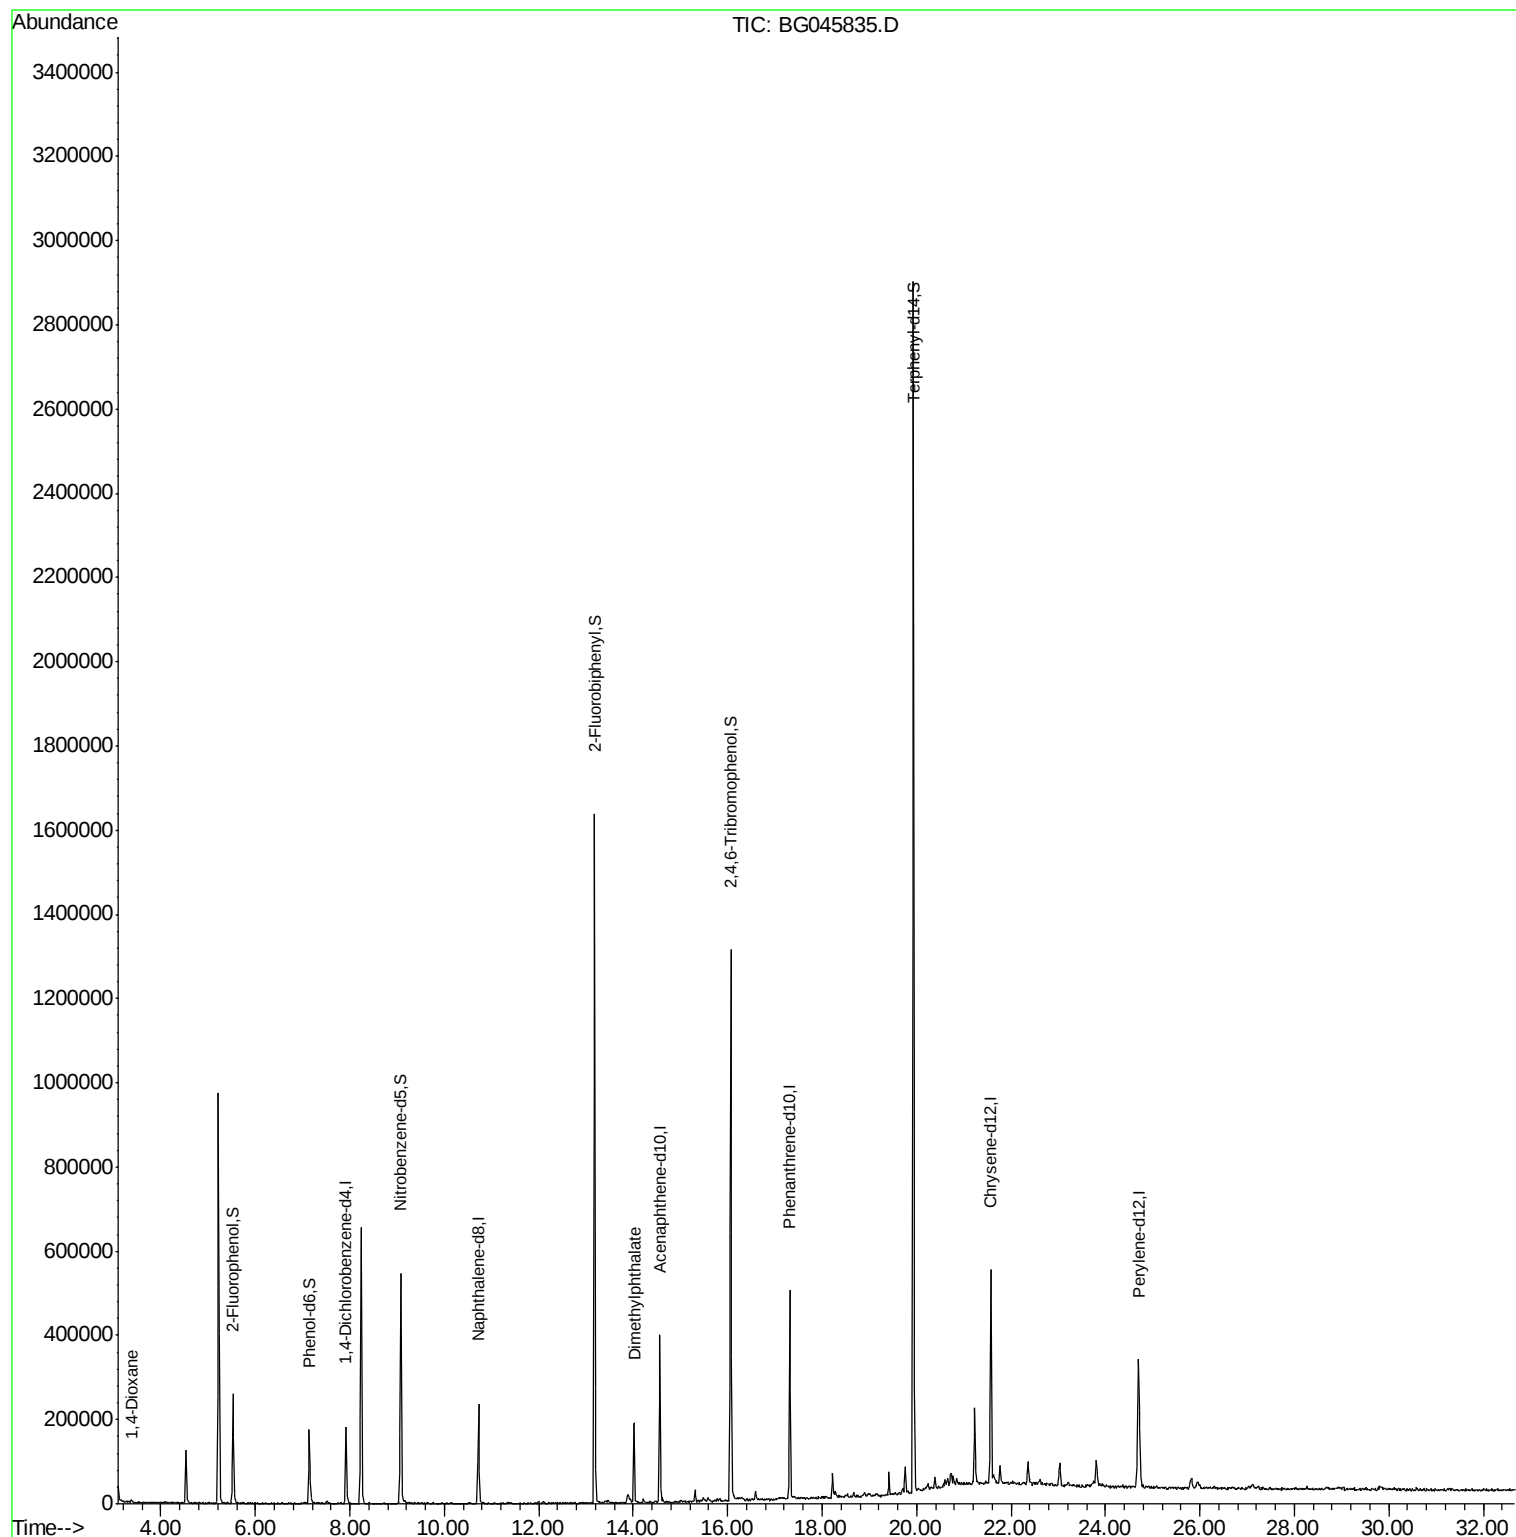




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.92 min Scan# 822
Delta R.T. -0.01 min
Lab File: BG045835.D
Acq: 23 Jun 2020 11:36

Instrument :
BNA_G
ClientSampleId :
SS043MW100-200615

Tot Ion:152 Resp: 53246
Ion Ratio Lower Upper
152 100
150 160.2 113.1 169.7
115 61.3 43.8 65.6

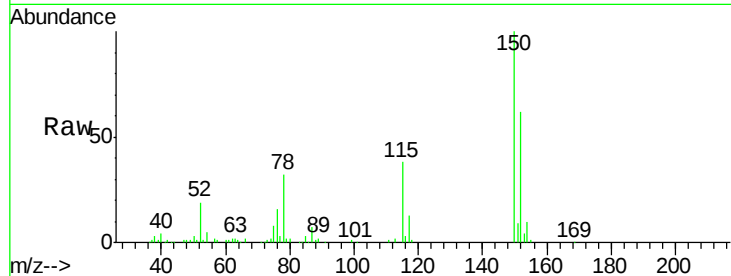


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

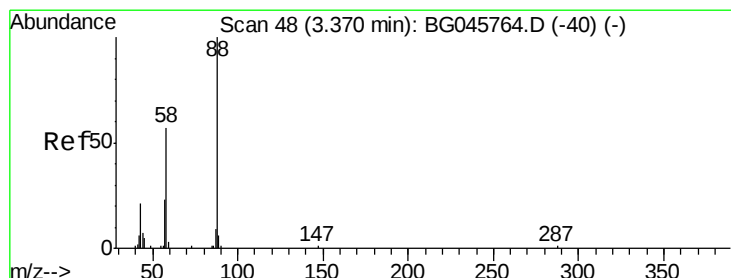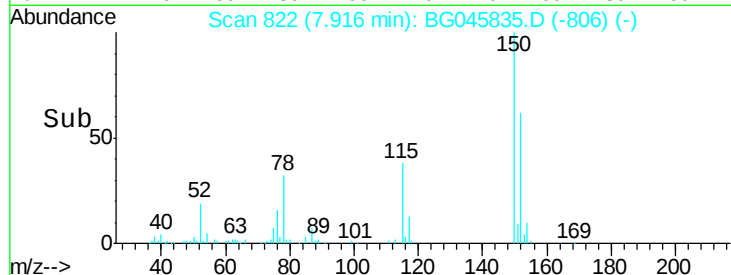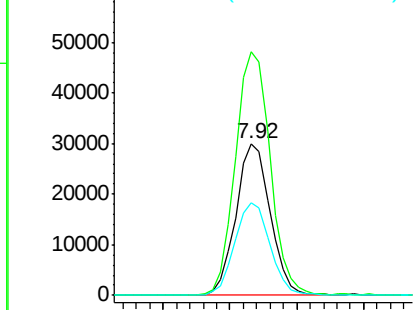



#2


1,4-Dioxane
Concen: 2.640 ng
RT: 3.38 min Scan# 49
Delta R.T. 0.01 min
Lab File: BG045835.D
Acq: 23 Jun 2020 11:36

Tgt Ion: 88 Resp: 3812
Ion Ratio Lower Upper
88 100
58 49.0 46.1 69.1
43 23.2 19.2 28.8

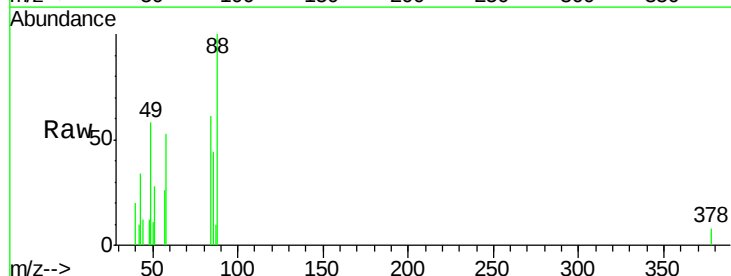

Abundance Ion 88.00 (87.70 to 88.70): BGC
Ion 58.00 (57.70 to 58.70): BGC
Ion 43.00 (42.70 to 43.70): BGC

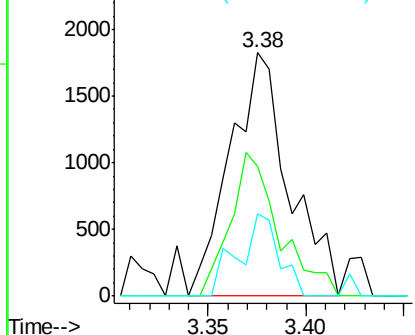



#5

2-Fluorophenol

Concen: 42.636 ng

RT: 5.53 min Scan# 415

Delta R.T. -0.01 min

Lab File: BG045835.D

Acq: 23 Jun 2020 11:36

Instrument :

BNA_G

ClientSampleId :

SS043MW100-200615


Tot Ion:112 Resp: 134391

Ion Ratio Lower Upper

112 100

64 52.3 46.6 69.8




63 32.3 26.3 39.5

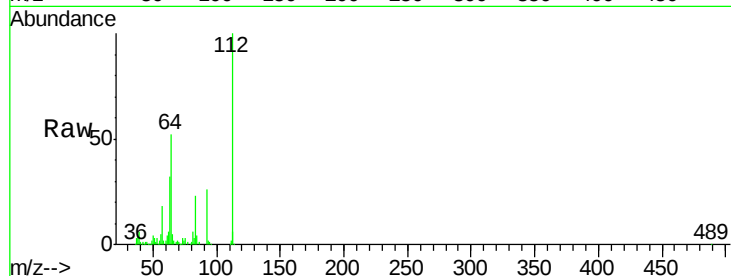

Abundance Ion 112.00 (111.70 to 112.70): BGC

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

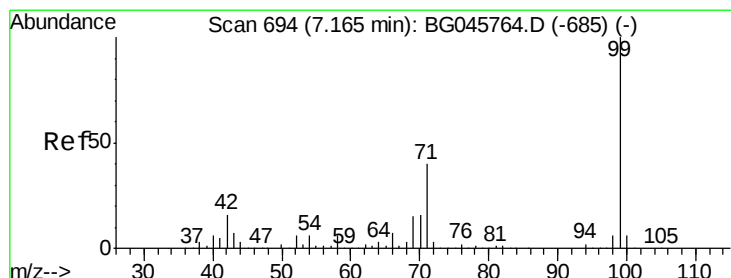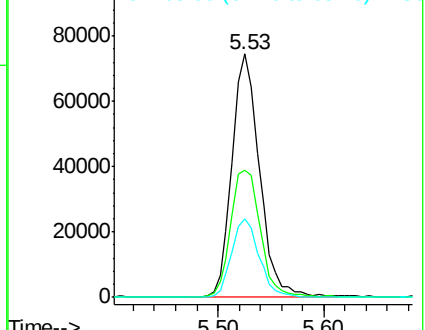

#7

Phenol-d6

Concen: 25.126 ng

RT: 7.14 min Scan# 690

Delta R.T. -0.02 min

Lab File: BG045835.D

Acq: 23 Jun 2020 11:36


Tgt Ion: 99 Resp: 120469

Ion Ratio Lower Upper

99 100

42 14.5 12.4 18.6



71 41.2 32.1 48.1

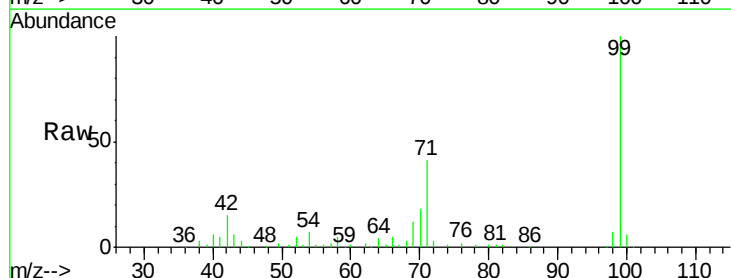


Abundance Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

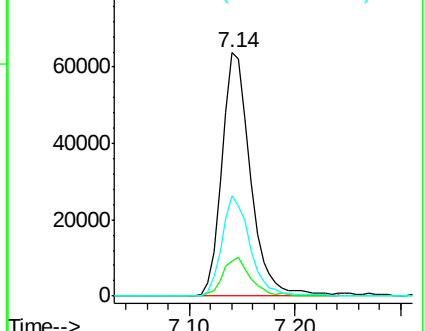



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.72 min Scan# 1300

Delta R.T. -0.00 min

Lab File: BG045835.D

Acq: 23 Jun 2020 11:36

Instrument :

BNA_G

ClientSampleId :

SS043MW100-200615

Tot Ion:136 Resp: 212971


Ion Ratio Lower Upper

136 100

137 10.8 8.7 13.1

54 6.1 5.8 8.6

68 4.7 4.0 6.0



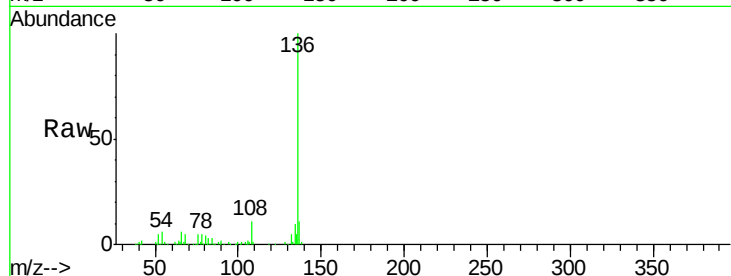


Abundance Ion 136.00 (135.70 to 136.70): B

Ion 137.00 (136.70 to 137.70): B

Ion 54.00 (53.70 to 54.70): B

Ion 68.00 (67.70 to 68.70): B

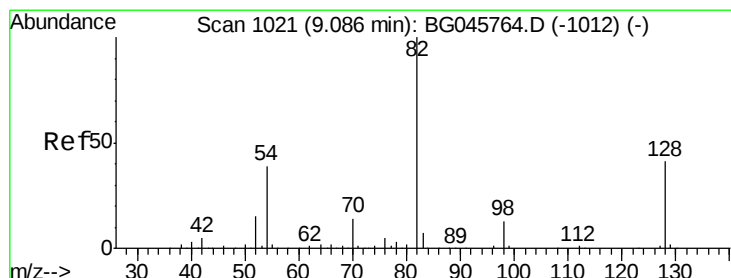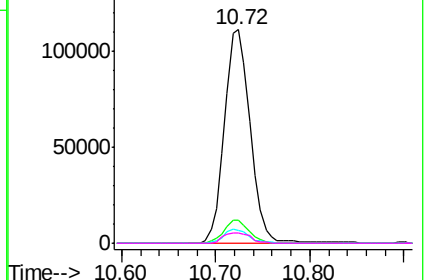

#23

Nitrobenzene-d5

Concen: 77.110 ng

RT: 9.08 min Scan# 1020

Delta R.T. -0.01 min

Lab File: BG045835.D

Acq: 23 Jun 2020 11:36


Tgt Ion: 82 Resp: 359480

Ion Ratio Lower Upper

82 100

128 37.1 32.5 48.7



54 41.4 31.2 46.8

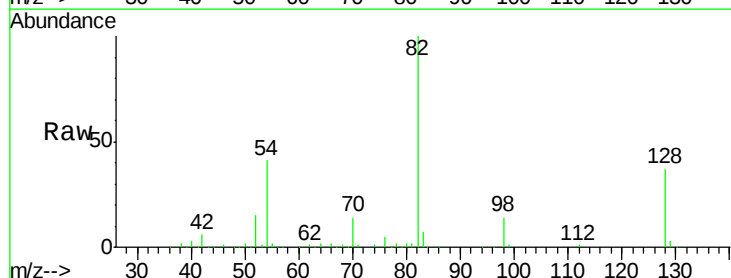


Abundance Ion 82.00 (81.70 to 82.70): B

Ion 128.00 (127.70 to 128.70): B

Ion 54.00 (53.70 to 54.70): B

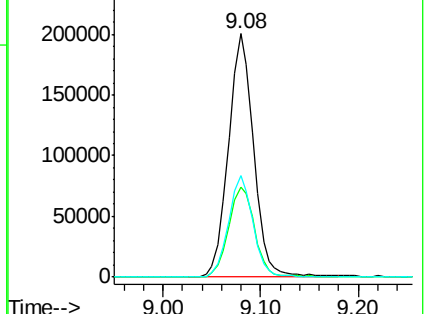



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.57 min Scan# 1954

Delta R.T. -0.00 min

Lab File: BG045835.D

Acq: 23 Jun 2020 11:36

Instrument :

BNA_G

ClientSampleId :

SS043MW100-200615


Tot Ion:164 Resp: 147255

Ion Ratio Lower Upper

164 100

162 97.6 77.4 116.0




160 41.7 33.3 49.9

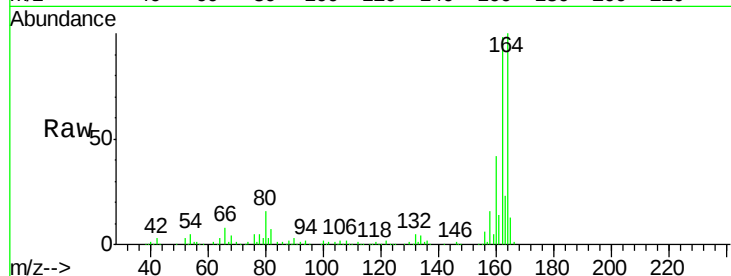

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

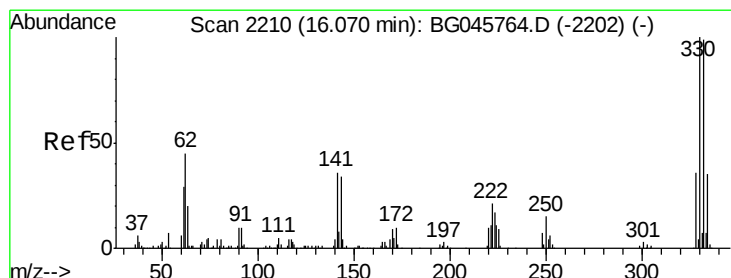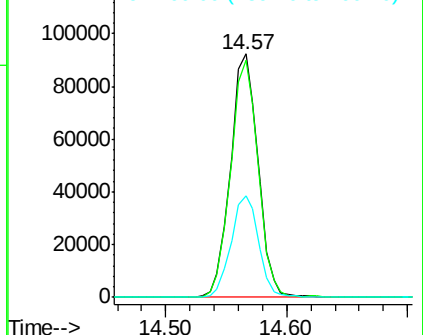

#42

2,4,6-Tribromophenol

Concen: 122.894 ng

RT: 16.06 min Scan# 2209

Delta R.T. -0.01 min

Lab File: BG045835.D

Acq: 23 Jun 2020 11:36


Tgt Ion:330 Resp: 273213

Ion Ratio Lower Upper

330 100

332 96.4 78.6 117.8



141 33.9 28.2 42.4

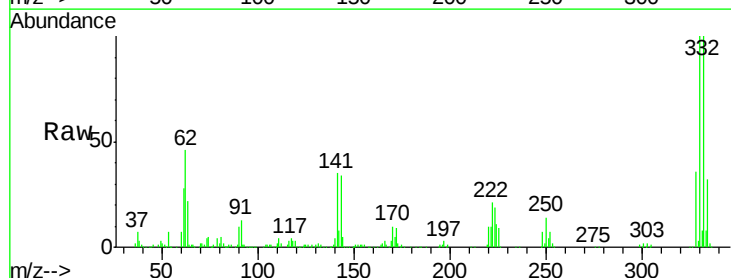


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



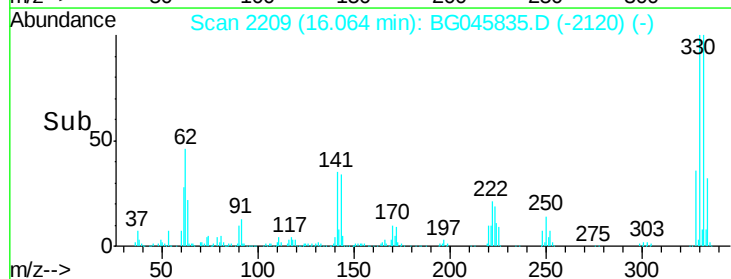
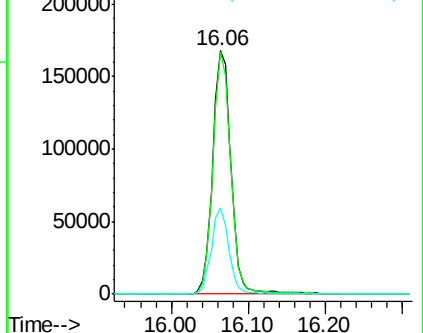


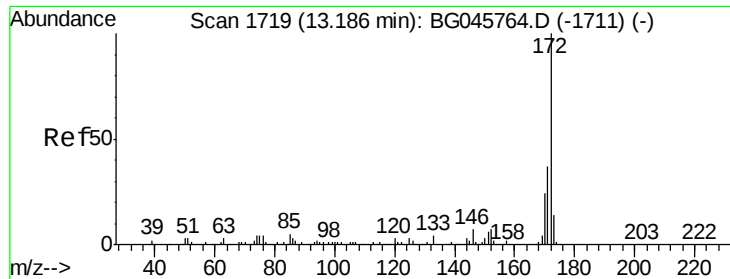

#45
2-Fluorobiphenyl
Concen: 85.061 ng
RT: 13.19 min Scan# 1719
Delta R.T. -0.00 min
Lab File: BG045835.D
Acq: 23 Jun 2020 11:36




Instrument :
BNA_G
ClientSampleId :
SS043MW100-200615


Tot Ion	Ratio	Lower	Upper
172	100		
171	36.6	29.9	44.9
170	24.0	19.3	28.9

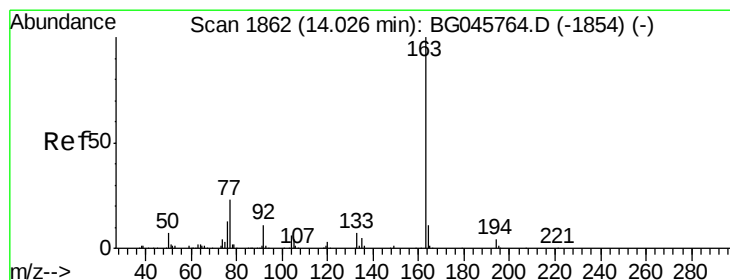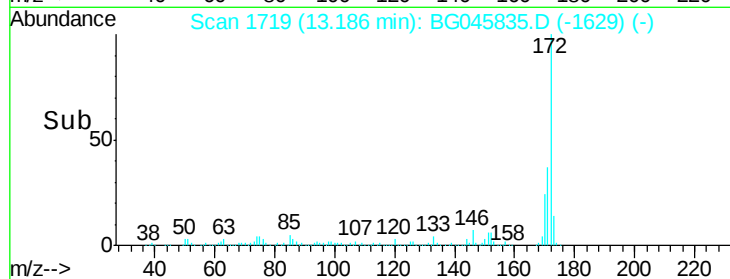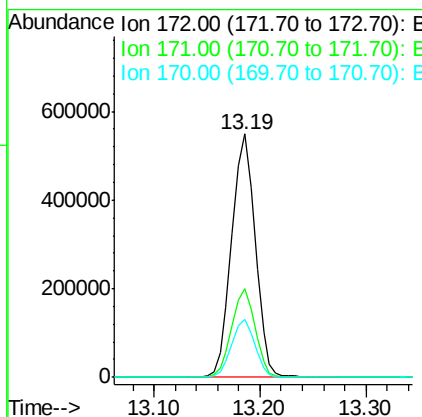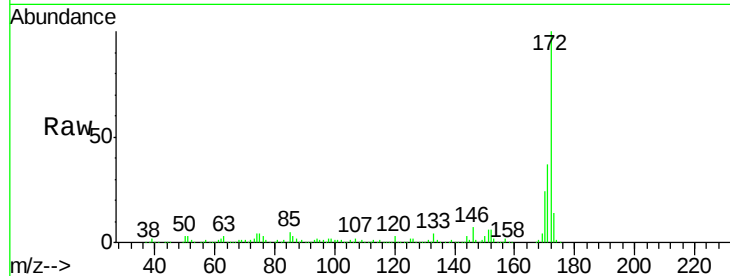

#50
Dimethylphthalate
Concen: 11.577 ng
RT: 14.02 min Scan# 1861
Delta R.T. -0.01 min
Lab File: BG045835.D
Acq: 23 Jun 2020 11:36

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.4	5.0
164	10.6	8.9	13.3

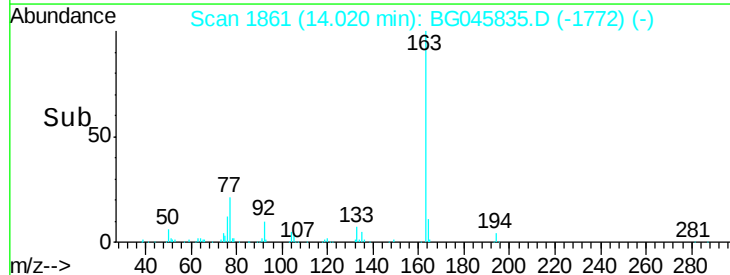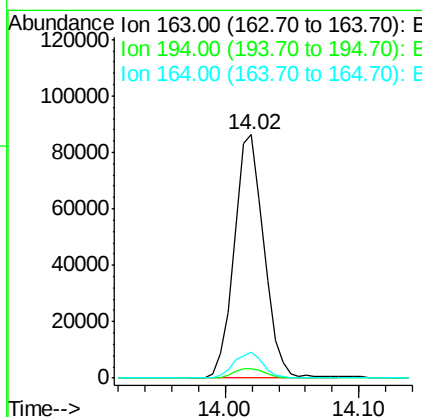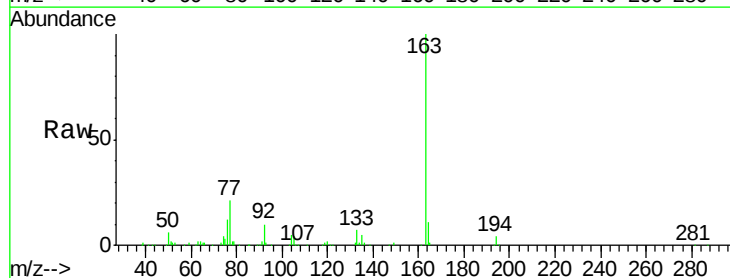

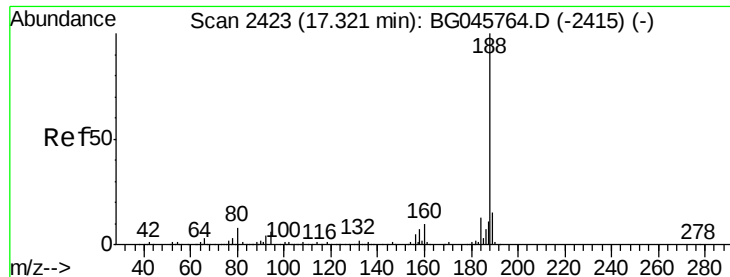

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.32 min Scan# 2422

Delta R.T. -0.01 min

Lab File: BG045835.D

Acq: 23 Jun 2020 11:36

Instrument :

BNA_G

ClientSampleId :

SS043MW100-200615


Tot Ion:188 Resp: 319822

Ion Ratio Lower Upper

188 100

94 6.7 5.1 7.7




80 7.7 6.2 9.4

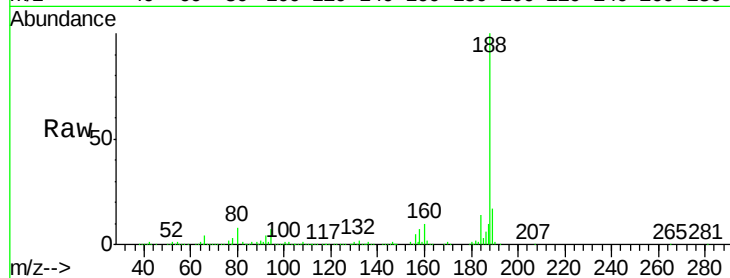

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

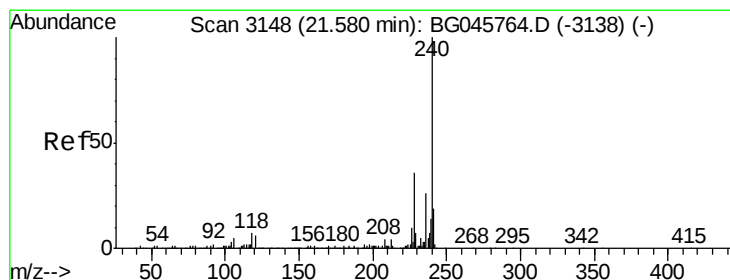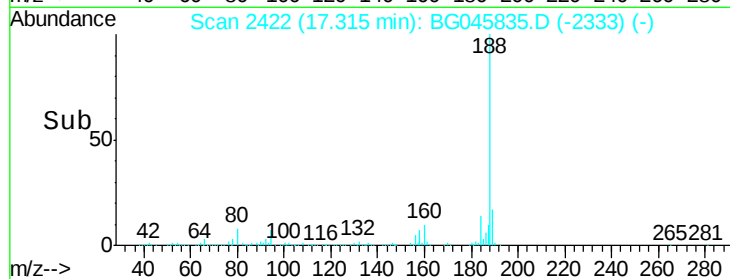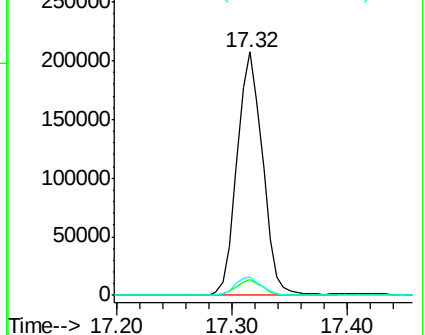

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.57 min Scan# 3147

Delta R.T. -0.01 min

Lab File: BG045835.D

Acq: 23 Jun 2020 11:36


Tgt Ion:240 Resp: 316802

Ion Ratio Lower Upper

240 100

120 6.3 5.0 7.4



236 24.6 20.6 30.8

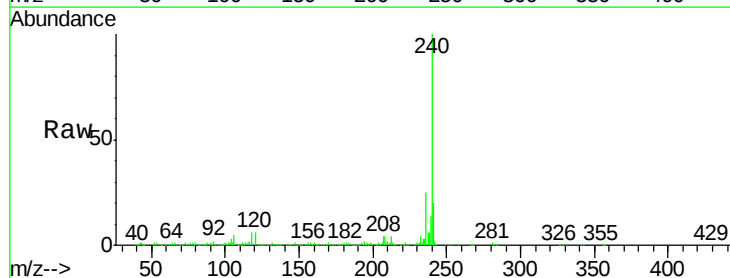


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

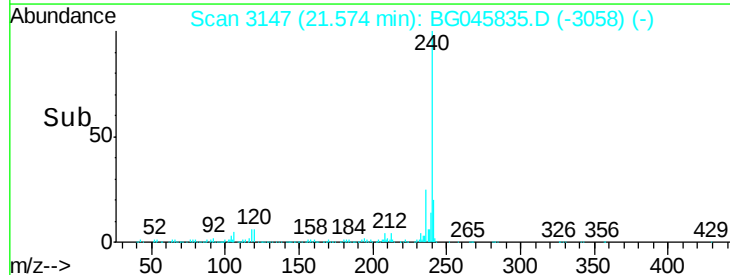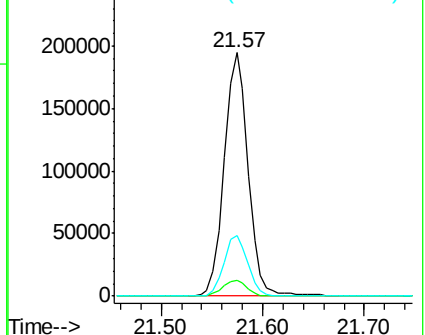



#79

Terphenyl-d14

Concen: 88.483 ng

RT: 19.94 min Scan# 2868

Delta R.T. -0.00 min

Lab File: BG045835.D

Acq: 23 Jun 2020 11:36

Instrument :

BNA_G

ClientSampleId :

SS043MW100-200615


Tot Ion:244 Resp: 1383188

Ion Ratio Lower Upper

244 100

212 8.8 7.2 10.8




122 8.1 6.4 9.6

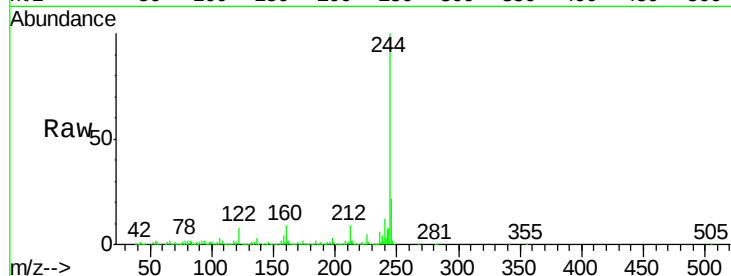

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

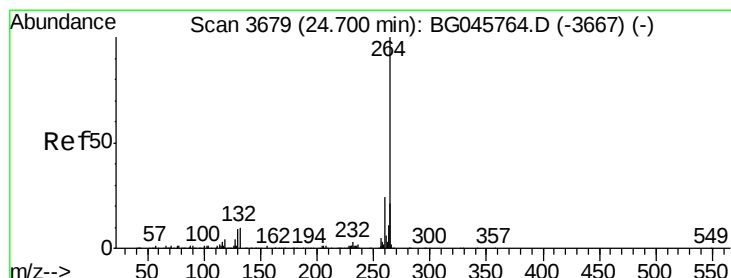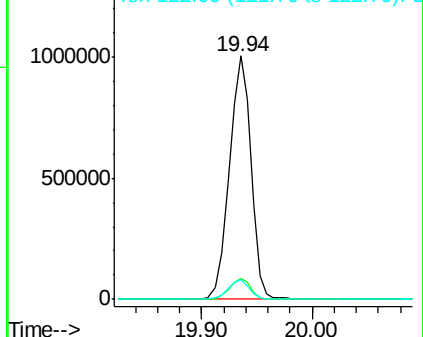

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.70 min Scan# 3679

Delta R.T. -0.00 min

Lab File: BG045835.D

Acq: 23 Jun 2020 11:36


Tgt Ion:264 Resp: 335828

Ion Ratio Lower Upper

264 100

260 22.3 19.0 28.4

265 22.0 17.4 26.0

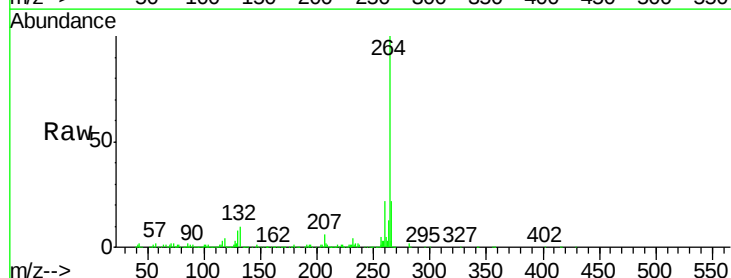

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

