
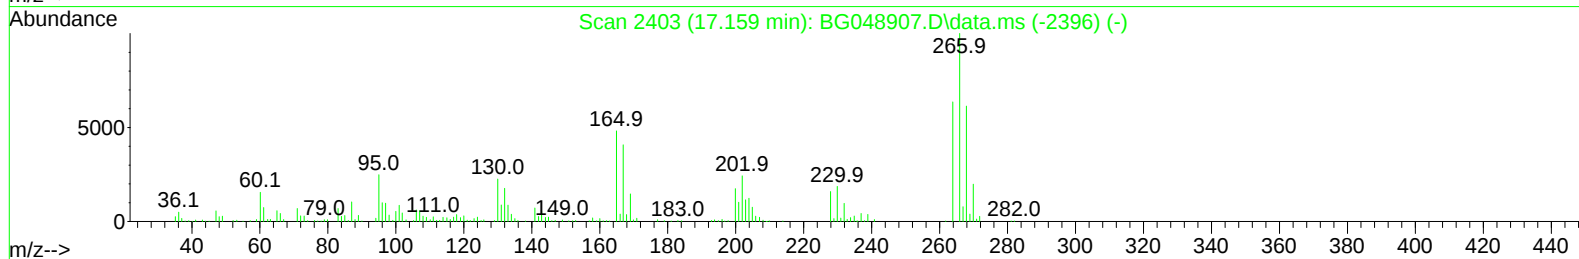
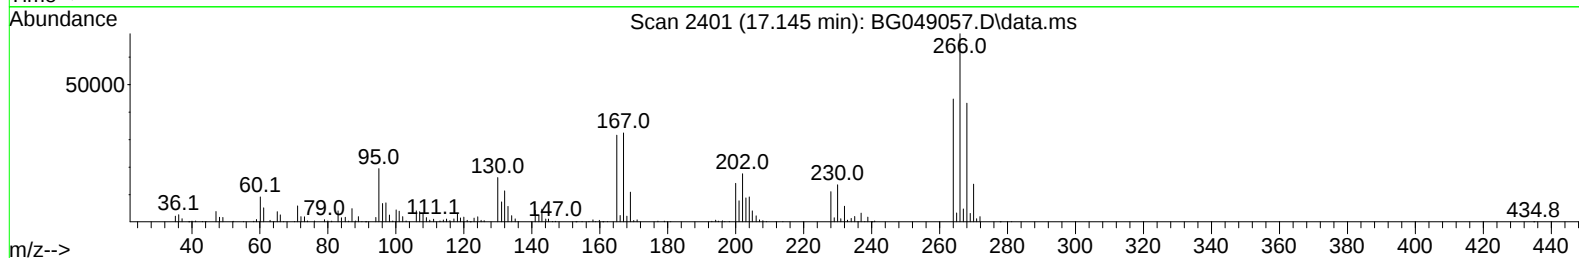


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062321\
Data File : BG049057.D
Acq On : 23 Jun 2021 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 19:09:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

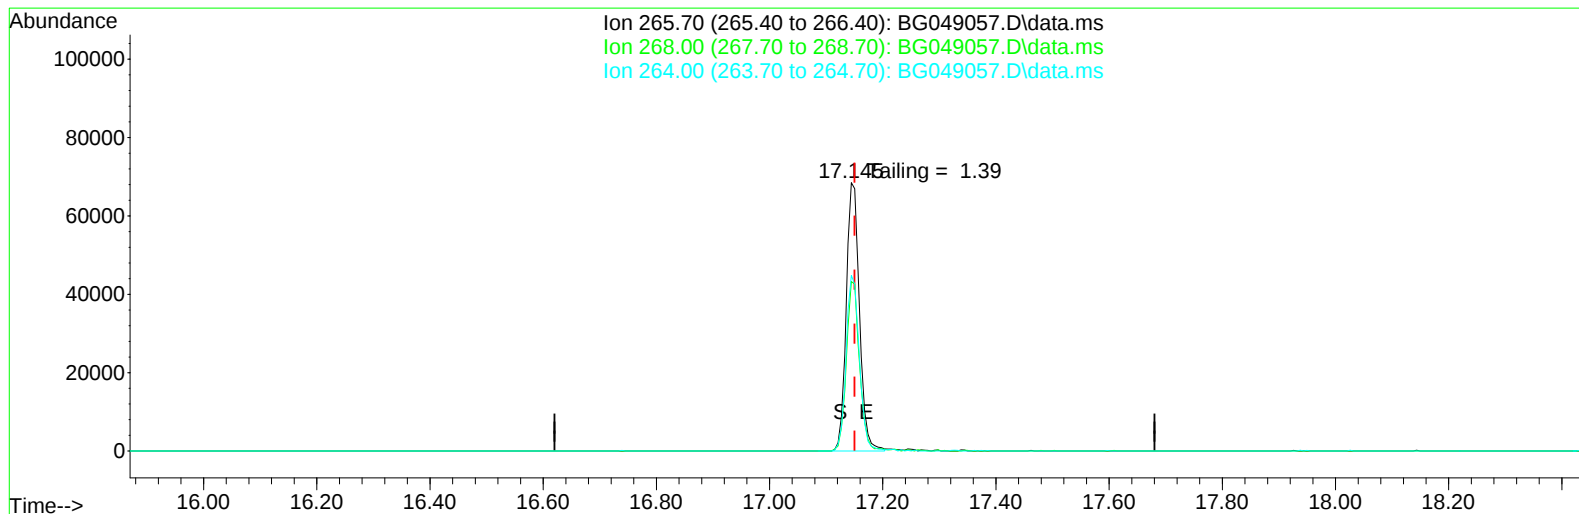

TIC: BG049057.D\data.ms

(70) Pentachlorophenol (C)




17.145min (-0.005) 211107.75 ng

response 111603

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.16
264.00	61.30	65.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062321\
 Data File : BG049057.D
 Acq On : 23 Jun 2021 11:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 19:09:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 16 12:04:50 2021
 Response via : Initial Calibration

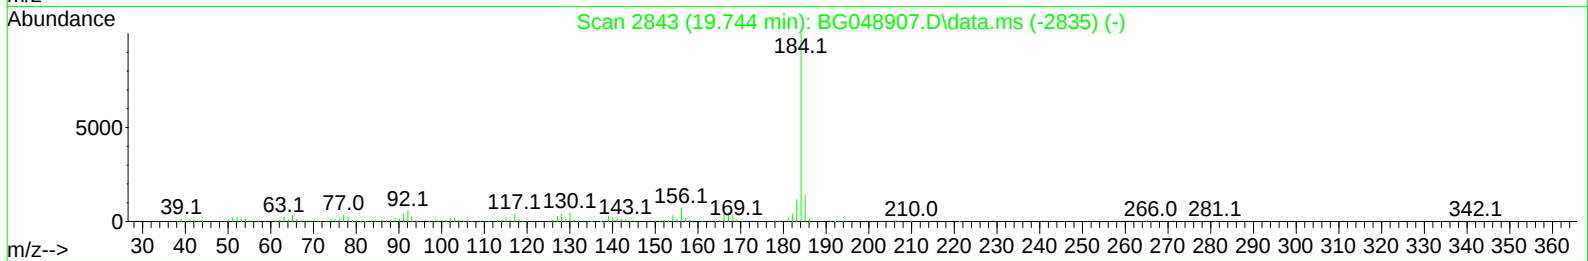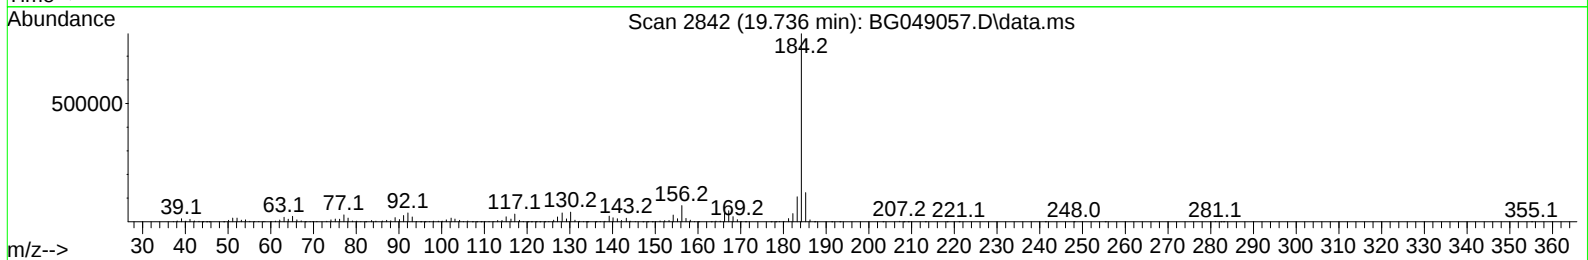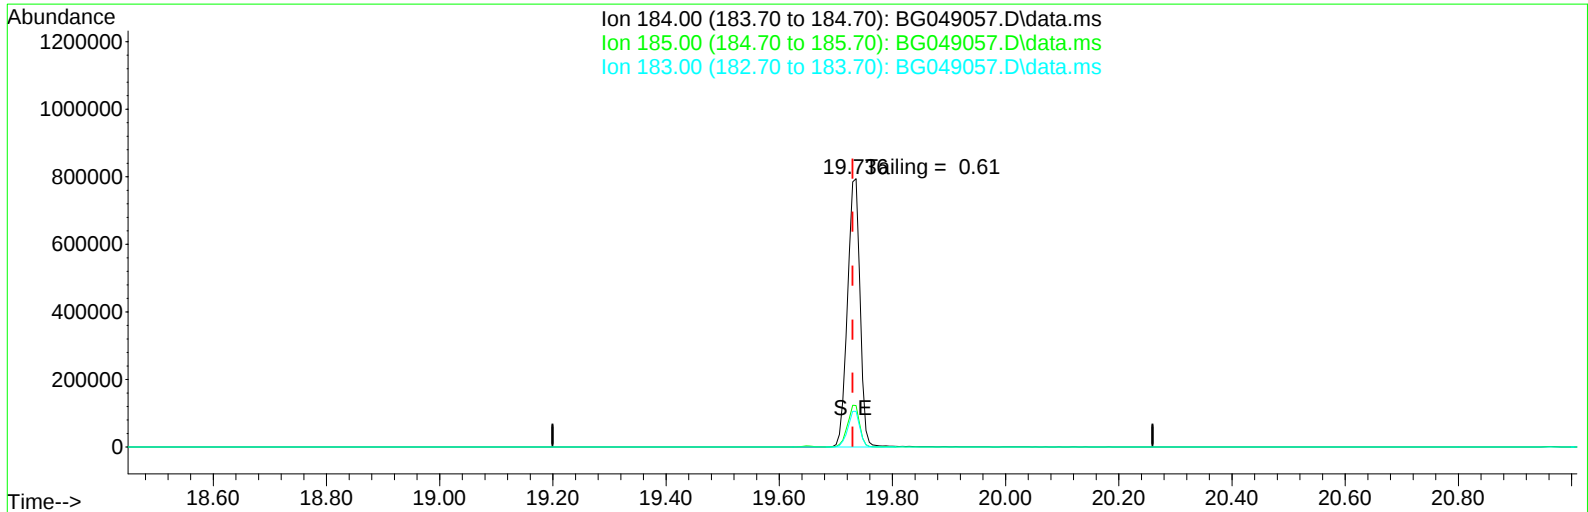

TIC: BG049057.D\data.ms

(77) Benzidine**19.736min (+ 0.006) 862065.47 ng****response 1233005**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.48
183.00	11.70	13.31
0.00	0.00	0.00