

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062321\
 Data File : BG049072.D
 Acq On : 23 Jun 2021 22:16
 Operator : CG/JU
 Sample : M2795-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B3-6-8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049072.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.156	16	20	29	rVV2	37174	69978	9.22%	1.323%
2	3.232	30	33	37	rVB4	7088	9397	1.24%	0.178%
3	5.189	362	366	372	rVB2	9076	13953	1.84%	0.264%
4	5.653	439	445	455	rBV	139278	241764	31.84%	4.569%
5	7.257	710	718	727	rBV	148865	277564	36.56%	5.246%
6	8.109	856	863	869	rBV	103211	181877	23.95%	3.437%
7	9.272	1053	1061	1068	rBV	93405	178026	23.45%	3.365%
8	10.694	1298	1303	1309	rBV5	5978	11127	1.47%	0.210%
9	10.929	1335	1343	1351	rBV	137353	250795	33.03%	4.740%
10	13.368	1752	1758	1766	rBV	254068	388523	51.17%	7.343%
11	14.748	1986	1993	2001	rBV	243781	387031	50.98%	7.315%
12	16.235	2238	2246	2258	rBV	246729	399355	52.60%	7.547%
13	17.498	2454	2461	2466	rBV	349604	559400	73.68%	10.572%
14	17.533	2466	2467	2473	rVB2	15424	18691	2.46%	0.353%
15	18.373	2606	2610	2613	rBV4	11113	14138	1.86%	0.267%
16	19.543	2804	2809	2813	rBV	31242	41943	5.52%	0.793%
17	19.643	2821	2826	2829	rBV7	6045	11217	1.48%	0.212%
18	19.866	2858	2864	2867	rBV6	10038	15177	2.00%	0.287%
19	19.901	2867	2870	2877	rVV	29307	45657	6.01%	0.863%
20	19.983	2879	2884	2887	rBV5	5364	8119	1.07%	0.153%
21	20.101	2898	2904	2912	rBV	581832	759248	100.00%	14.349%
22	20.771	3017	3018	3022	rVB4	8177	10368	1.37%	0.196%
23	21.411	3122	3127	3132	rBV8	15268	30424	4.01%	0.575%
24	21.781	3181	3190	3196	rBV2	365961	659058	86.80%	12.456%
25	22.604	3328	3330	3338	rVB8	5345	8722	1.15%	0.165%
26	23.332	3449	3454	3458	rVB7	6539	12393	1.63%	0.234%
27	24.043	3571	3575	3578	rBV4	7136	11159	1.47%	0.211%
28	24.161	3593	3595	3602	rVB7	8168	8983	1.18%	0.170%
29	25.101	3744	3755	3769	rBV2	219796	658549	86.74%	12.446%
30	27.022	4079	4082	4085	rBV4	6166	8633	1.14%	0.163%




Sum of corrected areas: 5291269

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062321\
Data File : BG049072.D
Acq On : 23 Jun 2021 22:16
Operator : CG/JU
Sample : M2795-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B3-6-8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

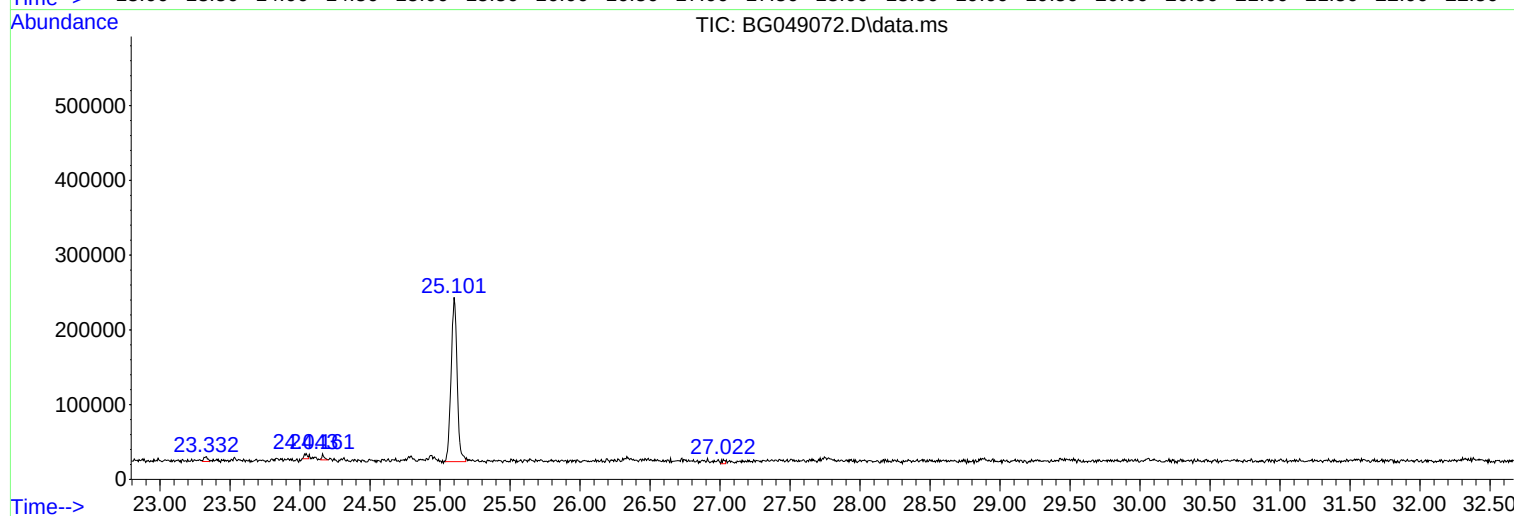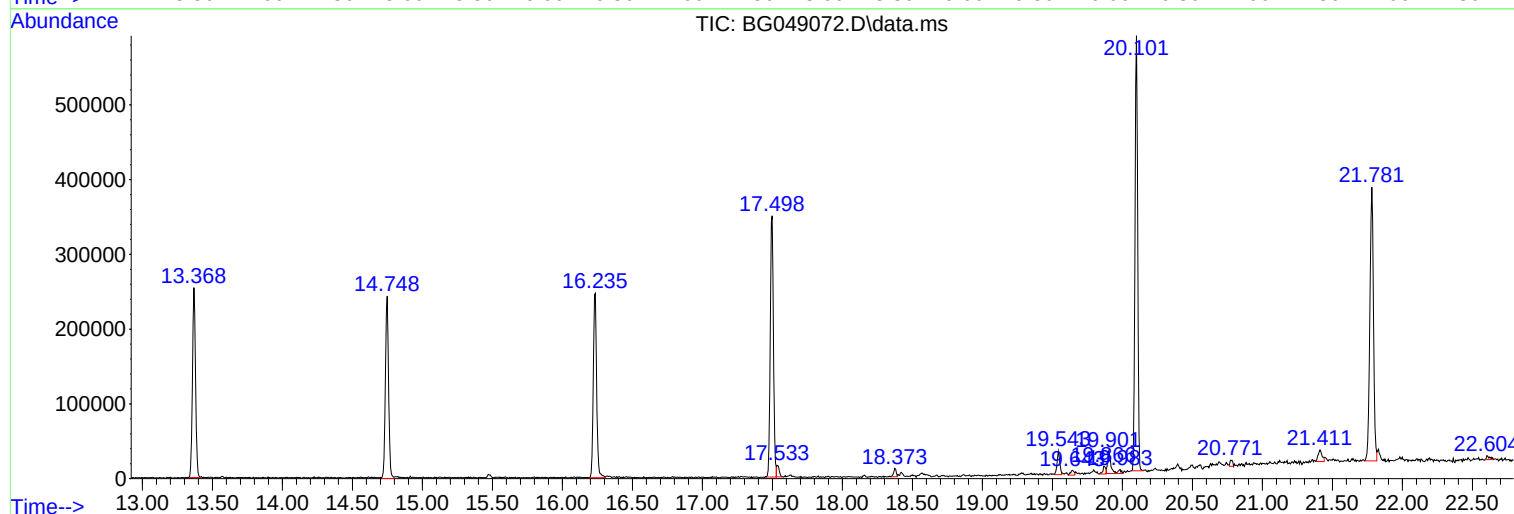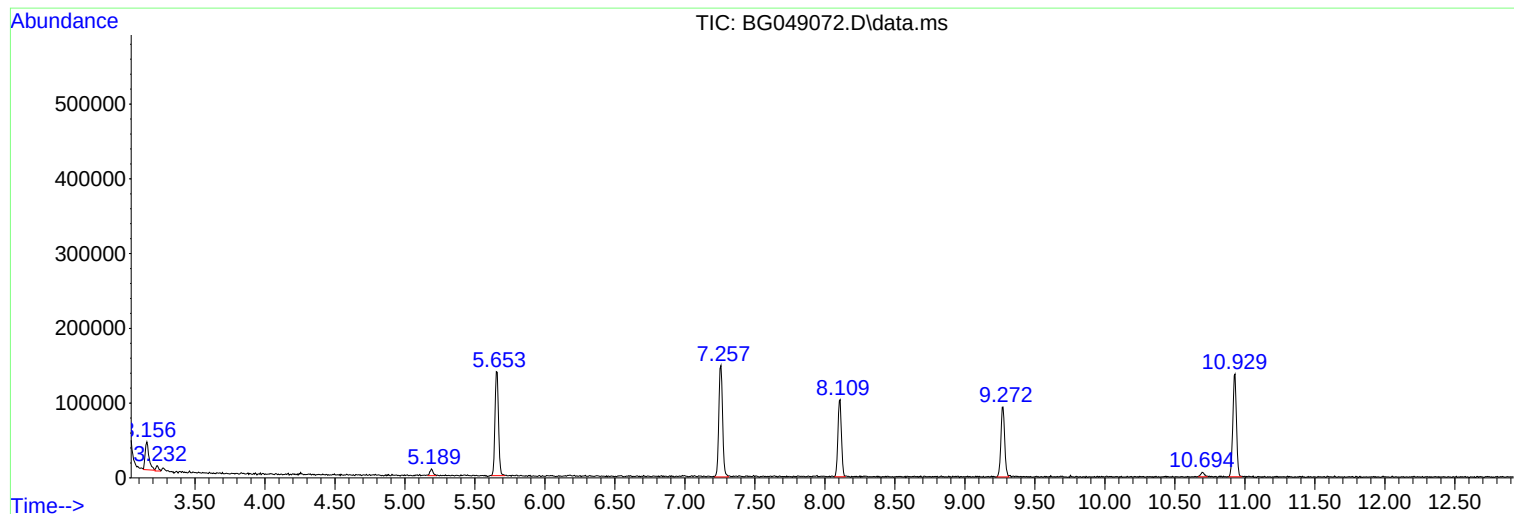

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062321\
Data File : BG049072.D
Acq On : 23 Jun 2021 22:16
Operator : CG/JU
Sample : M2795-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B3-6-8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062321\
Data File : BG049072.D
Acq On : 23 Jun 2021 22:16
Operator : CG/JU
Sample : M2795-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B3-6-8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------