
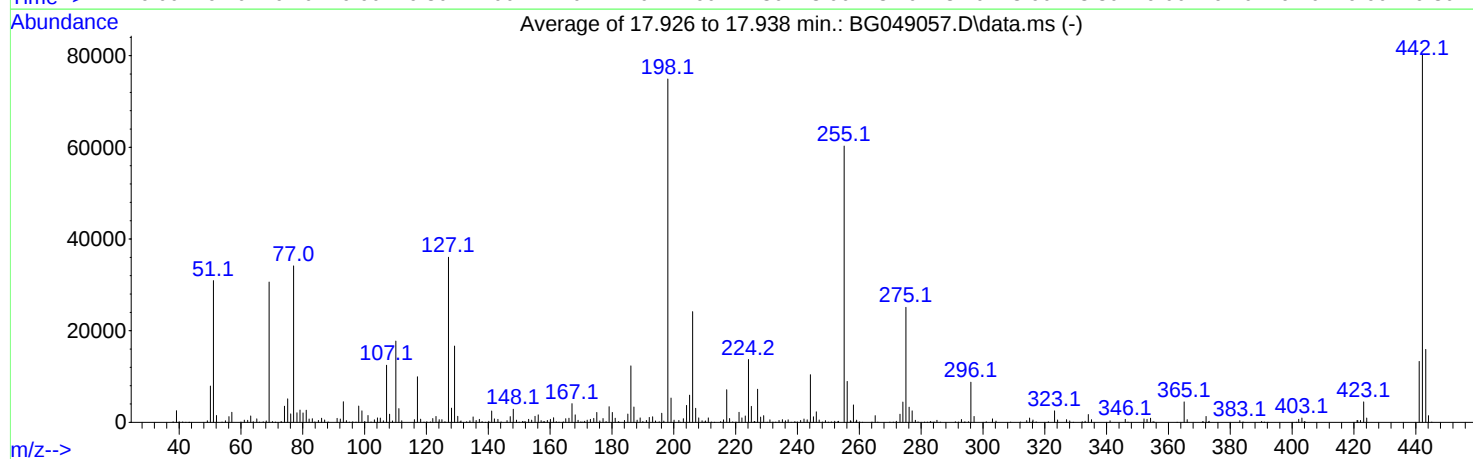


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062321\
 Data File : BG049057.D
 Acq On : 23 Jun 2021 11:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 24 11:02:36 2021

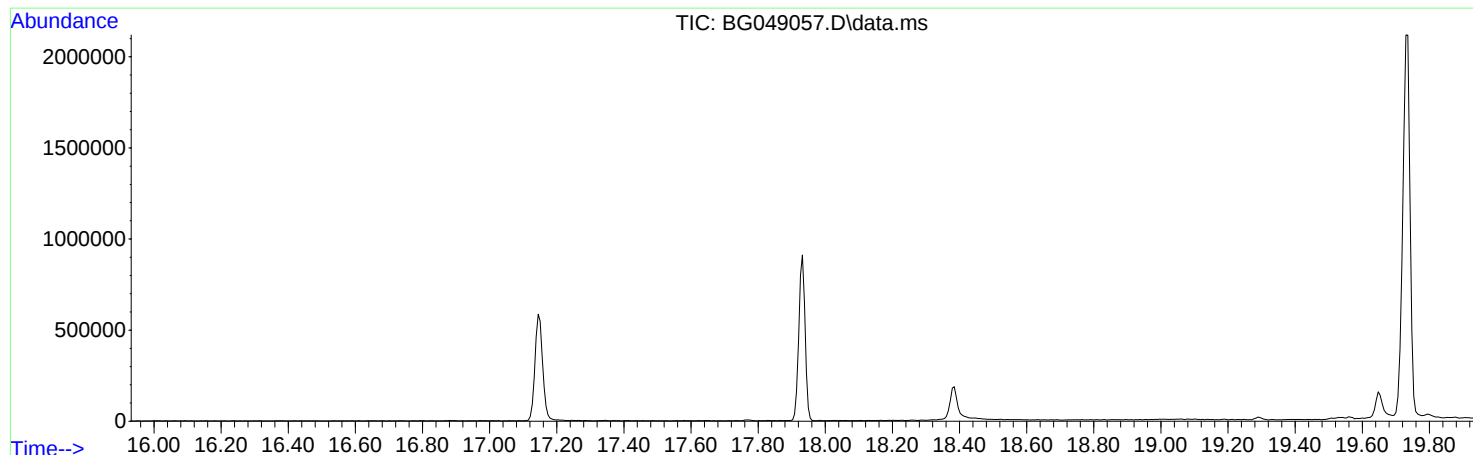




AutoFind: Scans 2534, 2535, 2536; Background Corrected with Scan 2527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	30917	PASS
68	69	0.00	2	1.0	320	PASS
69	198	0.00	100	40.9	30619	PASS
70	69	0.00	2	0.6	193	PASS
127	198	10	80	48.1	36013	PASS
197	198	0.00	2	0.4	274	PASS
198	198	100	100	100.0	74917	PASS
199	198	5	9	7.1	5320	PASS
275	198	10	60	33.5	25107	PASS
365	198	1	100	6.0	4481	PASS
441	198	0.01	100	17.8	13319	PASS
442	442	100	100	100.0	80259	PASS
443	442	15	24	19.8	15917	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062321\
Data File : BG049057.D
Acq On : 23 Jun 2021 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 23 19:09:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

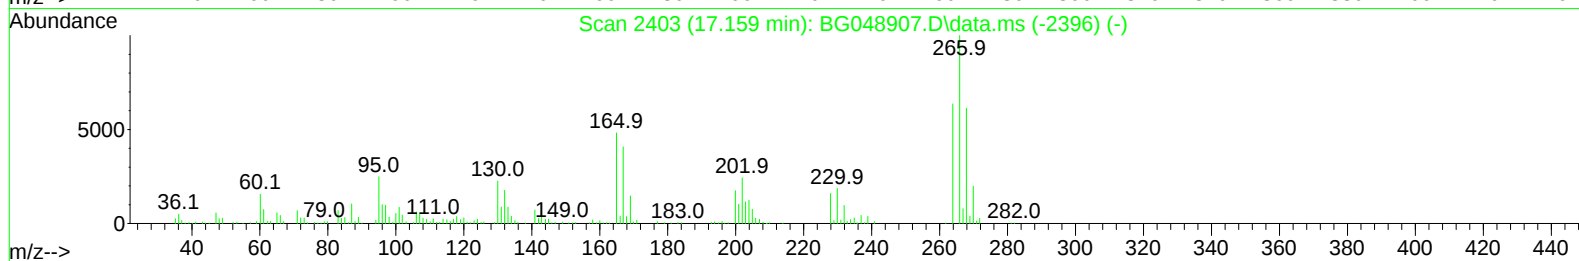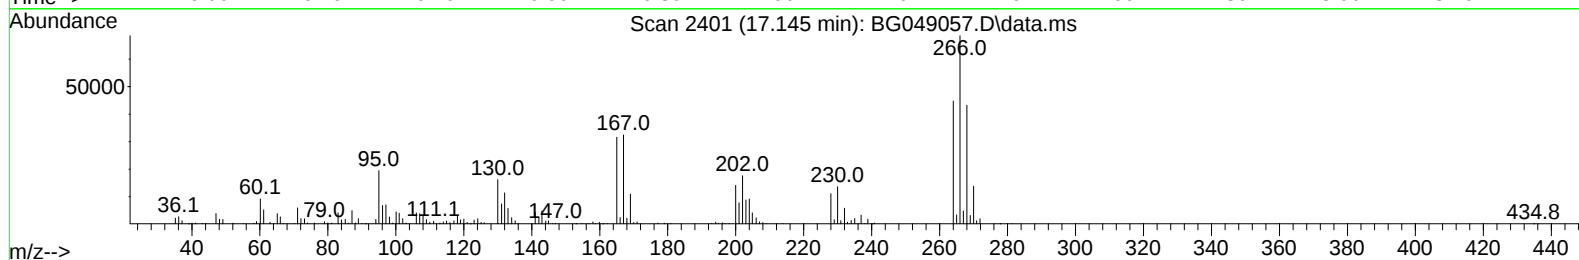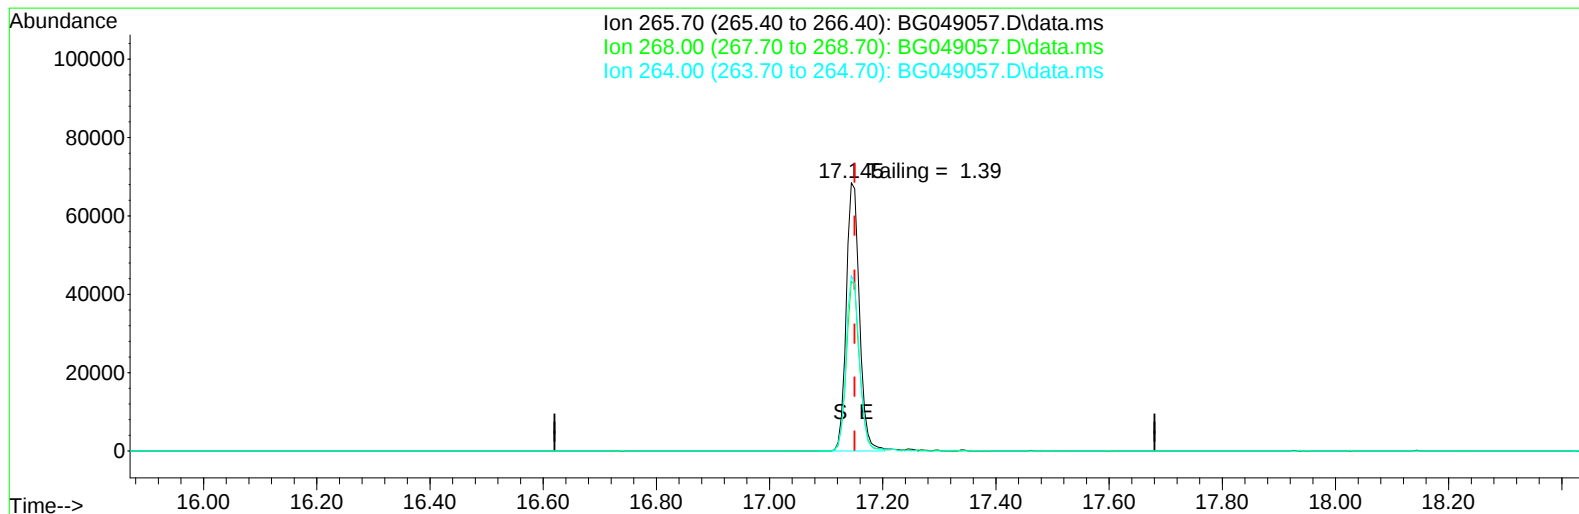

TIC: BG049057.D\data.ms

(70) Pentachlorophenol (C)

17.145min (-0.005) 211107.75 ng




response 111603

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.16
264.00	61.30	65.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062321\
Data File : BG049057.D
Acq On : 23 Jun 2021 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 23 19:09:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

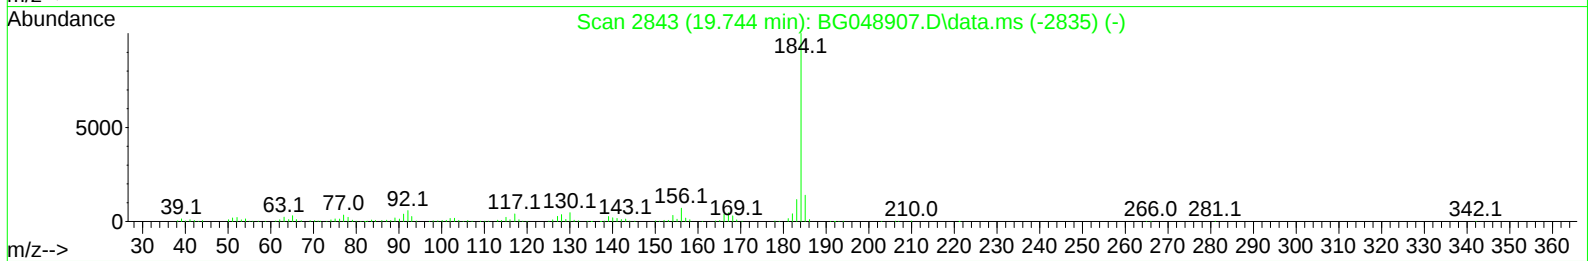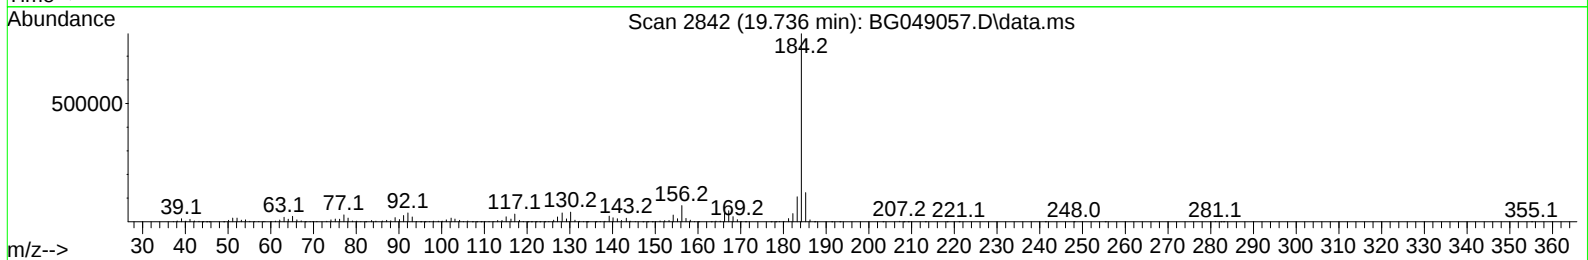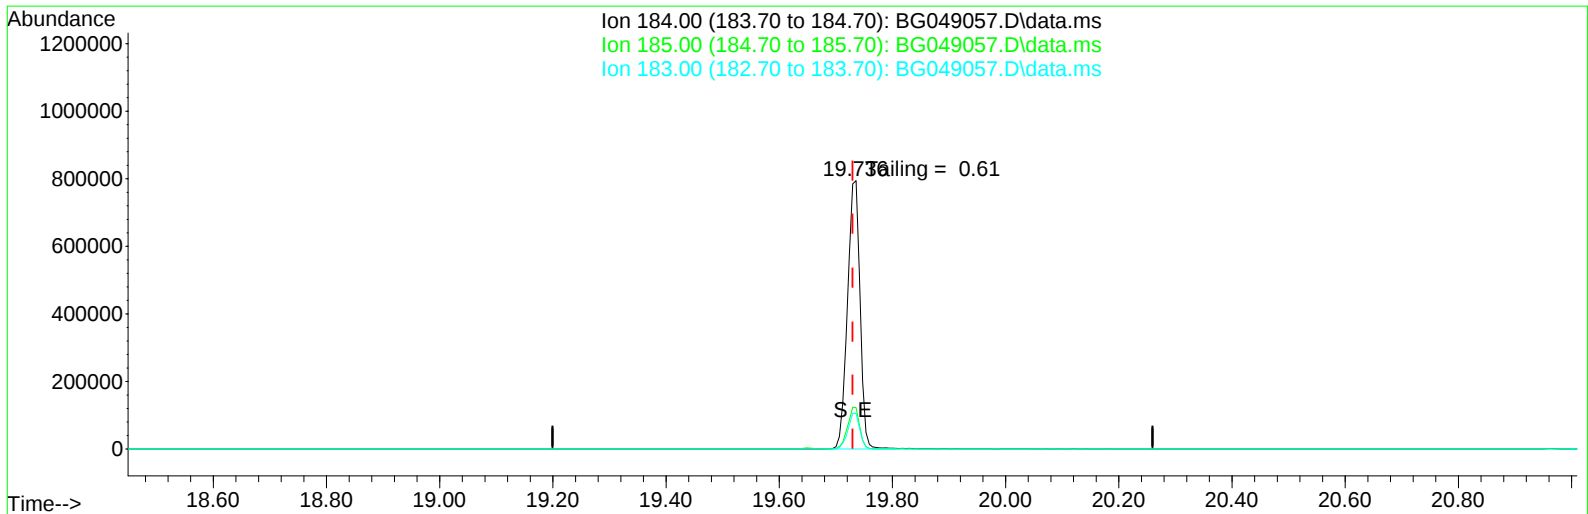

TIC: BG049057.D\data.ms

(77) Benzidine

19.736min (+ 0.006) 862065.47 ng

response 1233005

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.48
183.00	11.70	13.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/23/2021	BNA_G	BG049057.D
Compound Name	Response	Retention Time
DDT	294051	20.96
DDD	3659	20.51
DDE	539	20.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4198	298249	1.41