
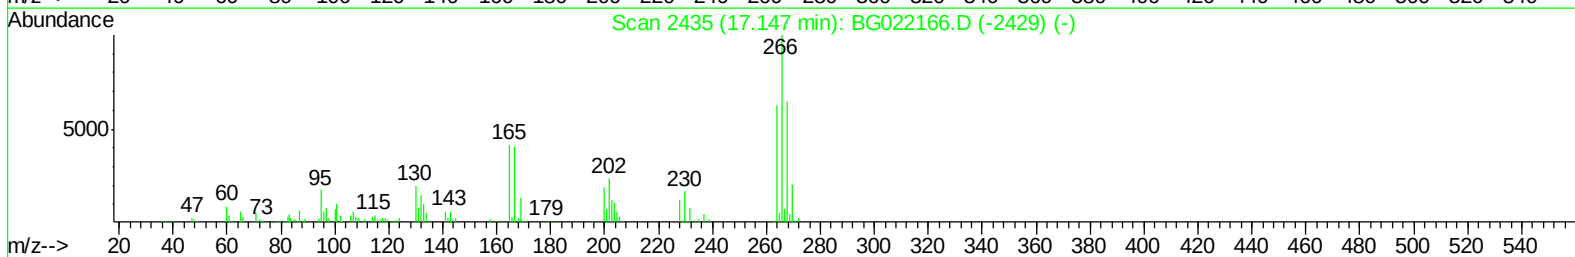
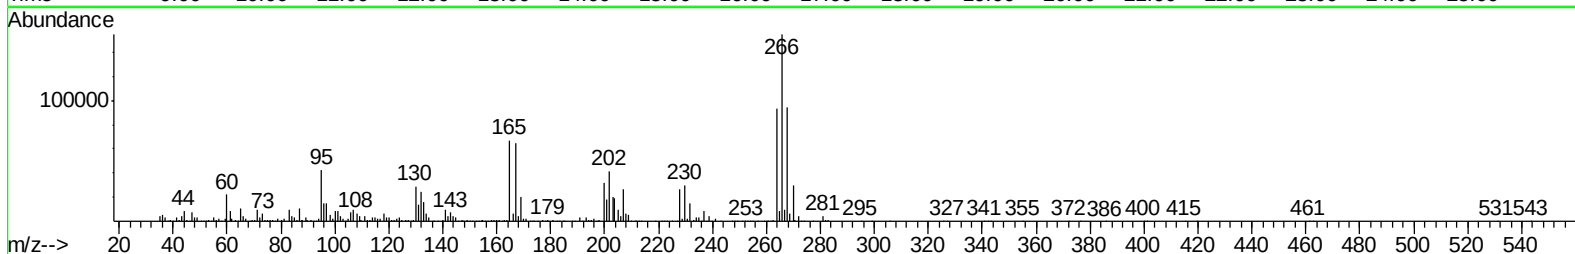


Data Path : Z:\HPCHEM1\BNA G\Data\BG062416\
Data File : BG022514.D
Acq On : 23 Jun 2016 21:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 08:08:15 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 04:19:57 2016
Response via : Initial Calibration

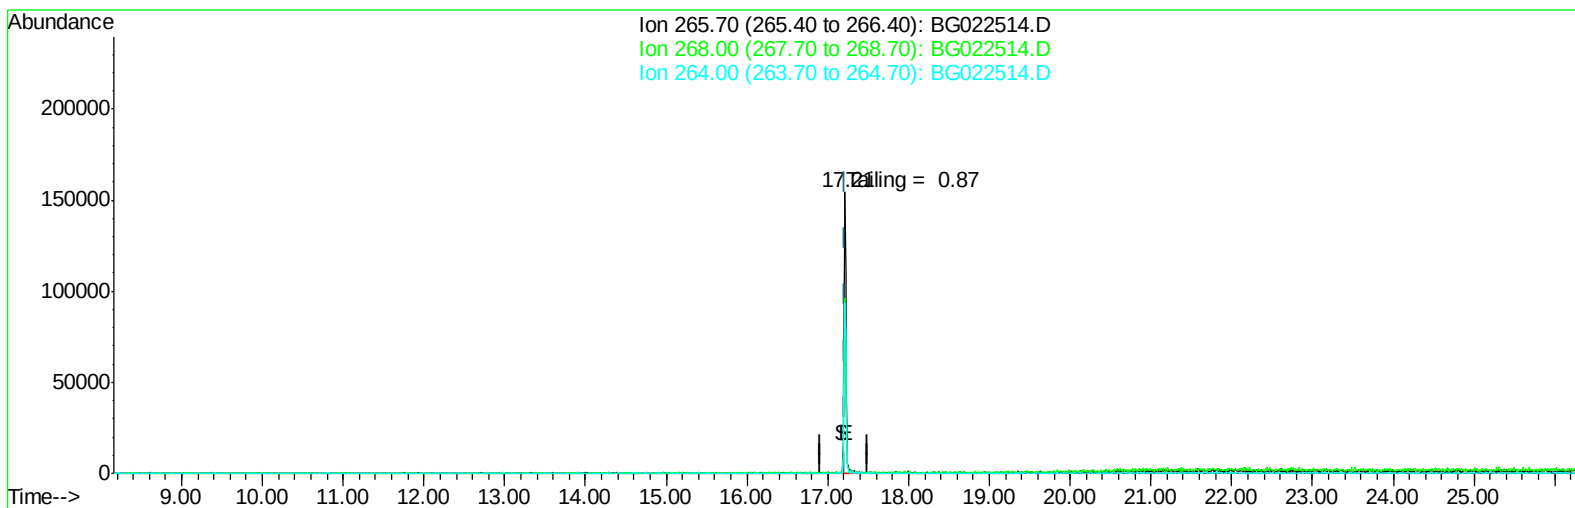

TIC: BG022514.D

(69) Pentachlorophenol (C)

17.214min (+0.004) 213583.04ng

response 241037

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	61.29
264.00	63.20	60.58
0.00	0.00	0.00