
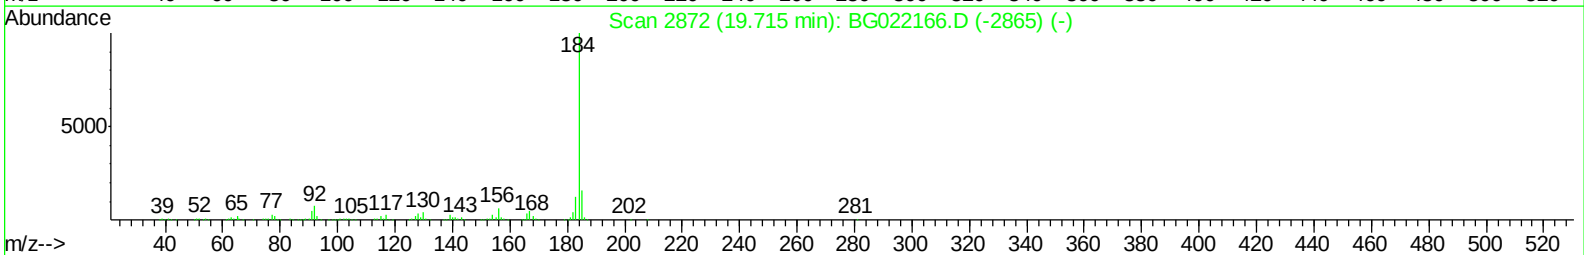
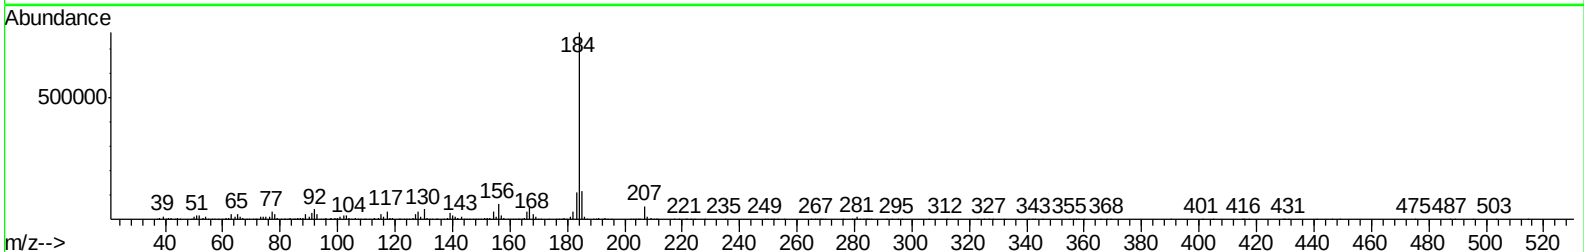


```
Data Path : Z:\HPCHEM1\BNA G\Data\BG062416\  
Data File : BG022523.D  
Acq On    : 24 Jun 2016    3:34  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jun 24 08:09:31 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 04:19:57 2016
Response via : Initial Calibration

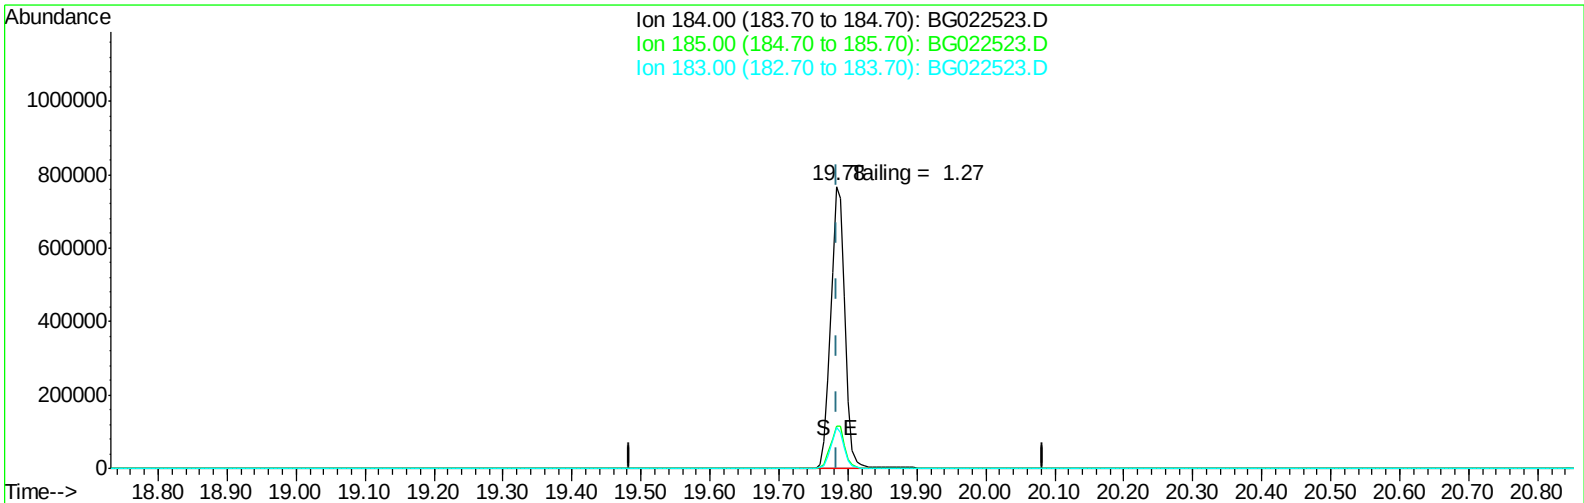

TIC: BG022523.D

(76) Benzidine




19.783min (-0.000) 10605.33ng

response 1099029

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.16
183.00	13.40	14.36
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG062416\
Data File : BG022523.D
Acq On : 24 Jun 2016 3:34
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 08:09:31 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 04:19:57 2016
Response via : Initial Calibration

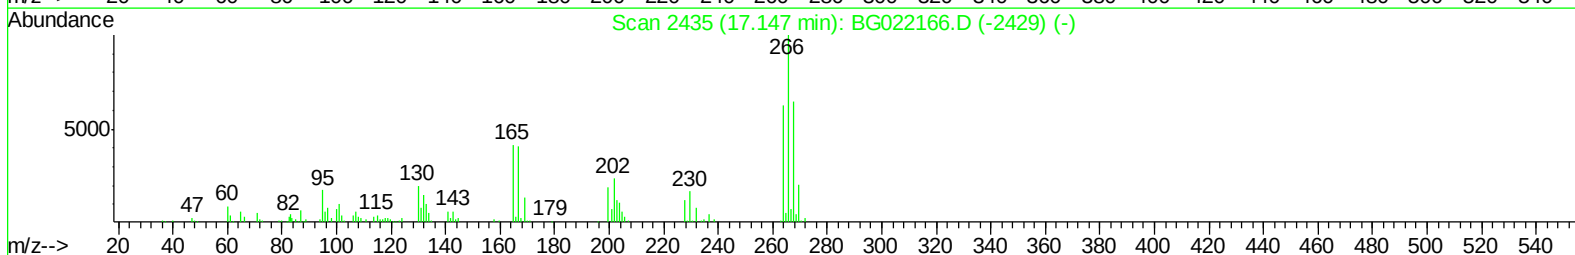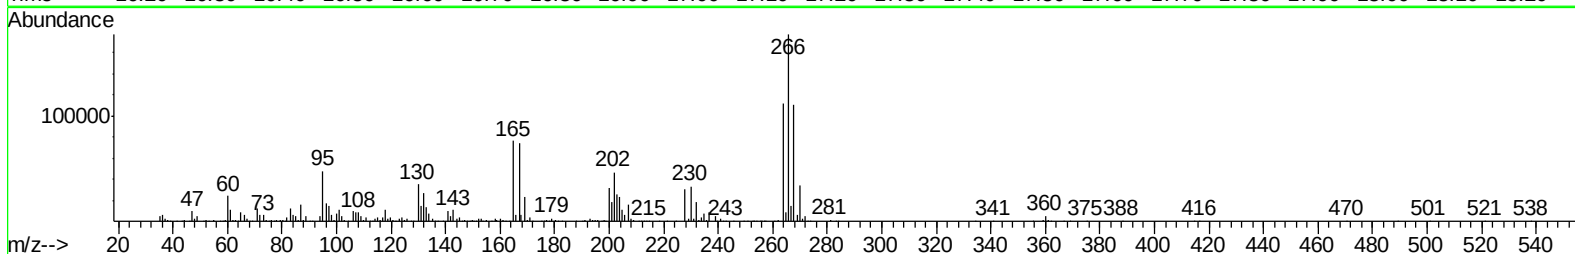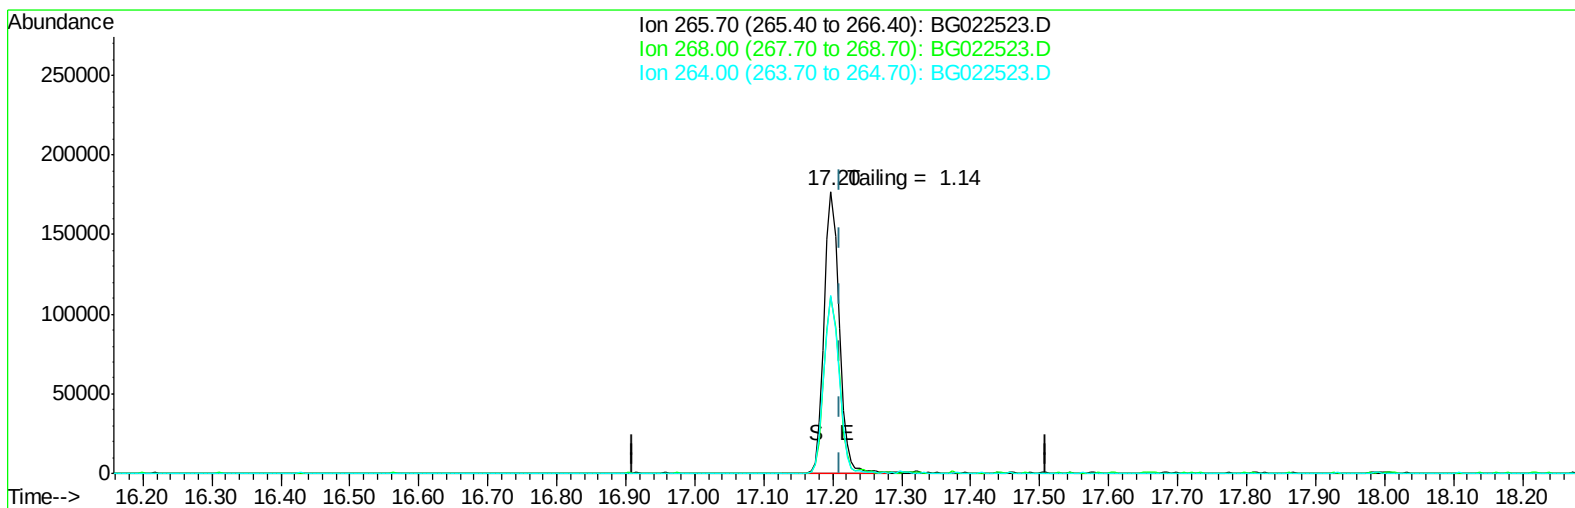

TIC: BG022523.D

(69) Pentachlorophenol (C)

17.198min (-0.012) 79468.95ng

response 268351

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	62.64
264.00	63.20	63.28
0.00	0.00	0.00