


Data Path : Z:\HPCHEM1\BNA G\DATA\BG062416\
 Data File : BG022523.D
 Acq On : 24 Jun 2016 3:34
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 24 04:19:57 2016

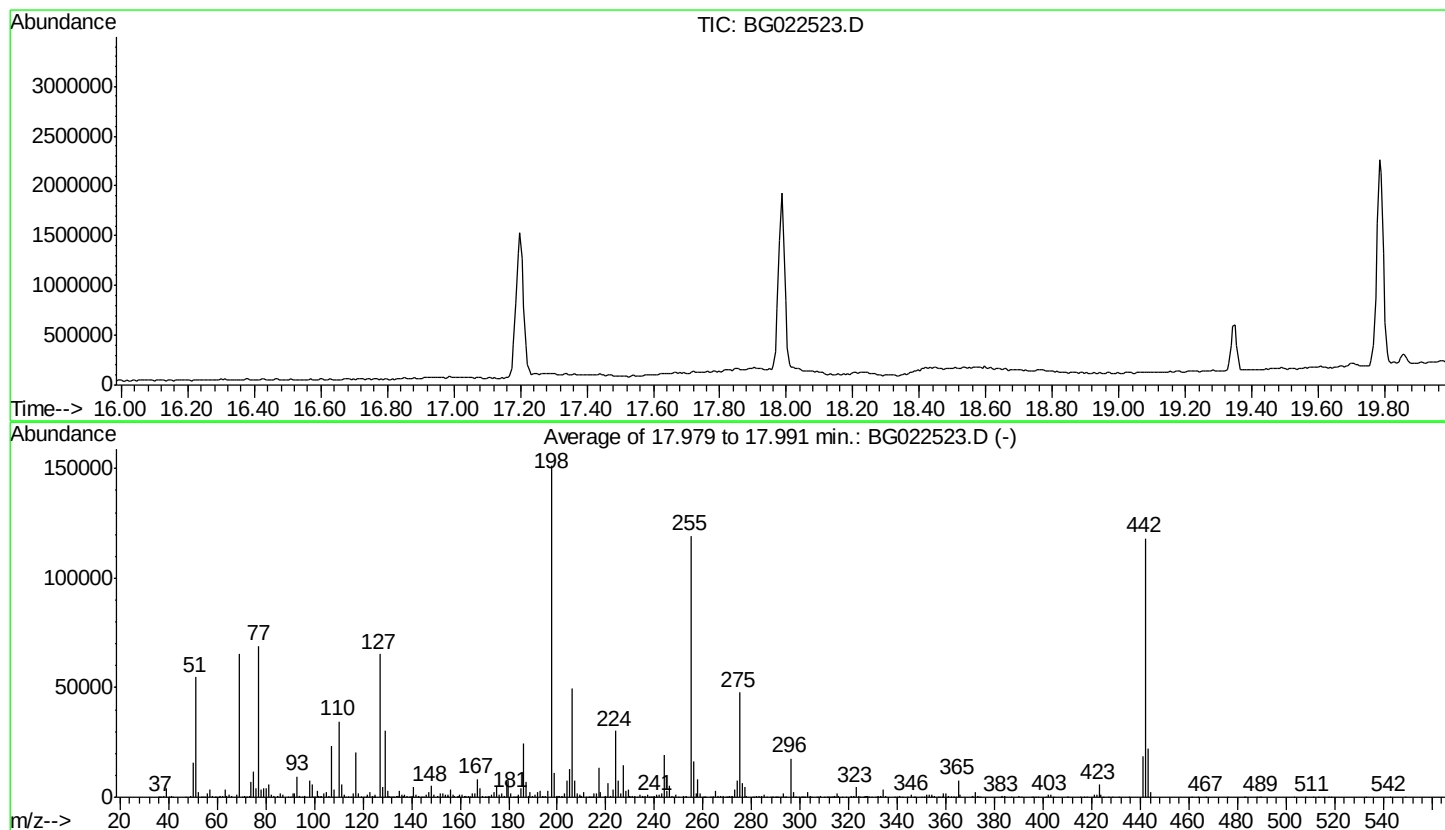

AutoFind: Scans 2577, 2578, 2579; Background Corrected with Scan 2570

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	54687	PASS
68	69	0.00	2	1.5	1012	PASS
69	198	0.00	100	43.2	65351	PASS
70	69	0.00	2	0.2	134	PASS
127	198	10	80	43.1	65202	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	151360	PASS
199	198	5	9	7.4	11165	PASS
275	198	10	60	31.6	47770	PASS
365	198	1	100	5.1	7743	PASS
441	442	0.01	24	15.7	18569	PASS
442	198	50	100	78.1	118152	PASS
443	442	15	24	18.6	22023	PASS