
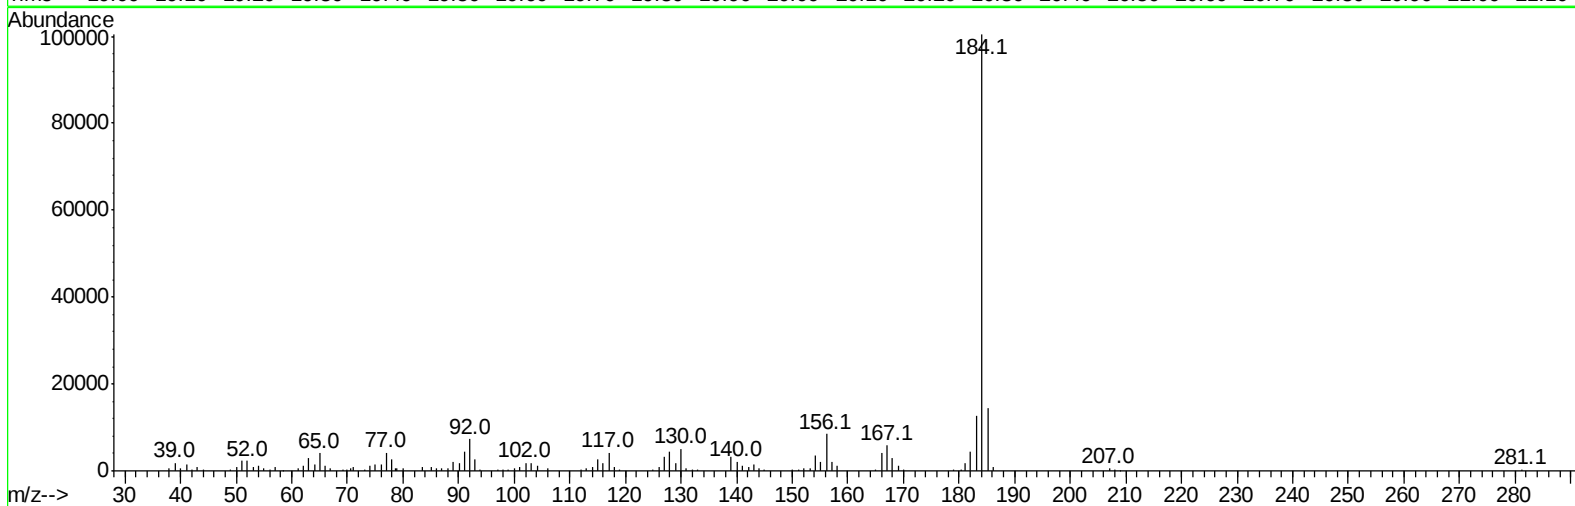


Data Path : Z:\HPCHEM1\BNA G\Data\BG062417\  
Data File : BG027650.D  
Acq On : 24 Jun 2017 8:48  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 09:15:36 2017  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jun 21 18:52:15 2017  
Response via : Initial Calibration

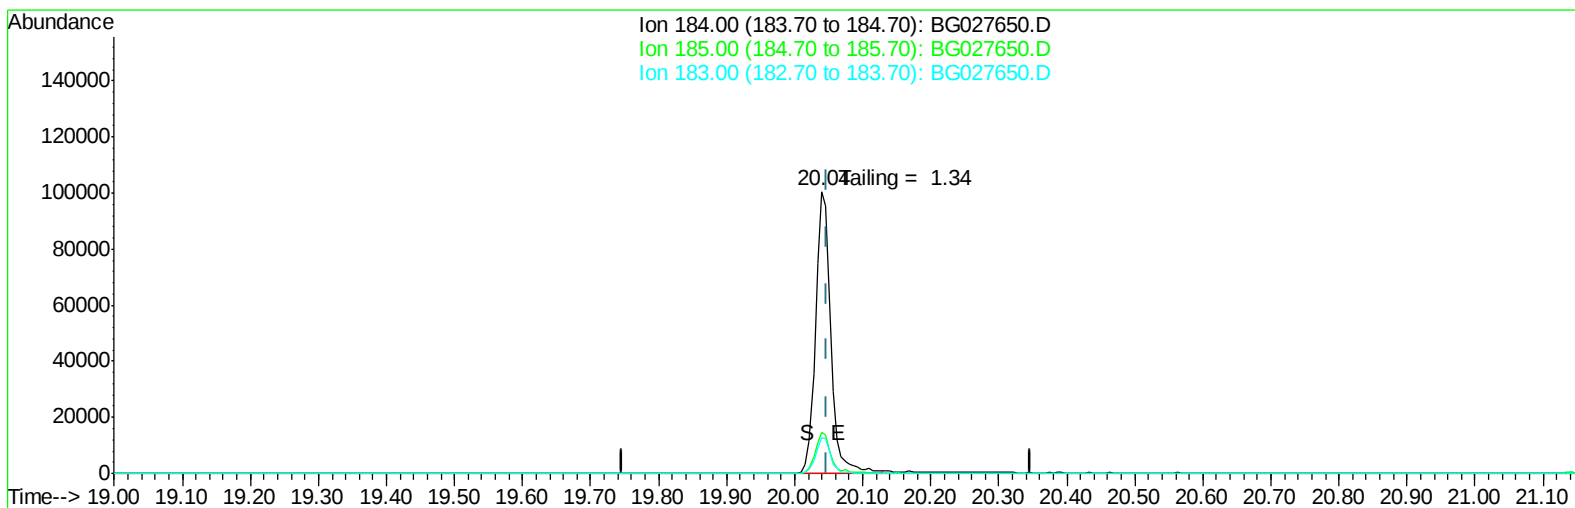

TIC: BG027650.D

(76) Benzidine



20.039min (-0.008) 0.00ng

response 160568

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.30 | 14.47 |
| 183.00 | 13.80 | 12.61 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA G\Data\BG062417\  
Data File : BG027650.D  
Acq On : 24 Jun 2017 8:48  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 09:15:36 2017  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jun 21 18:52:15 2017  
Response via : Initial Calibration

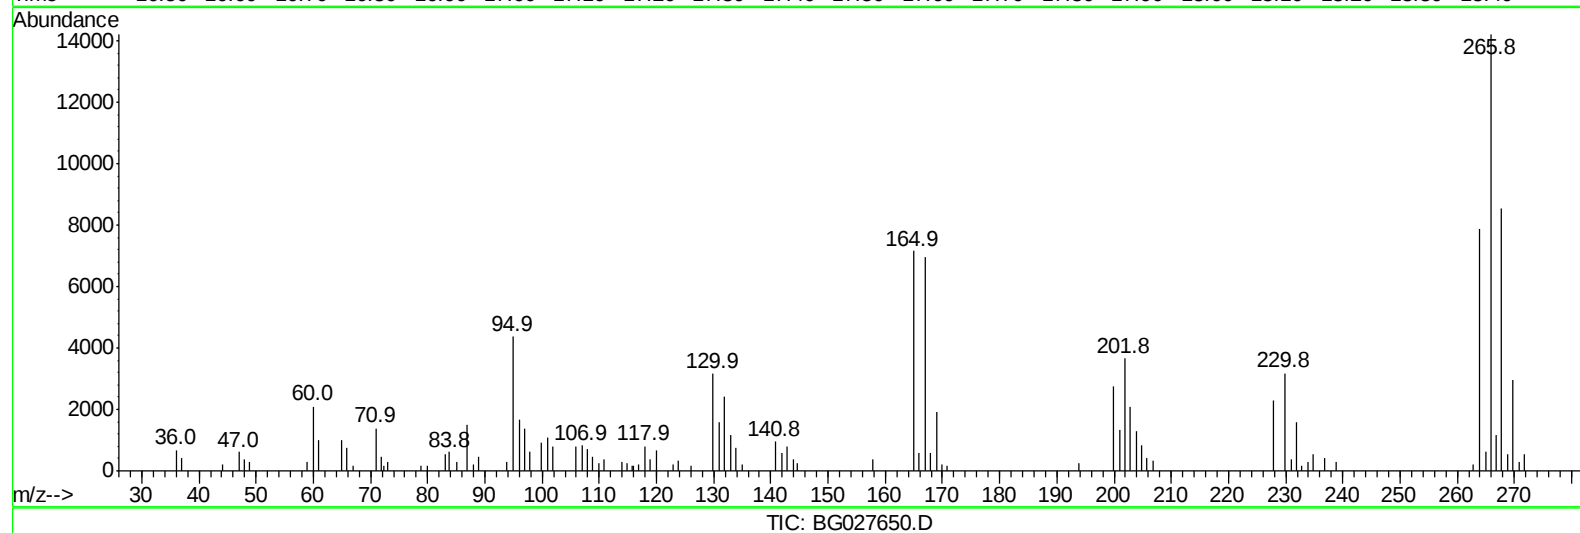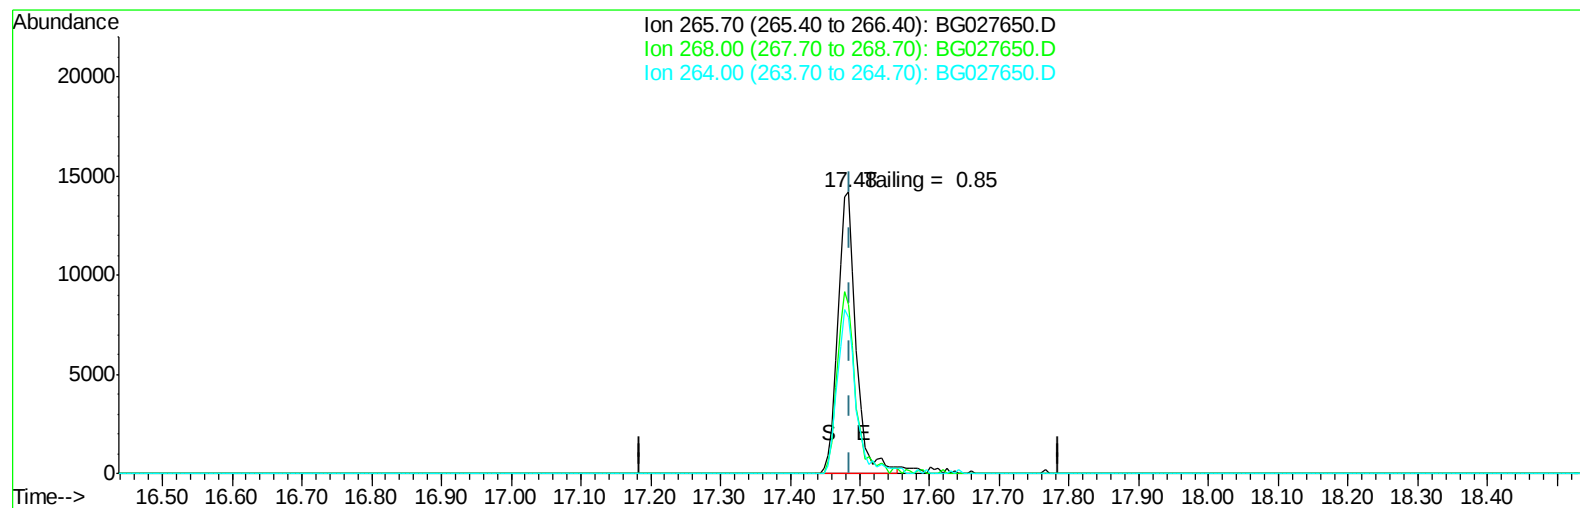

(69) Pentachlorophenol (C)

17.483min (-0.002) 0.00ng

response 24691

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 60.70 | 60.14 |
| 264.00 | 62.60 | 55.42 |
| 0.00   | 0.00  | 0.00  |