

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG062417\
 Data File : BG027662.D
 Acq On : 24 Jun 2017 16:49
 Operator : SJ/JU
 Sample : PB100066BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB100066BL

Quant Time: Jun 26 04:19:22 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 21 18:52:15 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.51	152	18044	20.00	ng	0.00
21) Naphthalene-d8	11.32	136	82132	20.00	ng	0.00
38) Acenaphthene-d10	15.09	164	54333	20.00	ng	0.00
63) Phenanthrene-d10	17.84	188	153717	20.00	ng	0.00
75) Chrysene-d12	22.20	240	171968	20.00	ng	-0.01
86) Perylene-d12	25.85	264	160164	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.09	112	183541	144.77	ng	0.00
7) Phenol-d6	7.65	99	258420	137.68	ng	0.00
23) Nitrobenzene-d5	9.67	82	158495	91.31	ng	0.00
41) 2,4,6-Tribromophenol	16.57	330	115861	143.04	ng	0.00
44) 2-Fluorobiphenyl	13.71	172	373182	93.82	ng	0.00
78) Terphenyl-d14	20.42	244	762264	104.44	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG062417\
Data File : BG027662.D
Acq On : 24 Jun 2017 16:49
Operator : SJ/JU
Sample : PB100066BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB100066BL

Quant Time: Jun 26 04:19:22 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 18:52:15 2017
Response via : Initial Calibration

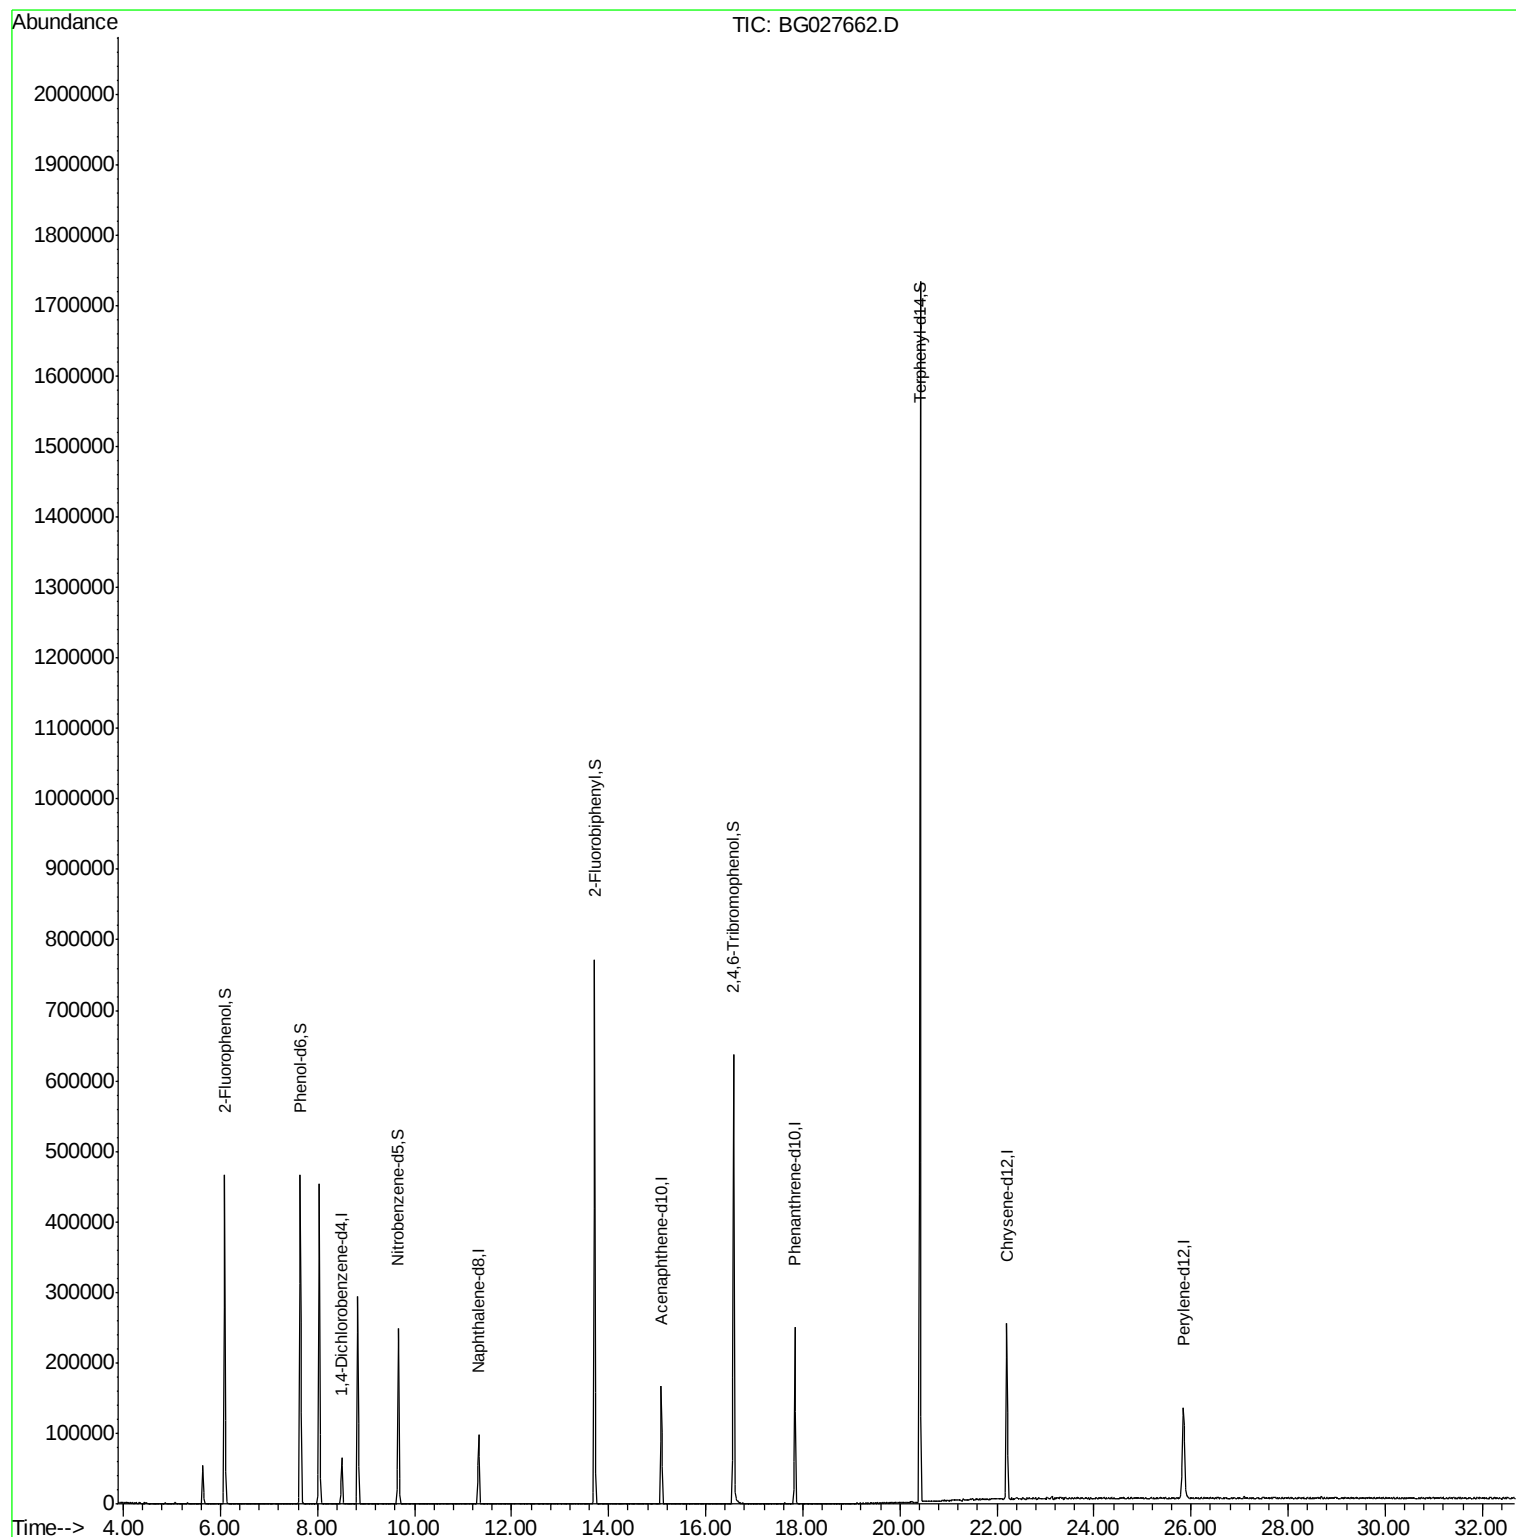

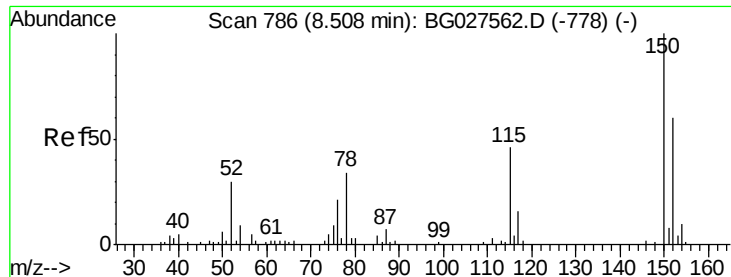


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.51 min Scan# 786
Delta R.T. -0.00 min
Lab File: BG027662.D
Acq: 24 Jun 2017 16:49

Instrument :
BNA_G
ClientSampleId :
PB100066BL

Tgt Ion:152 Resp: 18044
Ion Ratio Lower Upper
152 100
150 156.2 114.0 171.0
115 69.0 48.1 72.1

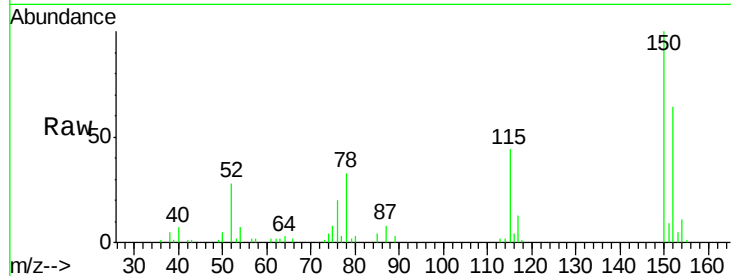


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

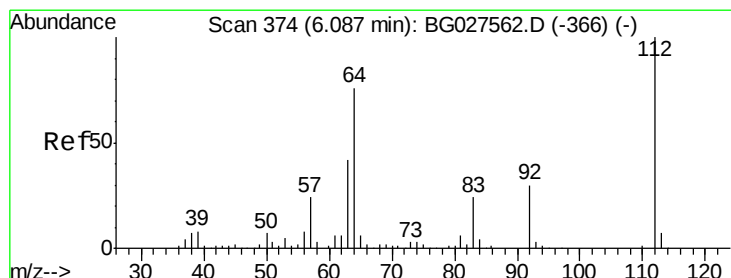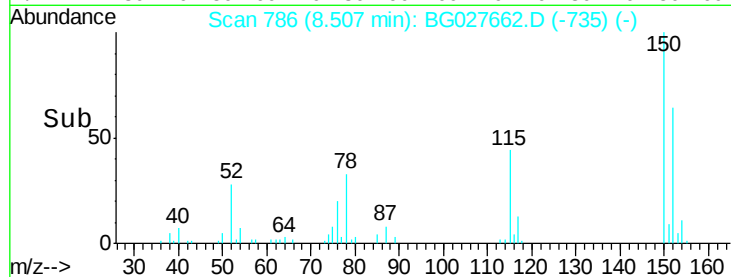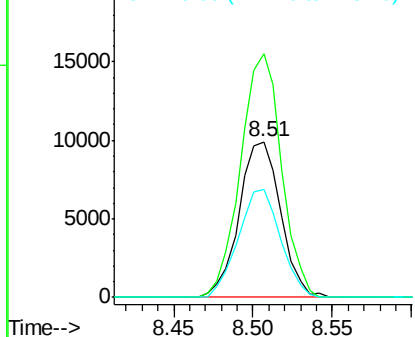



#5


2-Fluorophenol
Concen: 144.768 ng
RT: 6.09 min Scan# 375
Delta R.T. 0.00 min
Lab File: BG027662.D
Acq: 24 Jun 2017 16:49

Tgt Ion:112 Resp: 183541
Ion Ratio Lower Upper
112 100
64 71.1 61.8 92.6
63 41.1 37.2 55.8

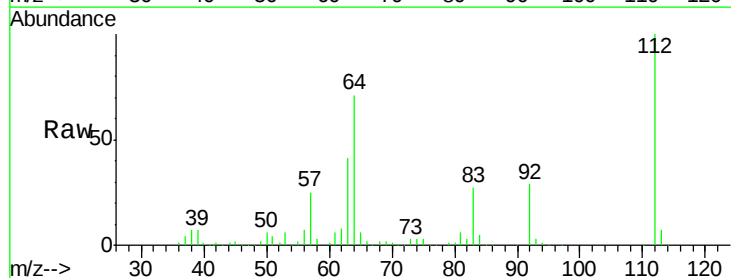

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

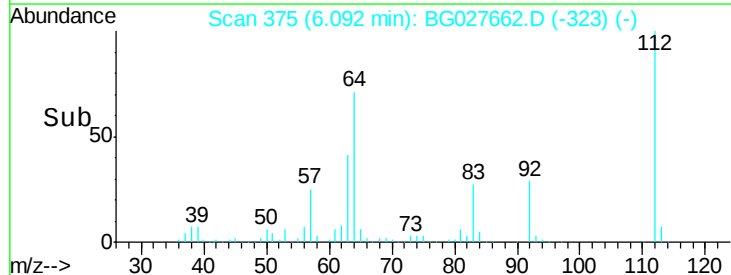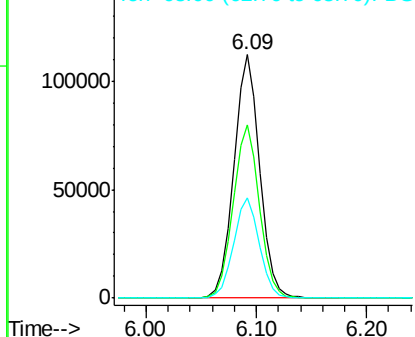

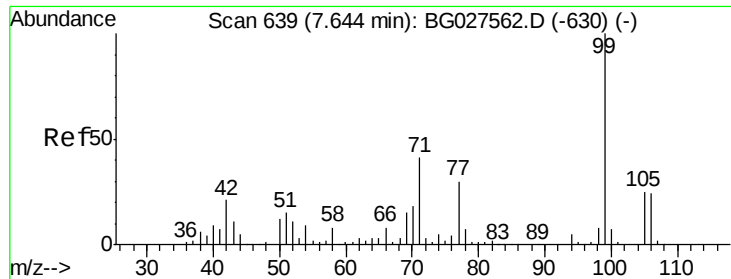

#7

Phenol-d6

Concen: 137.685 ng

RT: 7.65 min Scan# 640

Delta R.T. 0.00 min

Lab File: BG027662.D

Acq: 24 Jun 2017 16:49

Instrument :

BNA_G

ClientSampleId :

PB100066BL


Tgt Ion: 99 Resp: 258420

Ion Ratio Lower Upper

99 100

42 21.0 20.5 30.7

71 46.0 37.6 56.4



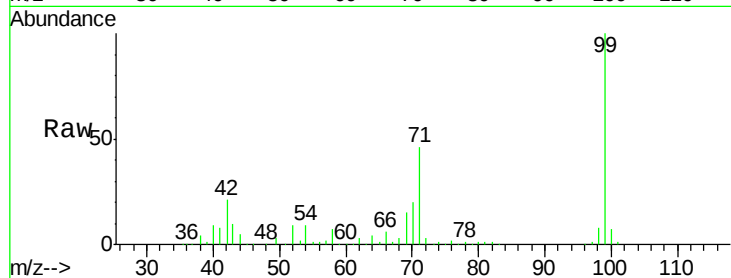


Abundance

Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

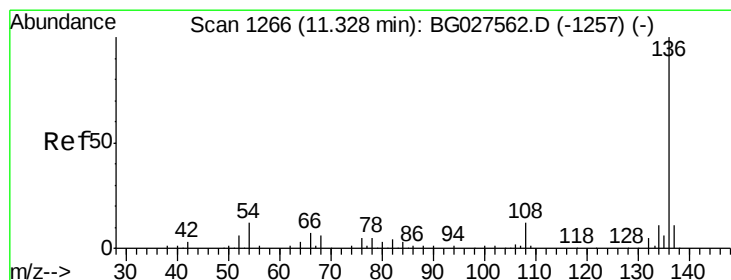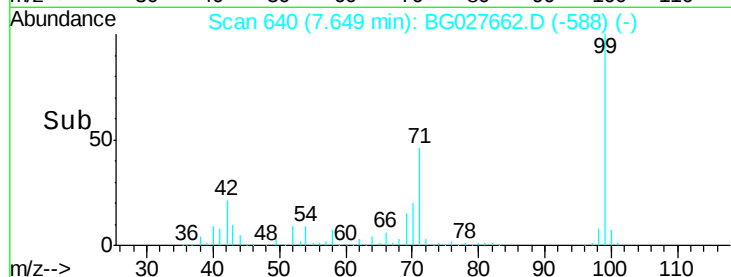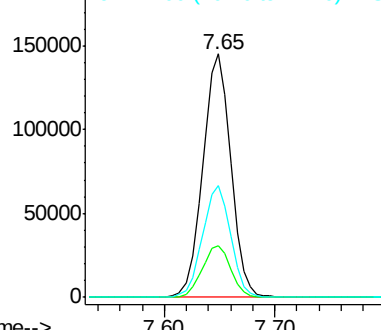

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.32 min Scan# 1265

Delta R.T. -0.01 min

Lab File: BG027662.D

Acq: 24 Jun 2017 16:49

Tgt Ion: 136 Resp: 82132


Ion Ratio Lower Upper

136 100

137 10.6 8.9 13.3

54 10.0 9.3 13.9

68 6.1 5.1 7.7

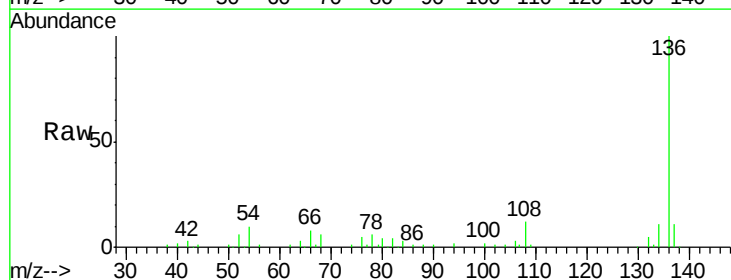



Abundance


Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC

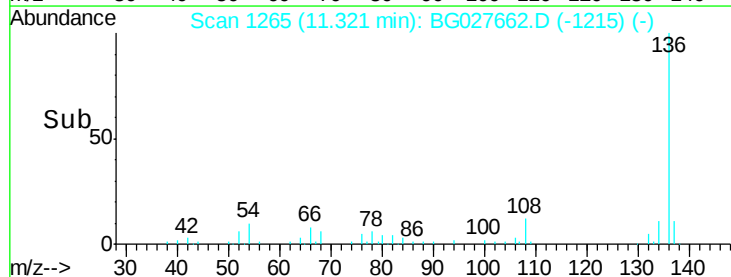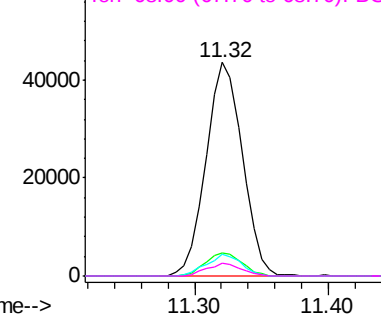


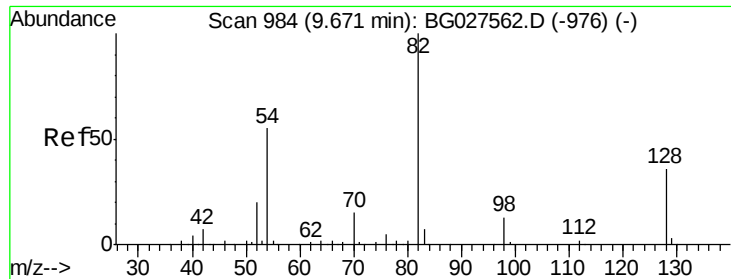




#23
 Nitrobenzene-d5
 Concen: 91.314 ng
 RT: 9.67 min Scan# 984
 Delta R.T. -0.00 min
 Lab File: BG027662.D
 Acq: 24 Jun 2017 16:49

Instrument :
 BNA_G
 ClientSampled :
 PB100066BL

Tgt Ion: 82 Resp: 158495
 Ion Ratio Lower Upper
 82 100
 128 37.4 26.4 39.6
 54 55.1 49.4 74.2

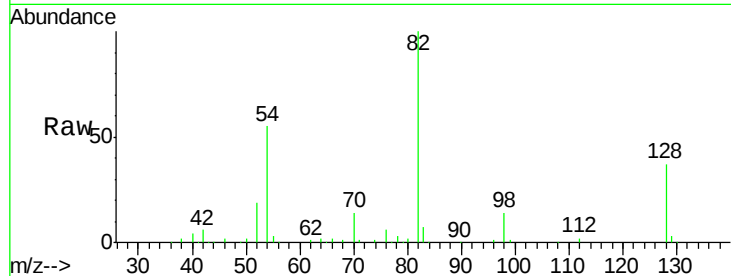


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

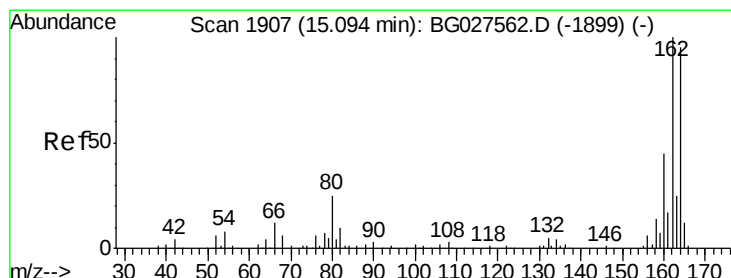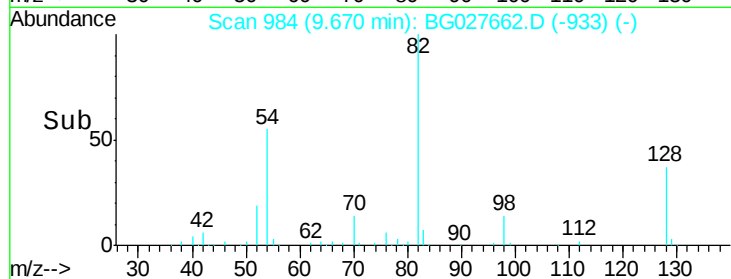
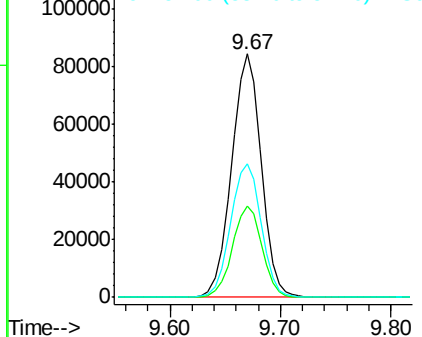



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.09 min Scan# 1906
 Delta R.T. -0.01 min
 Lab File: BG027662.D
 Acq: 24 Jun 2017 16:49

Tgt Ion: 164 Resp: 54333
 Ion Ratio Lower Upper
 164 100
 162 106.6 85.1 127.7
 160 46.1 34.7 52.1

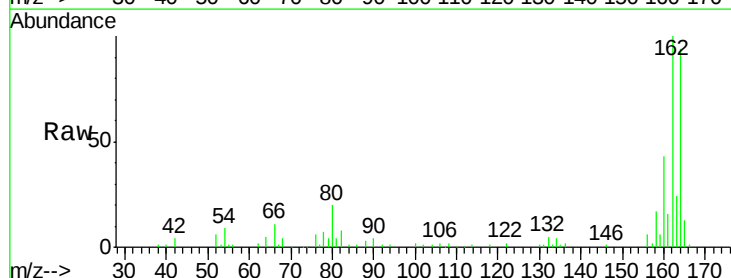

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC



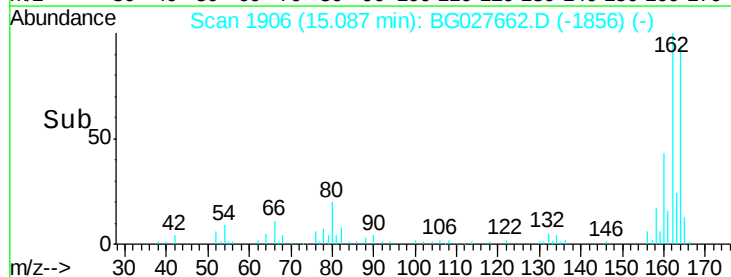
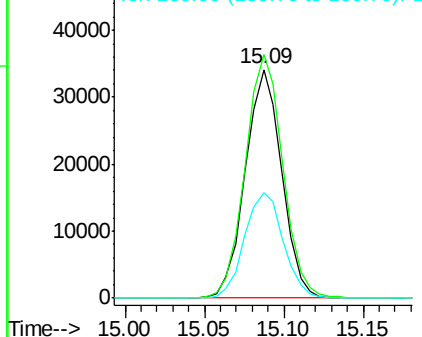


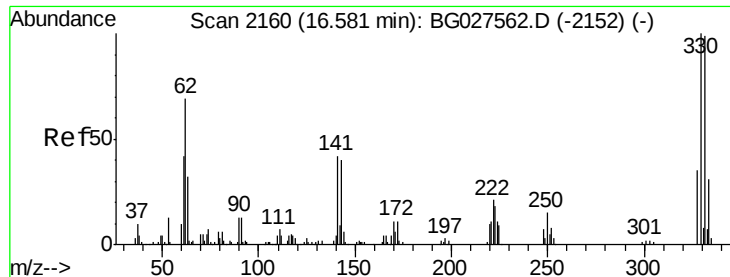

#41
 2,4,6-Tribromophenol
 Concen: 143.035 ng
 RT: 16.57 min Scan# 2159
 Delta R.T. -0.01 min
 Lab File: BG027662.D
 Acq: 24 Jun 2017 16:49




Instrument :
 BNA_G
 ClientSampleId :
 PB100066BL


Tgt Ion:330 Resp: 115861
 Ion Ratio Lower Upper
 330 100
 332 97.5 77.3 115.9
 141 42.5 32.1 48.1

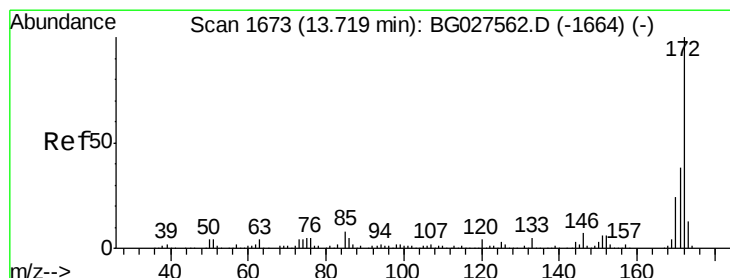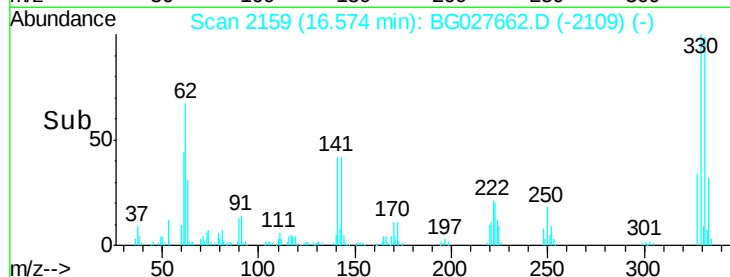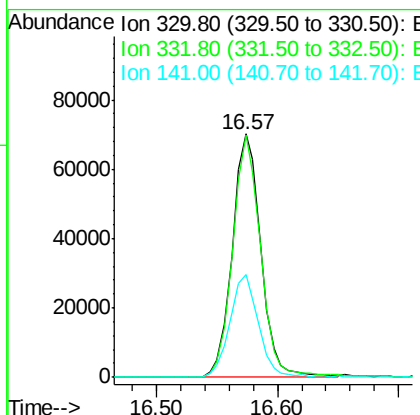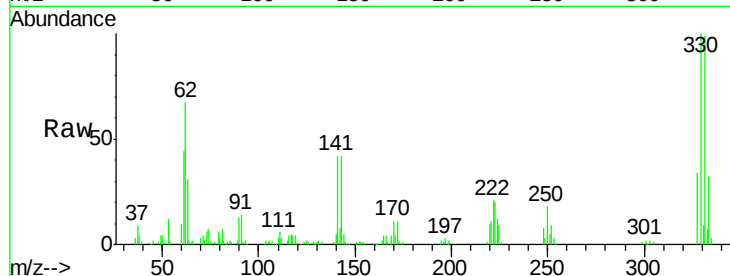

#44
 2-Fluorobiphenyl
 Concen: 93.822 ng
 RT: 13.71 min Scan# 1672
 Delta R.T. -0.01 min
 Lab File: BG027662.D
 Acq: 24 Jun 2017 16:49

Tgt Ion:172 Resp: 373182
 Ion Ratio Lower Upper
 172 100
 171 38.6 32.2 48.2
 170 25.3 21.8 32.6

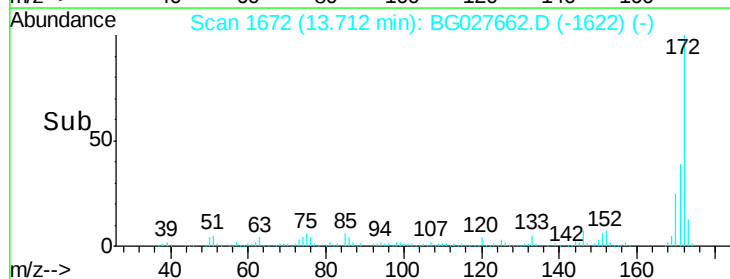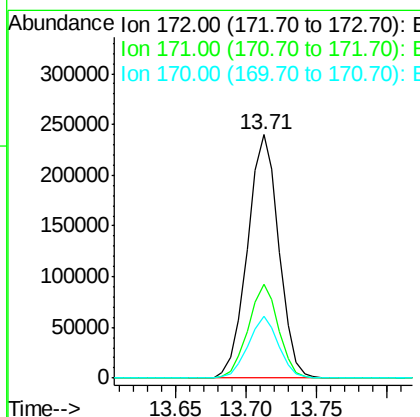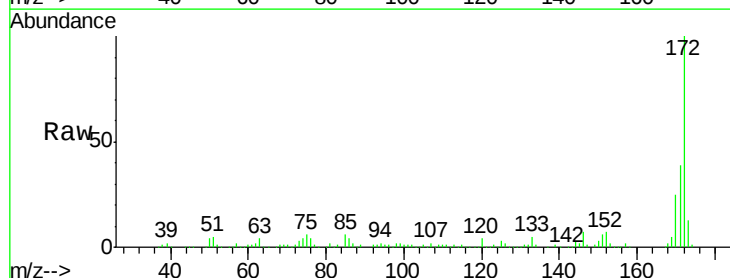


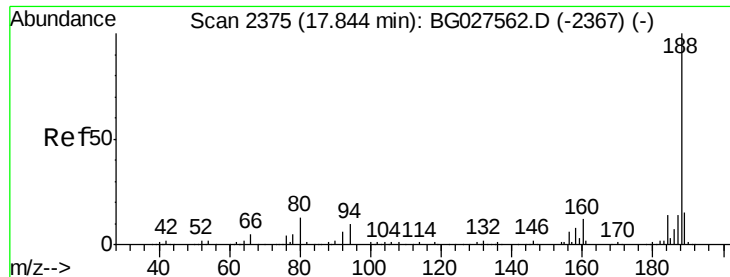




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.84 min Scan# 2374
Delta R.T. -0.01 min
Lab File: BG027662.D
Acq: 24 Jun 2017 16:49

Instrument :
BNA_G
ClientSampleId :
PB100066BL

Tgt Ion:188 Resp: 153717
Ion Ratio Lower Upper
188 100
94 7.5 5.8 8.8
80 9.5 7.5 11.3

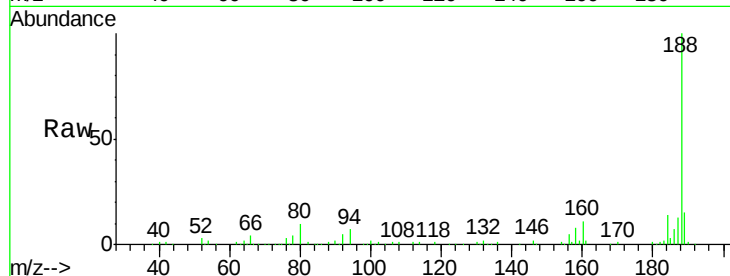


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

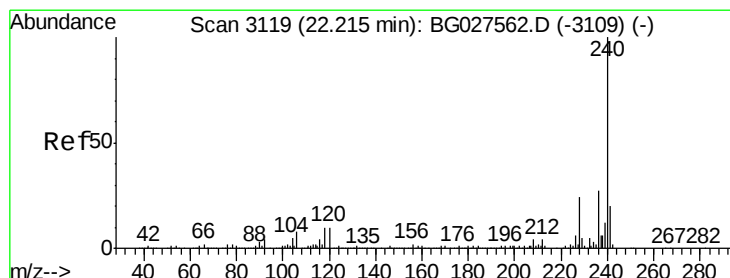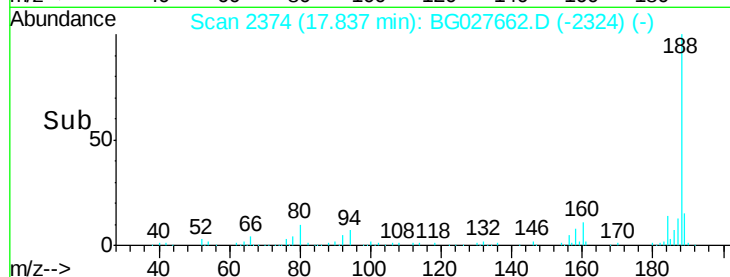
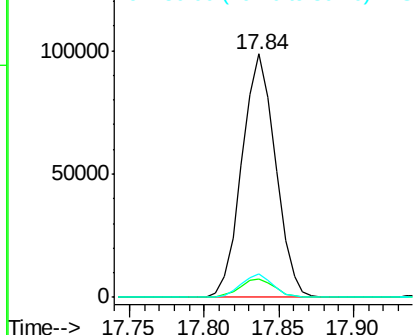



#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.20 min Scan# 3117
Delta R.T. -0.01 min
Lab File: BG027662.D
Acq: 24 Jun 2017 16:49

Tgt Ion:240 Resp: 171968
Ion Ratio Lower Upper
240 100
120 8.9 5.7 8.5#
236 25.6 22.2 33.4

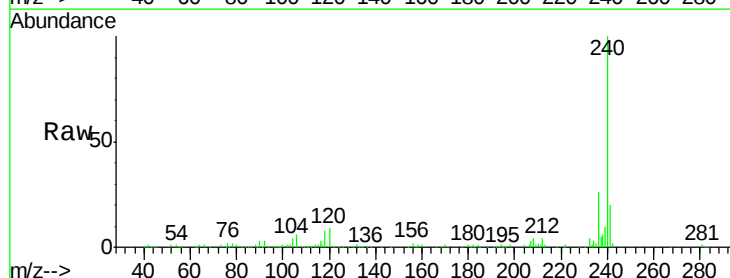

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

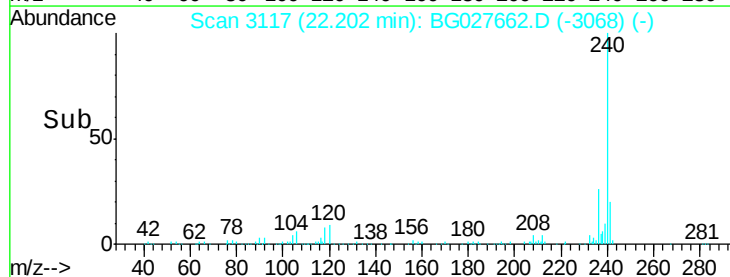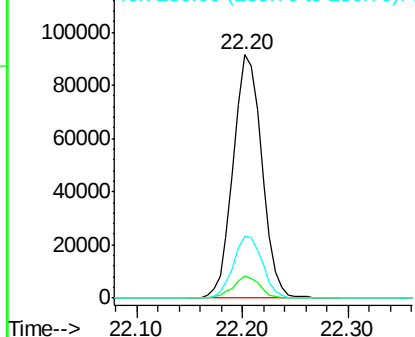

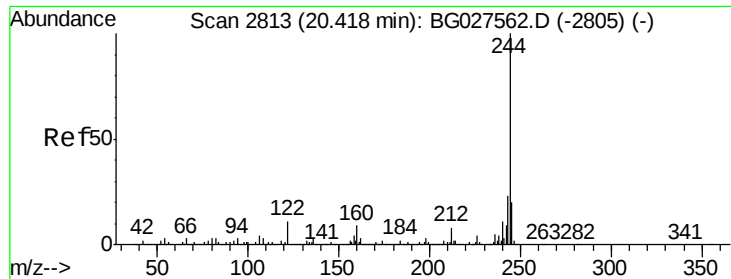

#78

Terphenyl-d14

Concen: 104.436 ng

RT: 20.42 min Scan# 2813

Delta R.T. -0.00 min

Lab File: BG027662.D

Acq: 24 Jun 2017 16:49

Instrument :

BNA_G

ClientSampleId :

PB100066BL


Tgt Ion:244 Resp: 762264

Ion Ratio Lower Upper

244 100

212 7.8 10.0 15.0#




122 9.1 8.6 12.8

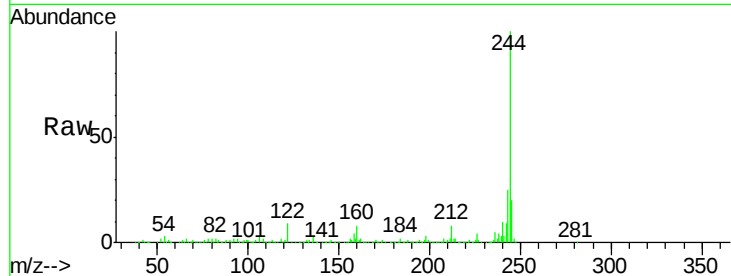

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

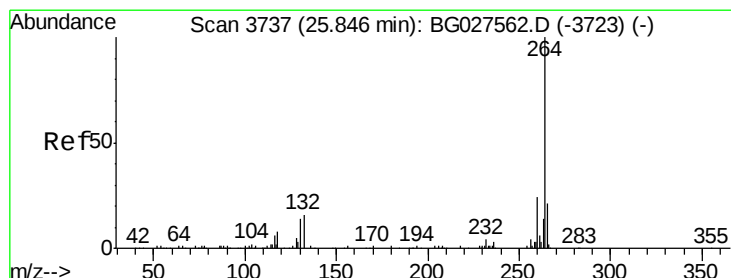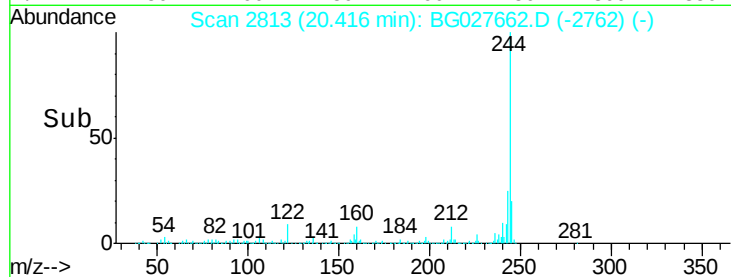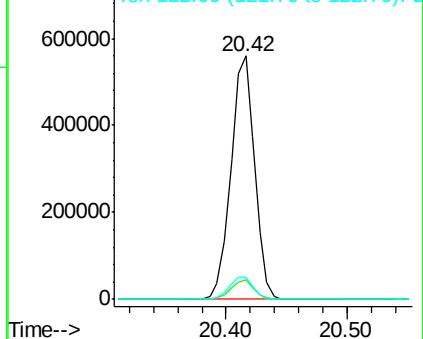

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.85 min Scan# 3737

Delta R.T. -0.00 min

Lab File: BG027662.D

Acq: 24 Jun 2017 16:49


Tgt Ion:264 Resp: 160164

Ion Ratio Lower Upper

264 100

260 24.8 21.8 32.8

265 22.1 18.2 27.4

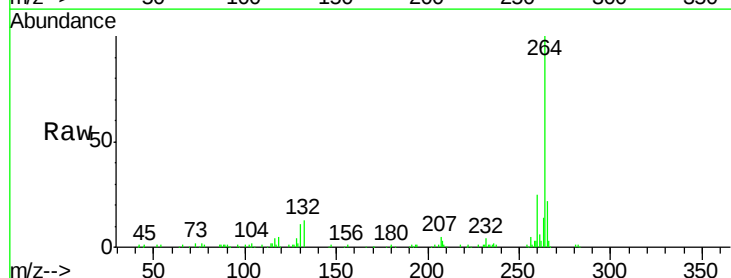

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

