

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG062417\
 Data File : BG027674.D
 Acq On : 25 Jun 2017 00:44
 Operator : SJ/JU
 Sample : I3868-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CL-01-062217-E

Quant Time: Jun 26 04:24:10 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 21 18:52:15 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.51	152	22056	20.00	ng	0.00
21) Naphthalene-d8	11.32	136	96340	20.00	ng	0.00
38) Acenaphthene-d10	15.09	164	56591	20.00	ng	0.00
63) Phenanthrene-d10	17.84	188	145685	20.00	ng	0.00
75) Chrysene-d12	22.20	240	167509	20.00	ng	-0.01
86) Perylene-d12	25.84	264	161367	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.09	112	165904	107.05	ng	0.00
7) Phenol-d6	7.65	99	209917	91.50	ng	0.00
23) Nitrobenzene-d5	9.67	82	159812	78.49	ng	0.00
41) 2,4,6-Tribromophenol	16.57	330	92482	109.62	ng	0.00
44) 2-Fluorobiphenyl	13.71	172	366261	88.41	ng	0.00
78) Terphenyl-d14	20.41	244	696749	98.00	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG062417\
Data File : BG027674.D
Acq On : 25 Jun 2017 00:44
Operator : SJ/JU
Sample : I3868-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-01-062217-E

Quant Time: Jun 26 04:24:10 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 18:52:15 2017
Response via : Initial Calibration

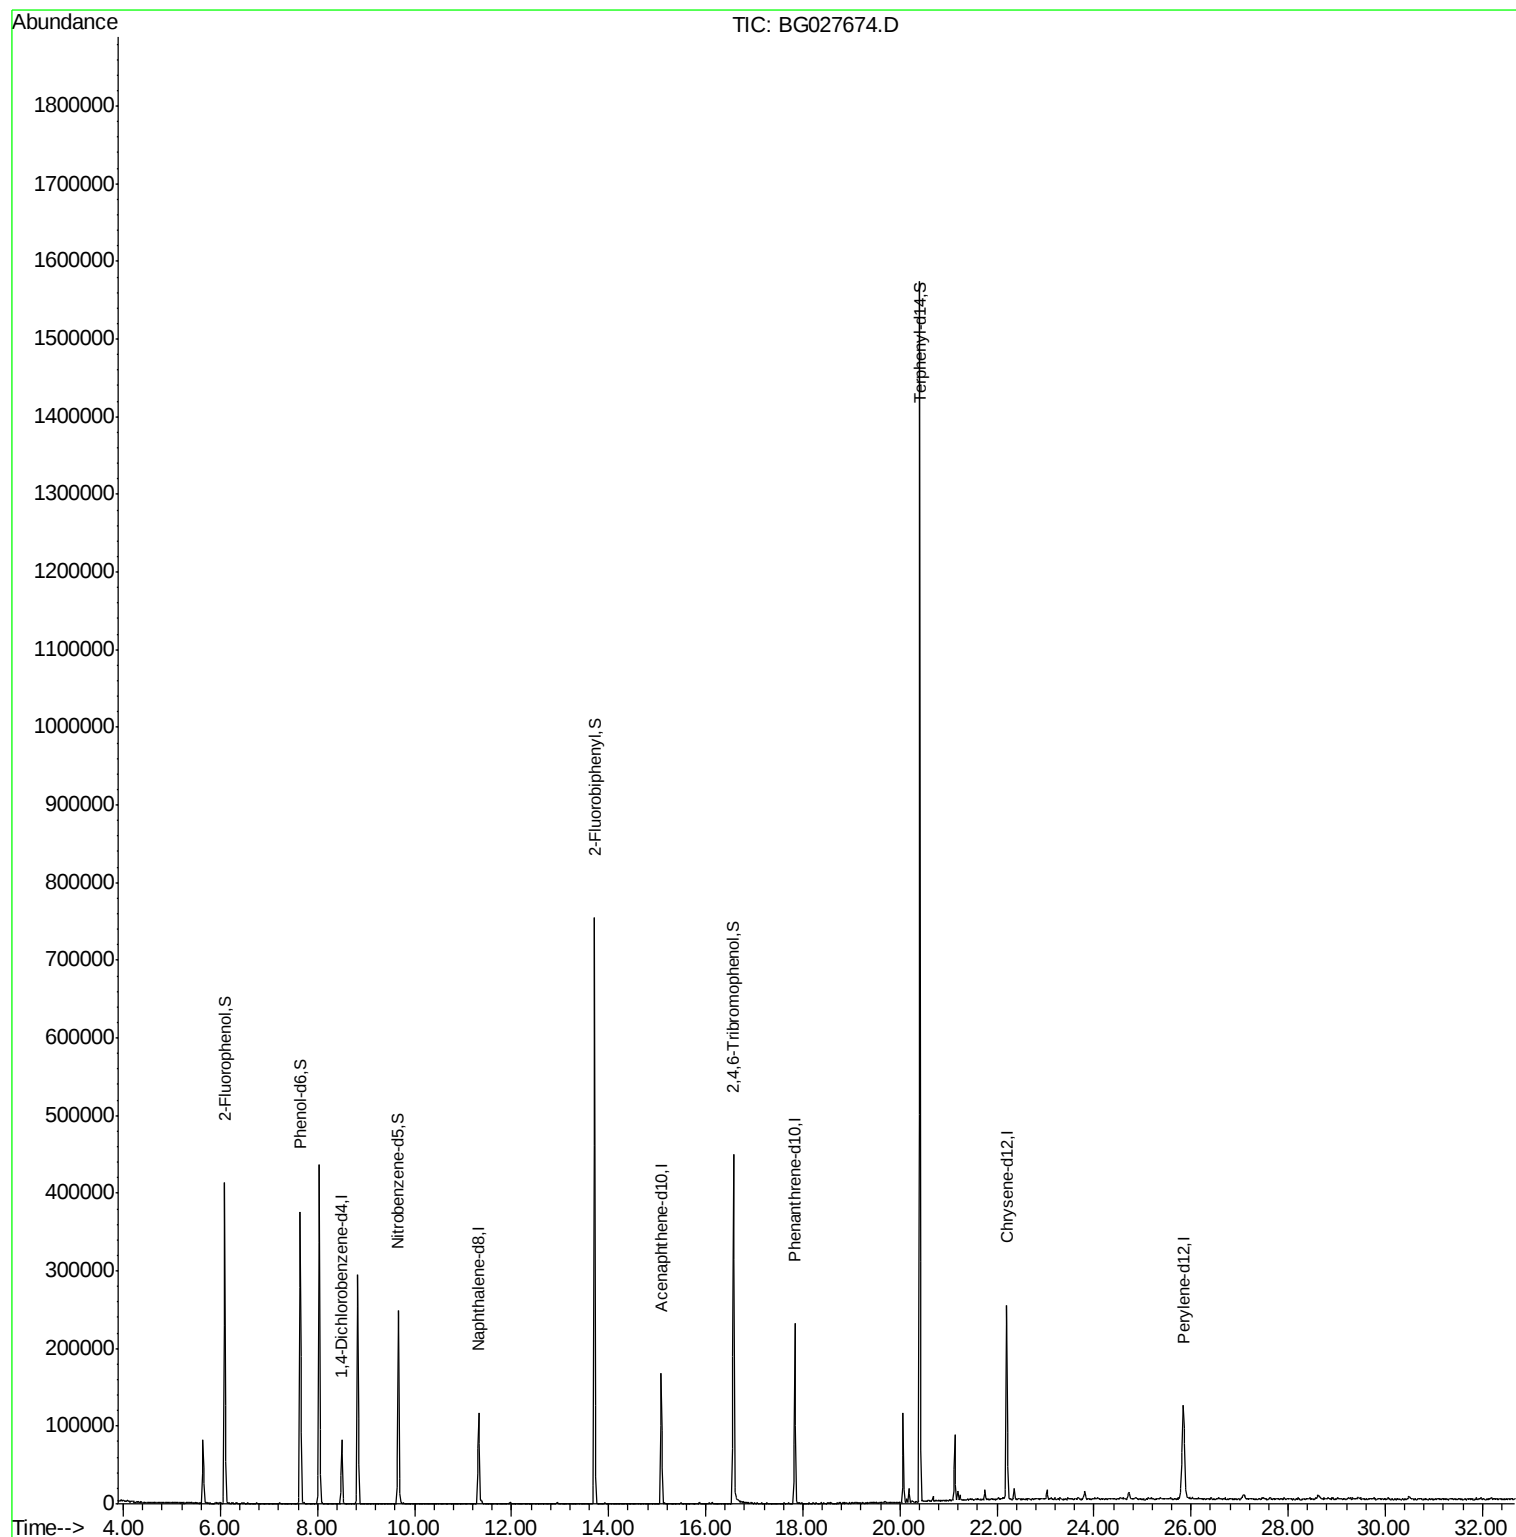




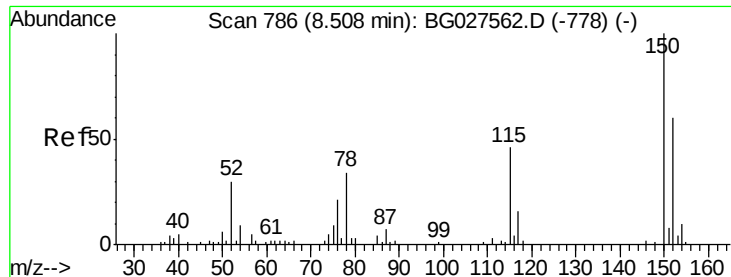


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.51 min Scan# 786
 Delta R.T. -0.00 min
 Lab File: BG027674.D
 Acq: 25 Jun 2017 00:44

Instrument :
 BNA_G
 ClientSampleId :
 CL-01-062217-E




Tgt Ion:152 Resp: 22056
 Ion Ratio Lower Upper
 152 100
 150 146.5 114.0 171.0
 115 75.0 48.1 72.1#

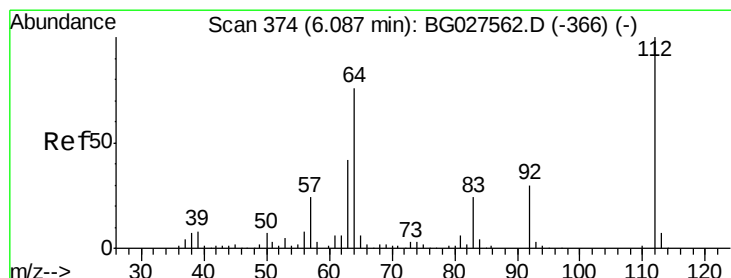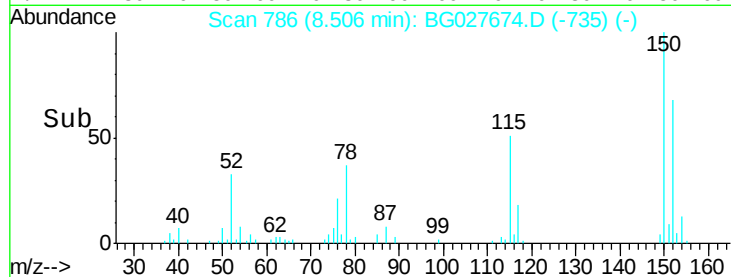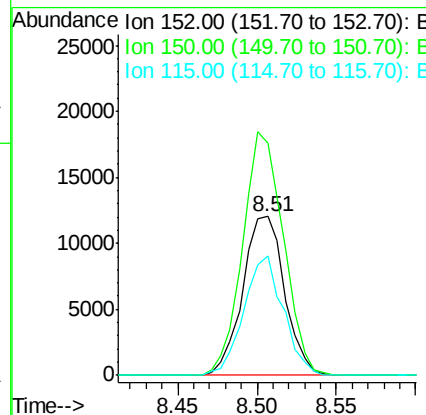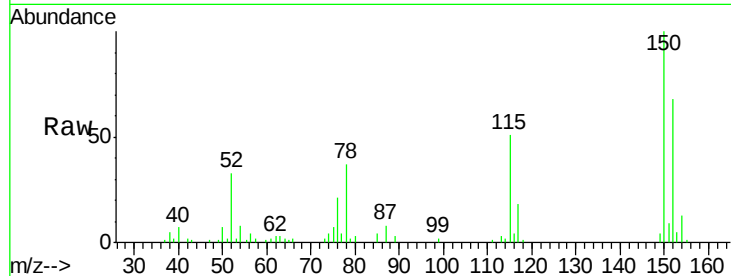


#5

2-Fluorophenol
 Concen: 107.054 ng
 RT: 6.09 min Scan# 375
 Delta R.T. 0.00 min
 Lab File: BG027674.D
 Acq: 25 Jun 2017 00:44

Tgt Ion:112 Resp: 165904
 Ion Ratio Lower Upper
 112 100
 64 73.1 61.8 92.6
 63 42.5 37.2 55.8

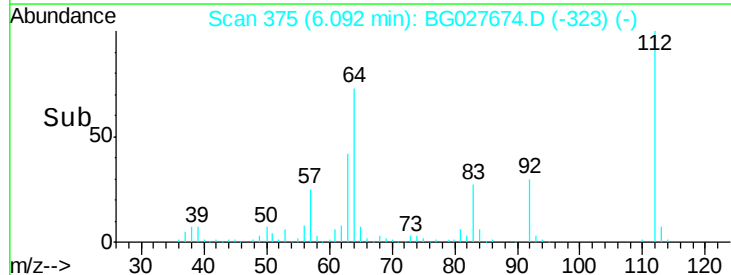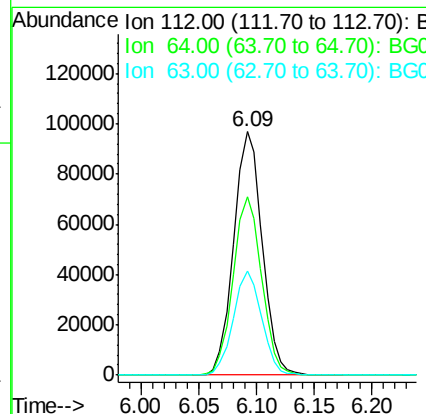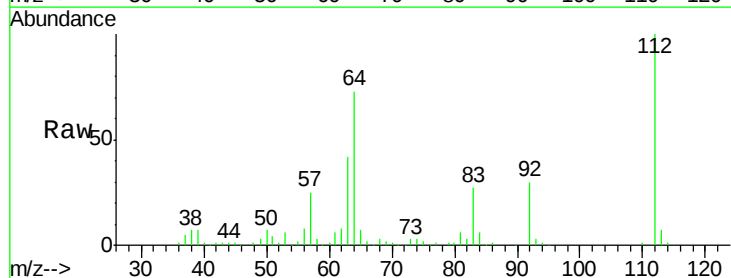

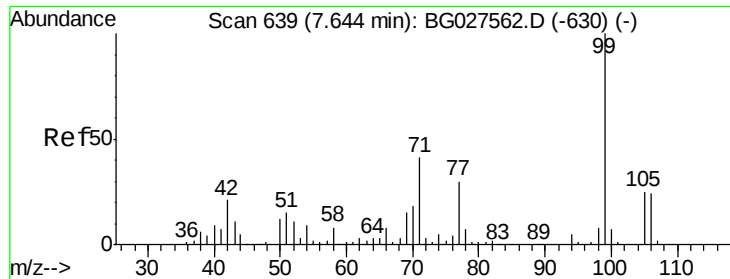

#7

Phenol-d6

Concen: 91.498 ng

RT: 7.65 min Scan# 640

Delta R.T. 0.00 min

Lab File: BG027674.D

Acq: 25 Jun 2017 00:44

Instrument :

BNA_G

ClientSampleId :

CL-01-062217-E


Tgt Ion: 99 Resp: 209917

Ion Ratio Lower Upper




99 100

42 22.3 20.5 30.7

71 47.9 37.6 56.4

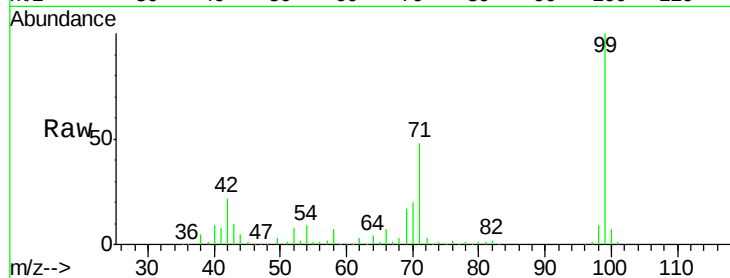

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

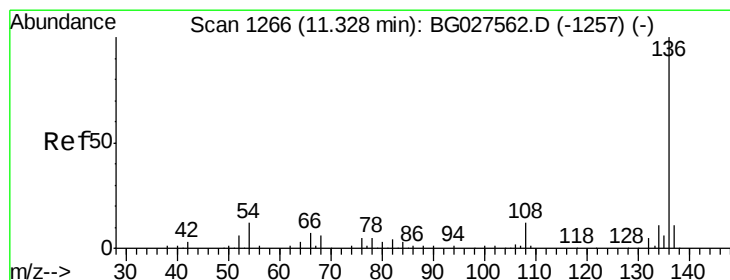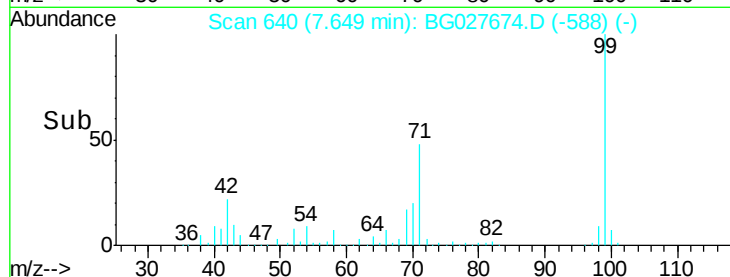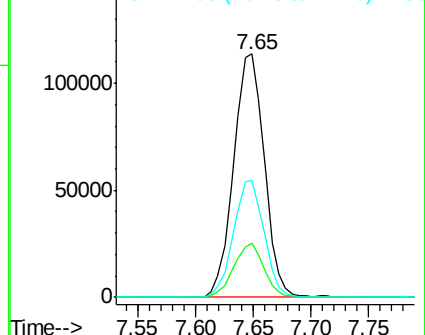

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.32 min Scan# 1265

Delta R.T. -0.01 min

Lab File: BG027674.D

Acq: 25 Jun 2017 00:44

Tgt Ion: 136 Resp: 96340


Ion Ratio Lower Upper

136 100



137 11.3 8.9 13.3


54 9.4 9.3 13.9

68 4.3 5.1 7.7#

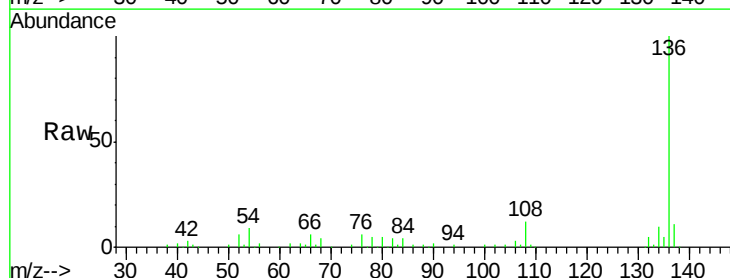

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

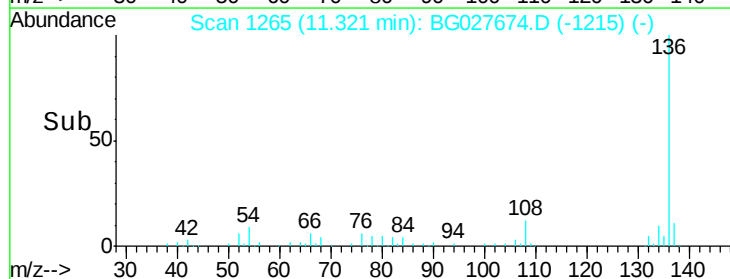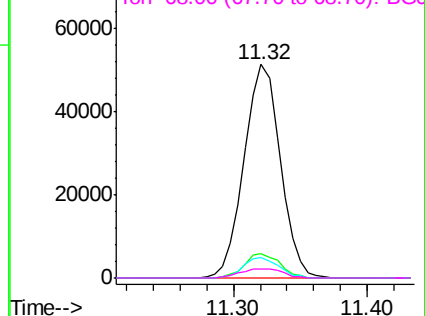


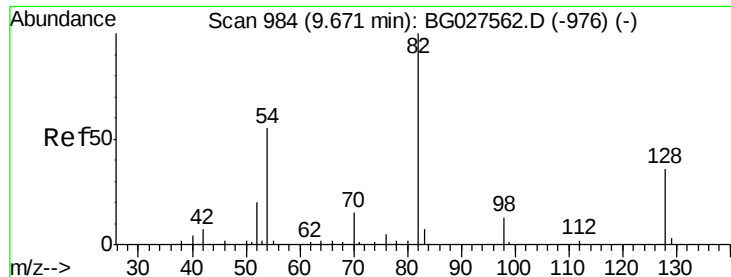




#23
 Nitrobenzene-d5
 Concen: 78.494 ng
 RT: 9.67 min Scan# 984
 Delta R.T. -0.00 min
 Lab File: BG027674.D
 Acq: 25 Jun 2017 00:44

Instrument :
 BNA_G
 ClientSampleId :
 CL-01-062217-E

Tgt Ion: 82 Resp: 159812
 Ion Ratio Lower Upper
 82 100
 128 37.7 26.4 39.6
 54 56.0 49.4 74.2

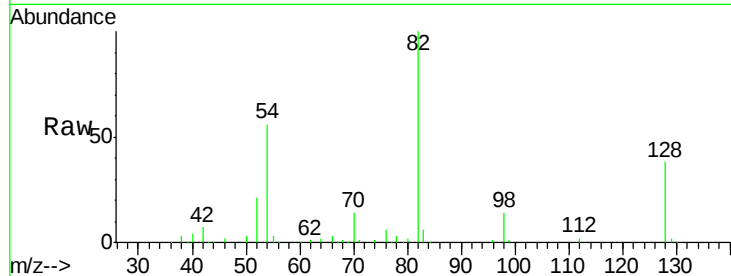


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

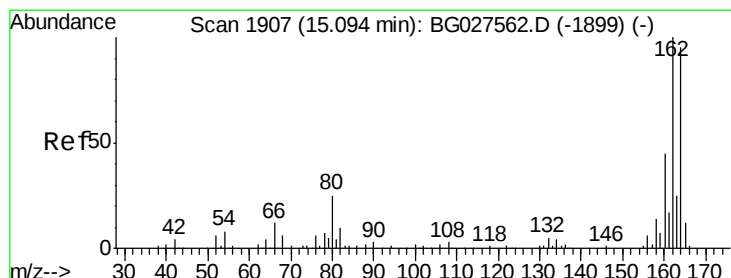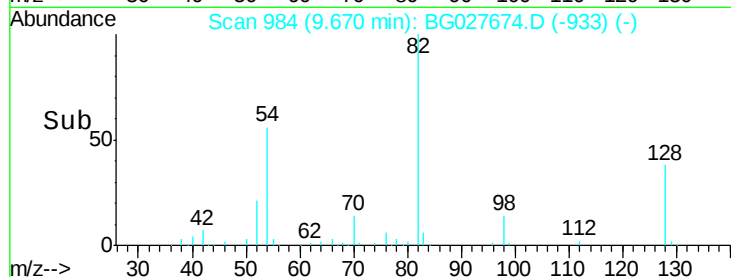
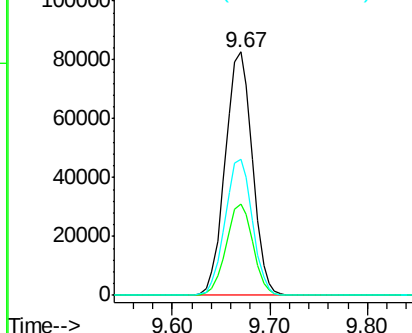



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.09 min Scan# 1906
 Delta R.T. -0.01 min
 Lab File: BG027674.D
 Acq: 25 Jun 2017 00:44

Tgt Ion: 164 Resp: 56591
 Ion Ratio Lower Upper
 164 100
 162 108.5 85.1 127.7
 160 49.6 34.7 52.1

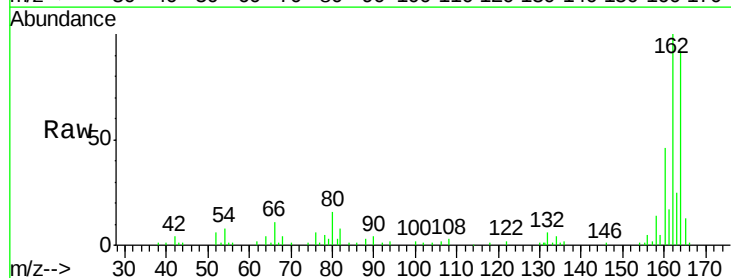

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

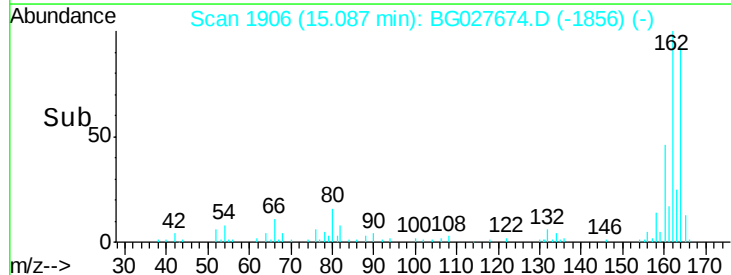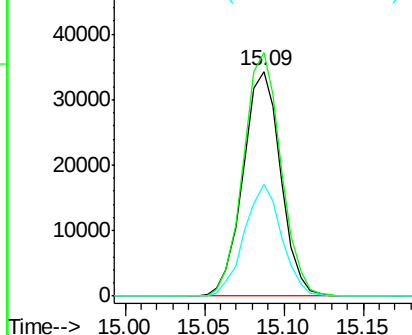


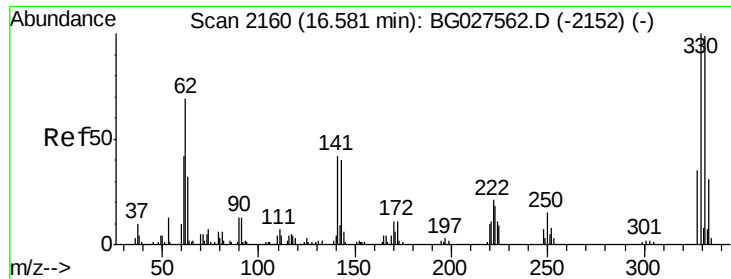




#41
 2,4,6-Tribromophenol
 Concen: 109.617 ng
 RT: 16.57 min Scan# 2159
 Delta R.T. -0.01 min
 Lab File: BG027674.D
 Acq: 25 Jun 2017 00:44

Instrument :
 BNA_G
 ClientSampleId :
 CL-01-062217-E

Tgt Ion:330 Resp: 92482
 Ion Ratio Lower Upper
 330 100
 332 94.3 77.3 115.9
 141 37.2 32.1 48.1

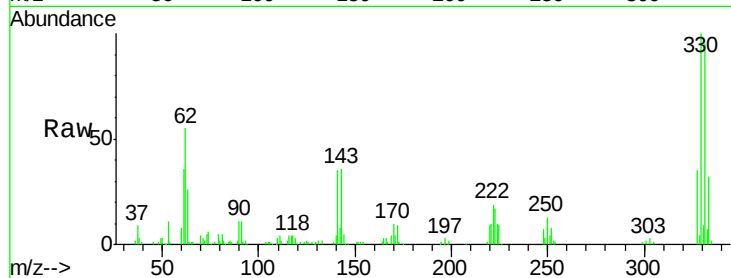


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

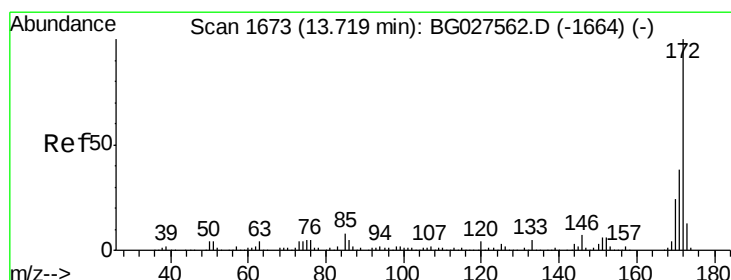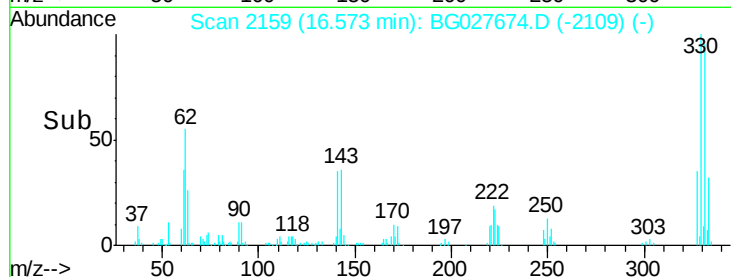
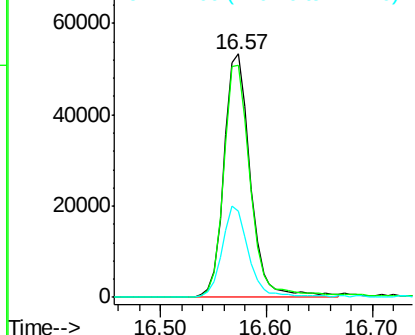



#44
 2-Fluorobiphenyl
 Concen: 88.408 ng
 RT: 13.71 min Scan# 1672
 Delta R.T. -0.01 min
 Lab File: BG027674.D
 Acq: 25 Jun 2017 00:44

Tgt Ion:172 Resp: 366261
 Ion Ratio Lower Upper
 172 100
 171 38.0 32.2 48.2
 170 24.2 21.8 32.6

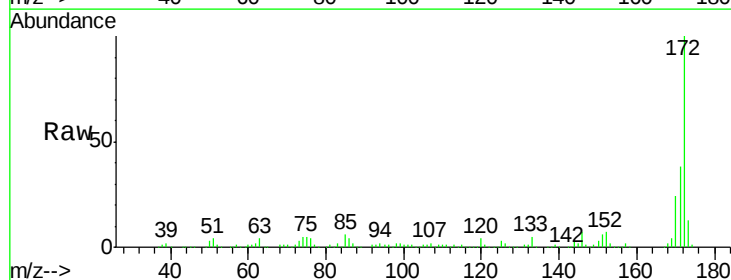

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

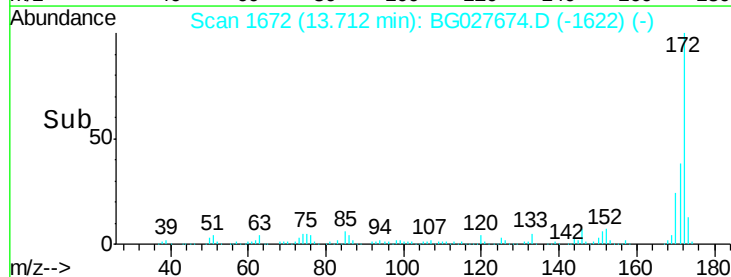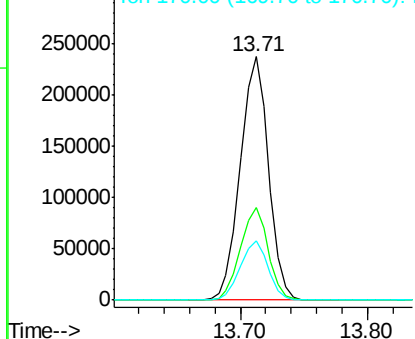


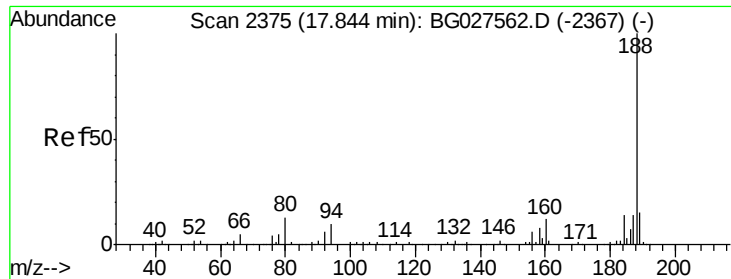




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.84 min Scan# 2374
Delta R.T. -0.01 min
Lab File: BG027674.D
Acq: 25 Jun 2017 00:44

Instrument :
BNA_G
ClientSampleId :
CL-01-062217-E

Tgt Ion:188 Resp: 145685
Ion Ratio Lower Upper
188 100
94 7.5 5.8 8.8
80 9.8 7.5 11.3

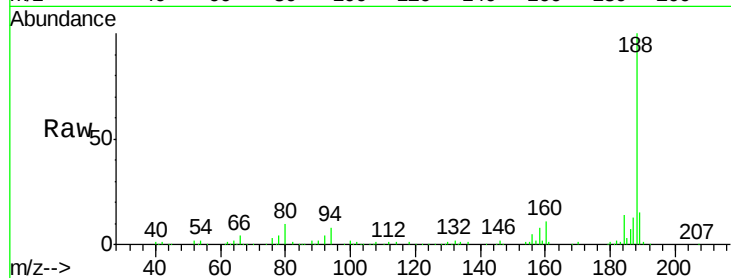


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

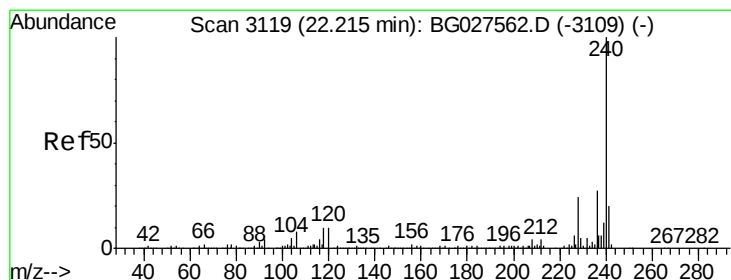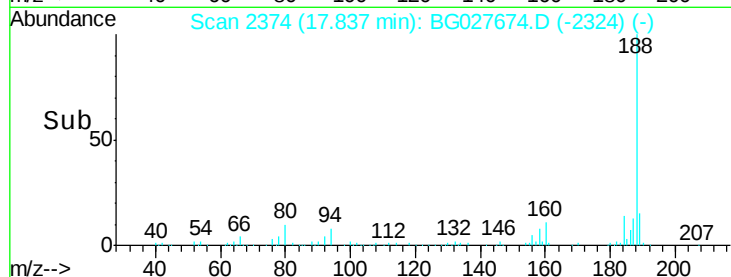
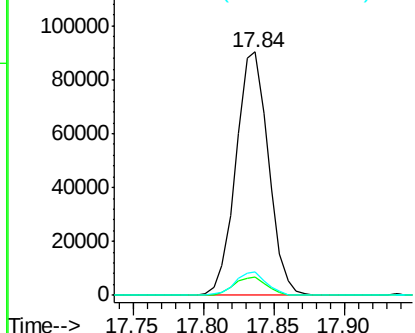



#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.20 min Scan# 3117
Delta R.T. -0.01 min
Lab File: BG027674.D
Acq: 25 Jun 2017 00:44

Tgt Ion:240 Resp: 167509
Ion Ratio Lower Upper
240 100
120 7.0 5.7 8.5
236 24.3 22.2 33.4

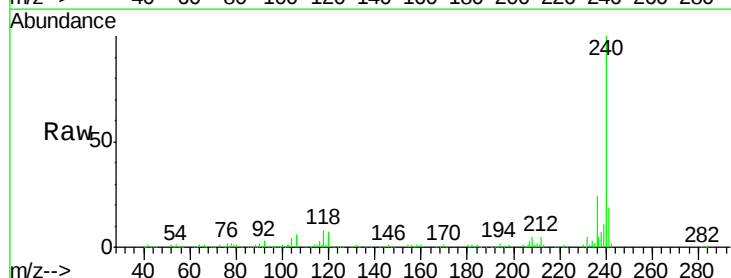

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



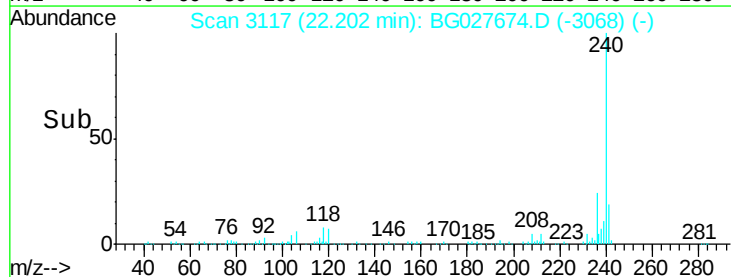
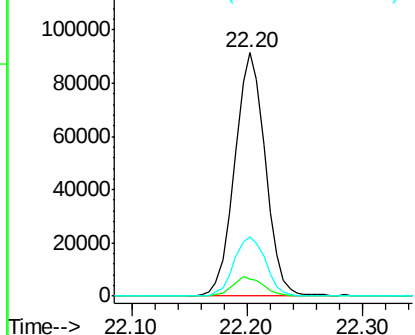


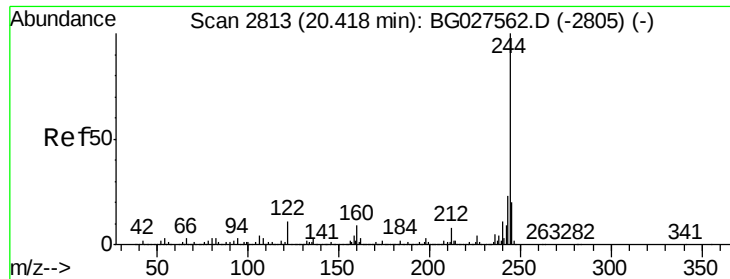

#78
 Terphenyl-d14
 Concen: 98.001 ng
 RT: 20.41 min Scan# 2812
 Delta R.T. -0.01 min
 Lab File: BG027674.D
 Acq: 25 Jun 2017 00:44

Instrument :
 BNA_G
 ClientSampleId :
 CL-01-062217-E

Tgt Ion:244 Resp: 696749
 Ion Ratio Lower Upper
 244 100
 212 8.3 10.0 15.0#
 122 9.5 8.6 12.8

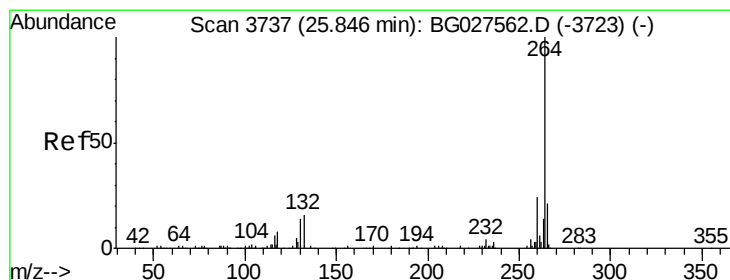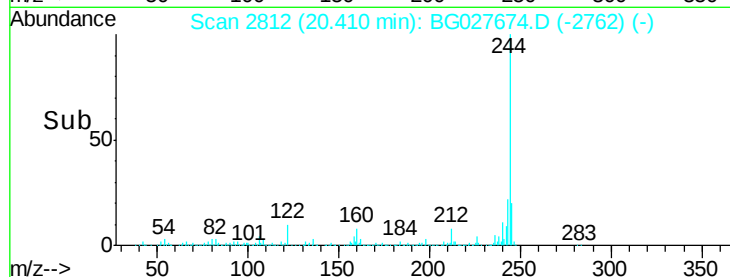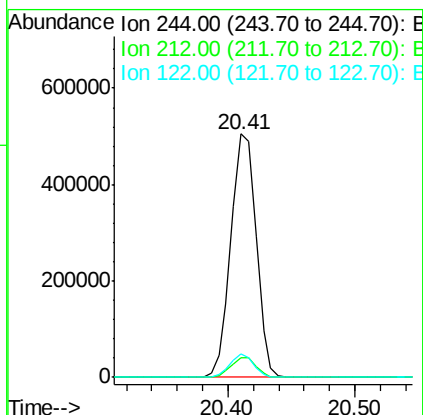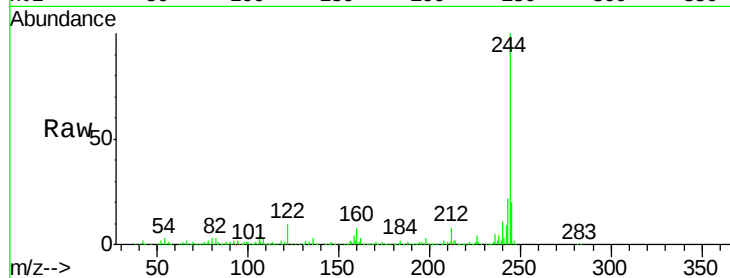

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.84 min Scan# 3736
 Delta R.T. -0.01 min
 Lab File: BG027674.D
 Acq: 25 Jun 2017 00:44

Tgt Ion:264 Resp: 161367
 Ion Ratio Lower Upper
 264 100
 260 23.1 21.8 32.8
 265 21.3 18.2 27.4

