


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_G\Data\BG062417\
 Data File : BG027650.D
 Acq On : 24 Jun 2017 8:48
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 21 18:52:15 2017

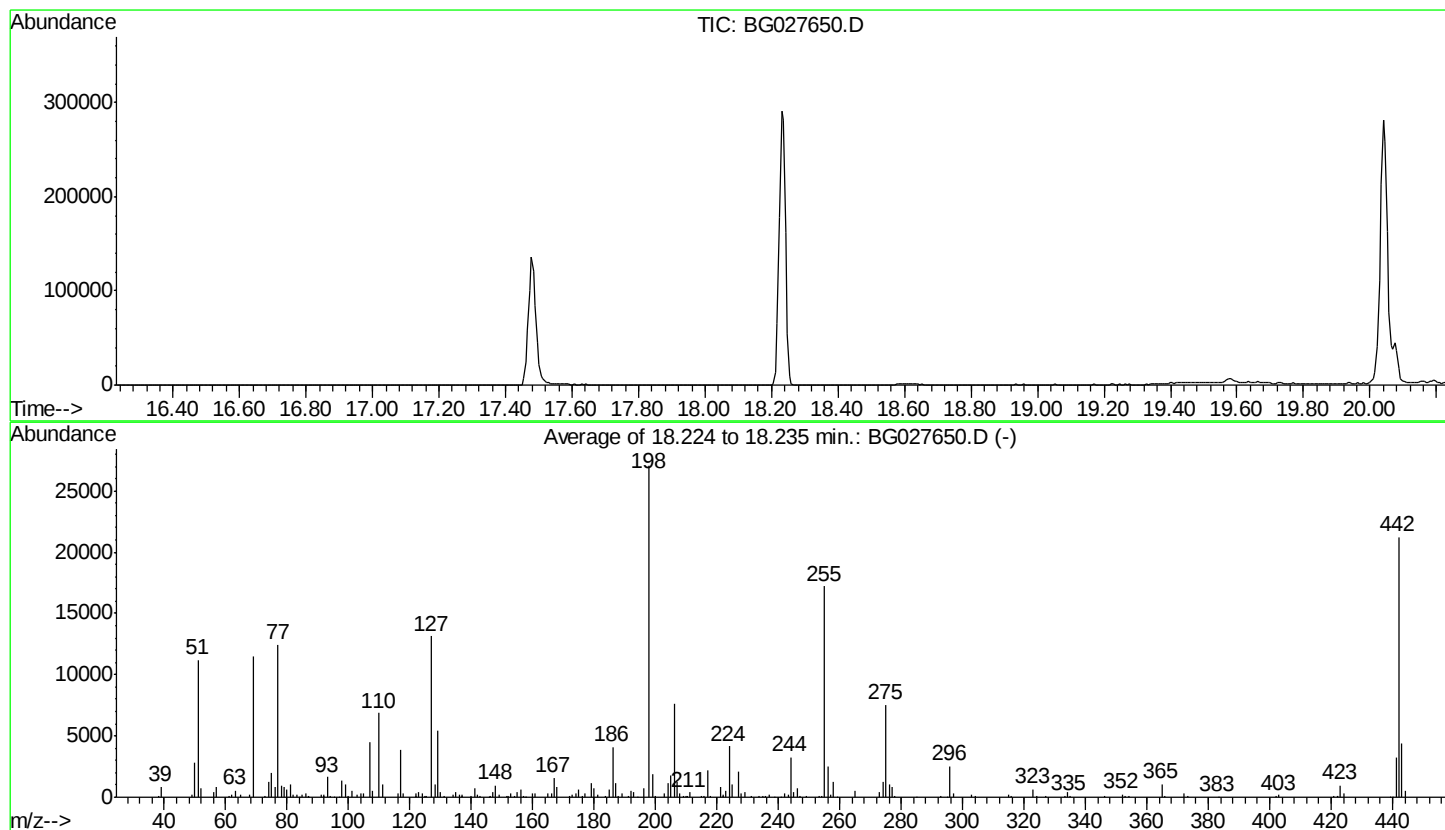

AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	11229	PASS
68	69	0.00	2	1.8	213	PASS
69	198	0.00	100	42.7	11544	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.5	13114	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	27061	PASS
199	198	5	9	6.9	1871	PASS
275	198	10	60	27.9	7552	PASS
365	198	1	100	3.9	1067	PASS
441	442	0.01	24	15.3	3257	PASS
442	198	50	100	78.5	21246	PASS
443	442	15	24	20.7	4402	PASS