
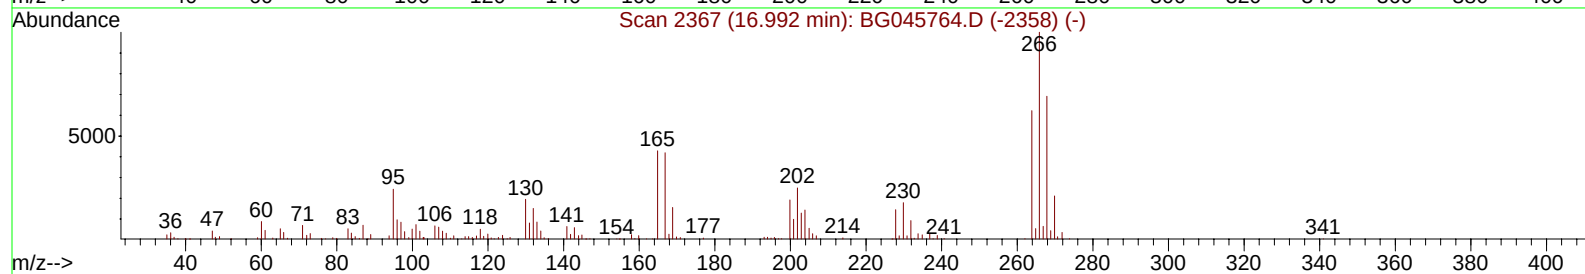
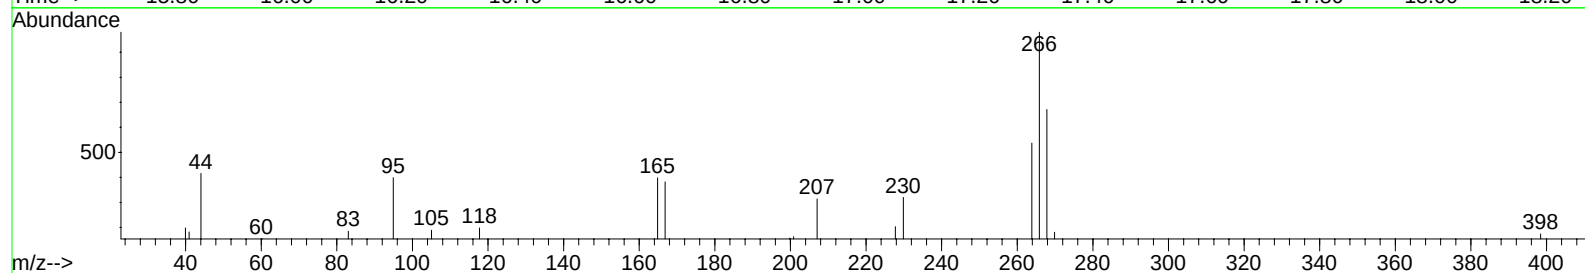


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062420\
 Data File : BG045840.D
 Acq On : 24 Jun 2020 10:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 18:53:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 15 18:34:19 2020
 Response via : Initial Calibration

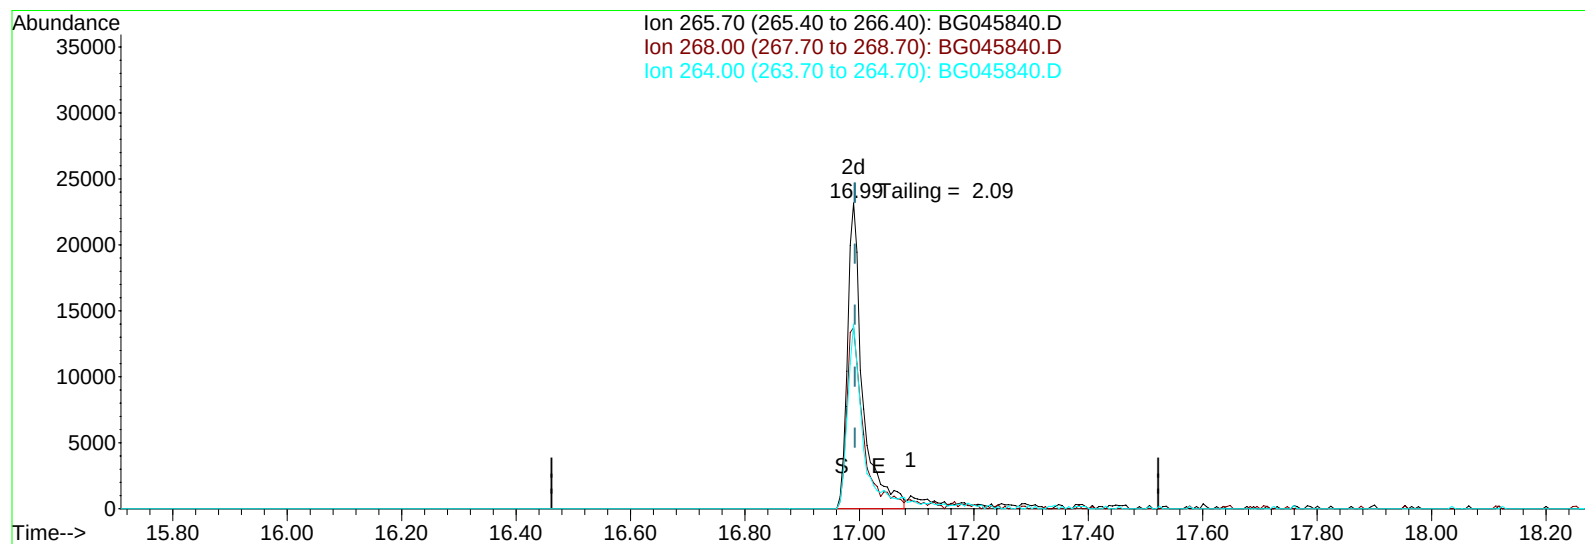

TIC: BG045840.D

(70) Pentachlorophenol (C)




17.090min (+0.098) 690.89ng

response 1581

Ion	Exp%	Act%
265.70	100	100
268.00	69.20	68.47
264.00	62.20	54.80
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062420\
 Data File : BG045840.D
 Acq On : 24 Jun 2020 10:03
 Operator : CG/JU
 Sample : DF TPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 18:53:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 15 18:34:19 2020
 Response via : Initial Calibration

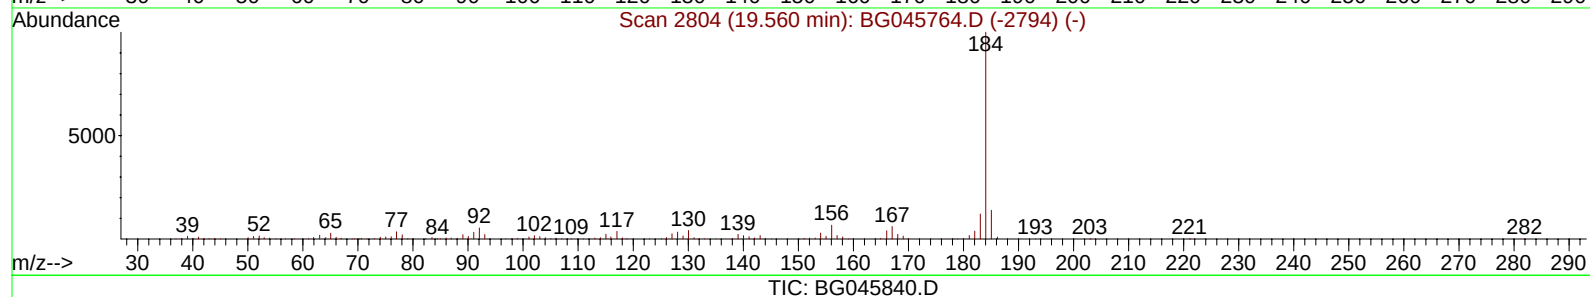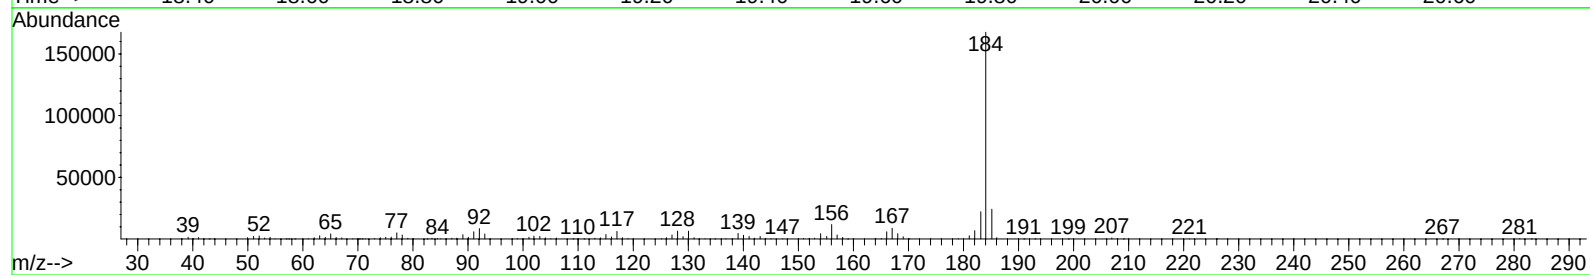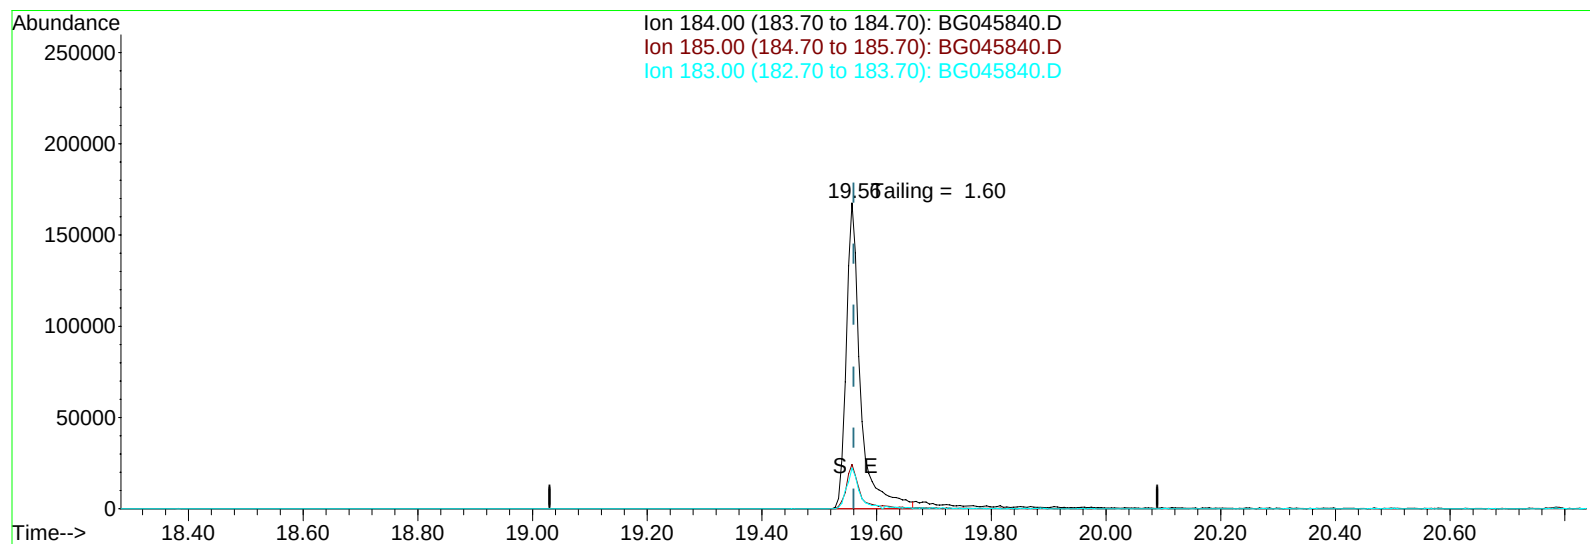

(77) Benzidine

19.557min (-0.003) 172917.31ng

response 296692

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.50
183.00	12.10	13.28
0.00	0.00	0.00