

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062420\
 Data File : BG045853.D
 Acq On : 24 Jun 2020 20:36
 Operator : CG/JU
 Sample : L3089-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 RB44767-RT

Quant Time: Jun 25 00:57:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 15 18:34:19 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	51910	20.00	ng	0.00
21) Naphthalene-d8	10.72	136	205985	20.00	ng	0.00
39) Acenaphthene-d10	14.56	164	149123	20.00	ng	0.00
64) Phenanthrene-d10	17.32	188	340716	20.00	ng	0.00
76) Chrysene-d12	21.57	240	331889	20.00	ng	0.00
86) Perylene-d12	24.70	264	342917	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	325117	105.80	ng	-0.02
7) Phenol-d6	7.14	99	414301	88.63	ng	-0.03
23) Nitrobenzene-d5	9.08	82	388437	86.15	ng	0.00
42) 2,4,6-Tribromophenol	16.06	330	298522	132.60	ng	0.00
45) 2-Fluorobiphenyl	13.19	172	906493	89.33	ng	0.00
79) Terphenyl-d14	19.94	244	1585680	96.83	ng	0.00
Target Compounds						
50) Dimethylphthalate	14.02	163	47635	4.078	ng	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062420\
Data File : BG045853.D
Acq On : 24 Jun 2020 20:36
Operator : CG/JU
Sample : L3089-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RB44767-RT

Quant Time: Jun 25 00:57:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 18:34:19 2020
Response via : Initial Calibration

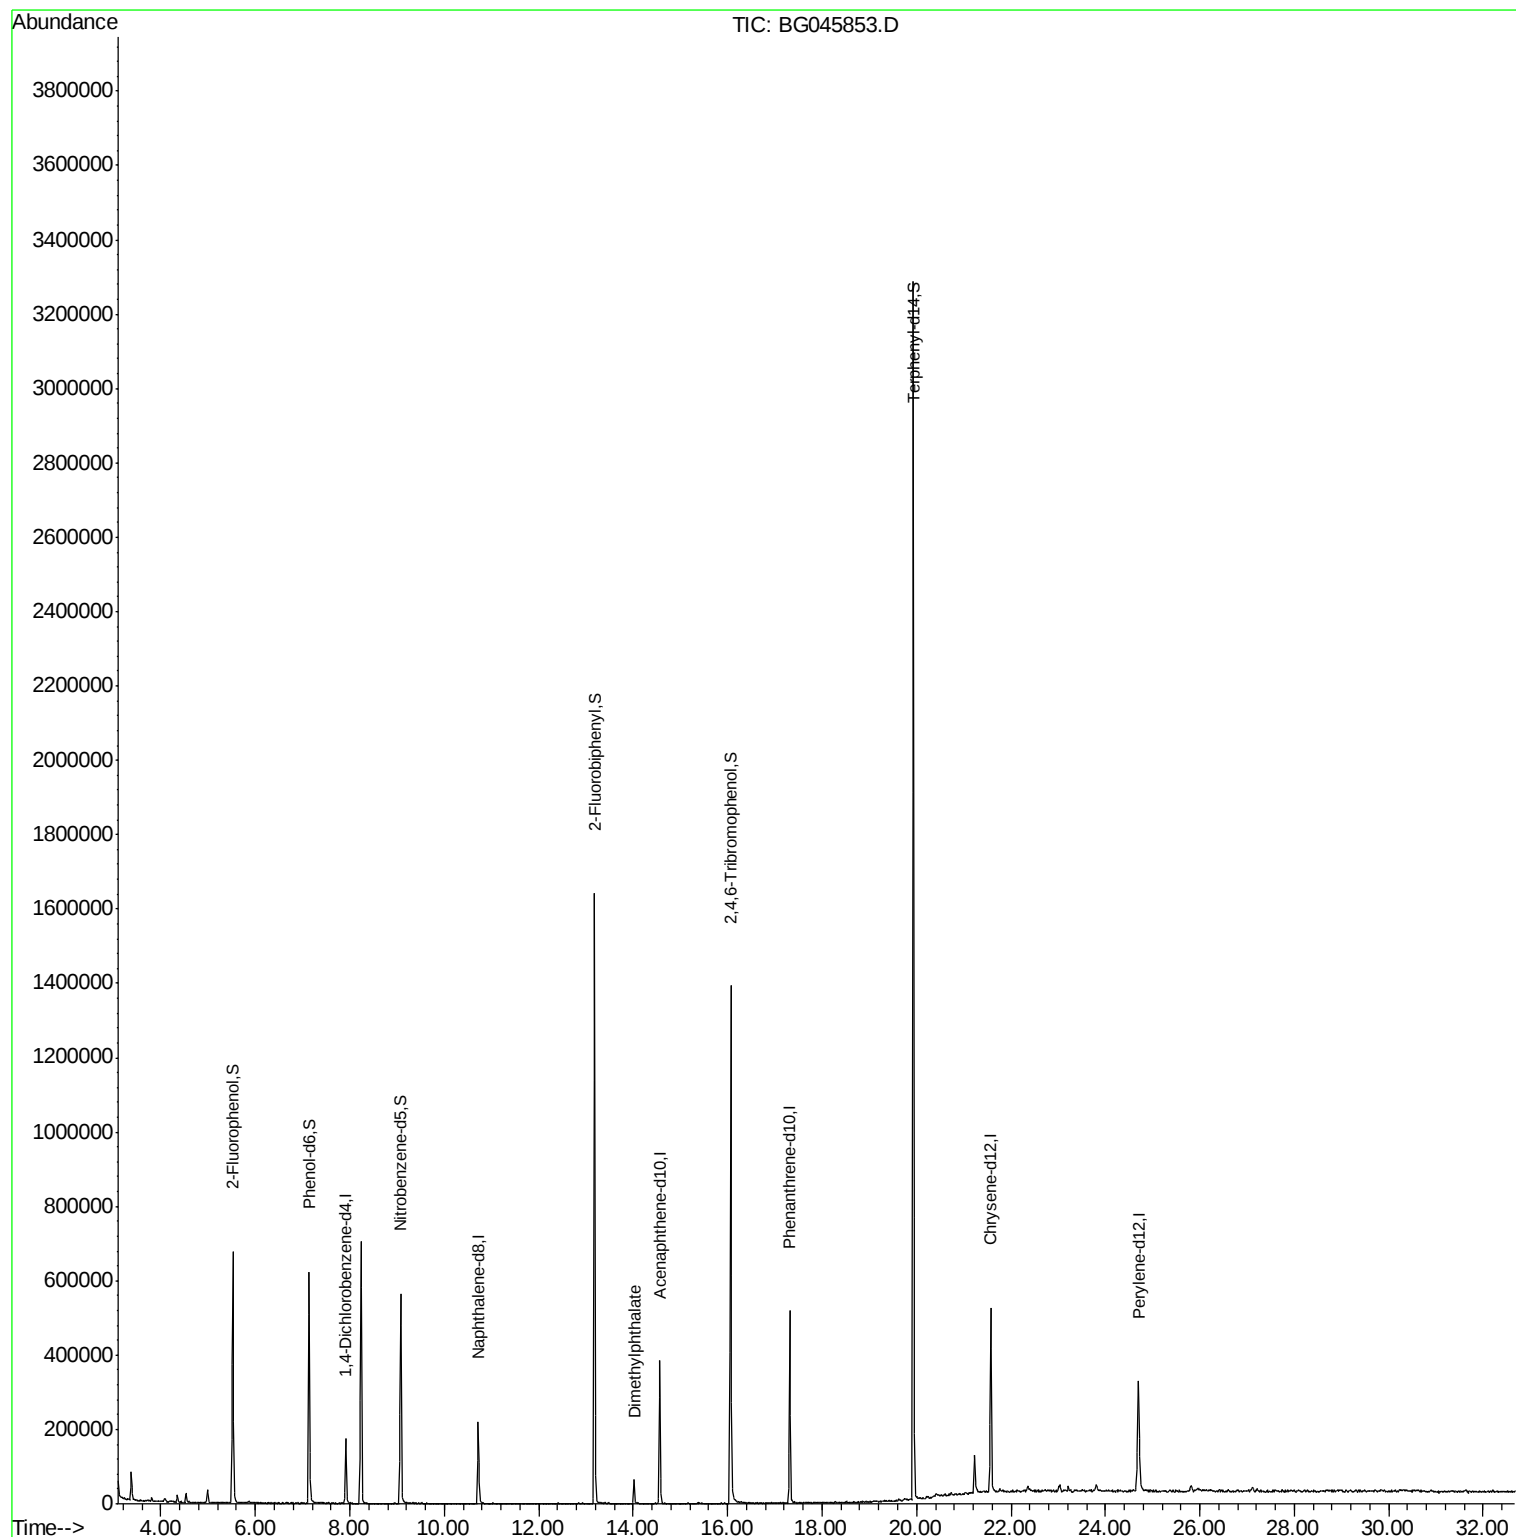







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.92 min Scan# 822
Delta R.T. -0.01 min
Lab File: BG045853.D
Acq: 24 Jun 2020 20:36

Instrument :
BNA_G
ClientSampleId :
RB44767-RT




Tot Ion	Ratio	Lower	Upper
152	100		
150	156.9	113.1	169.7
115	61.9	43.8	65.6

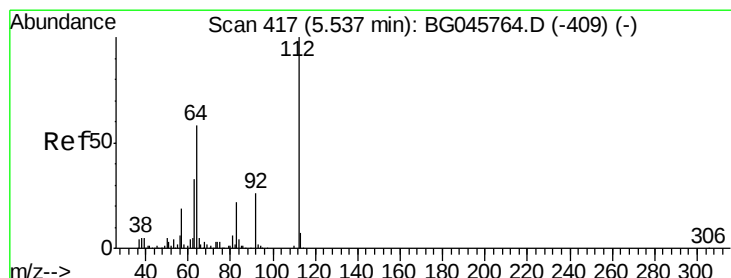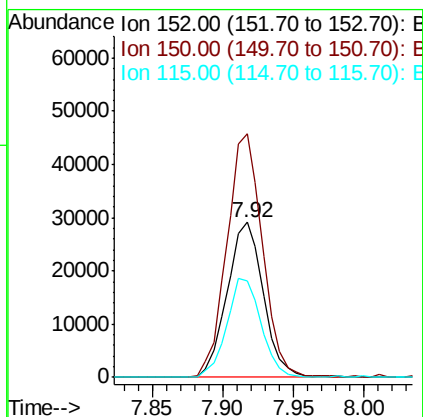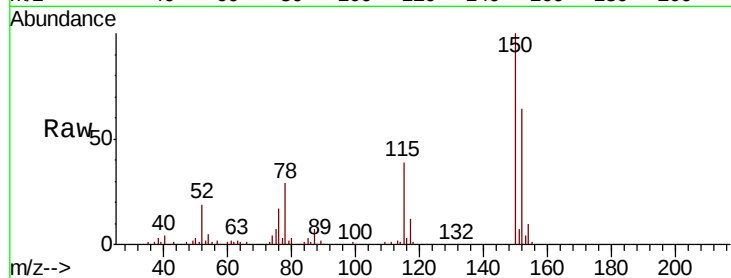


#5

2-Fluorophenol
Concen: 105.798 ng
RT: 5.52 min Scan# 414
Delta R.T. -0.02 min
Lab File: BG045853.D
Acq: 24 Jun 2020 20:36

Tgt Ion	Ratio	Lower	Upper
112	100		
64	58.2	46.6	69.8
63	33.2	26.3	39.5

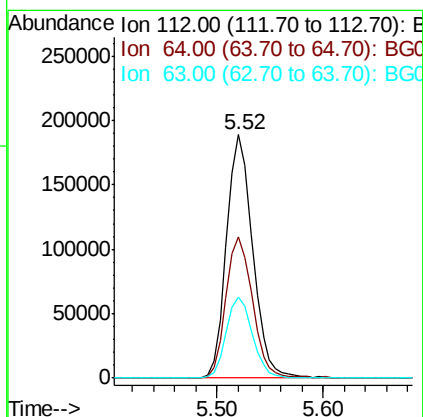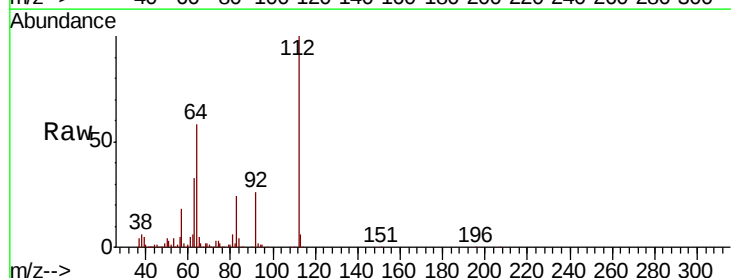

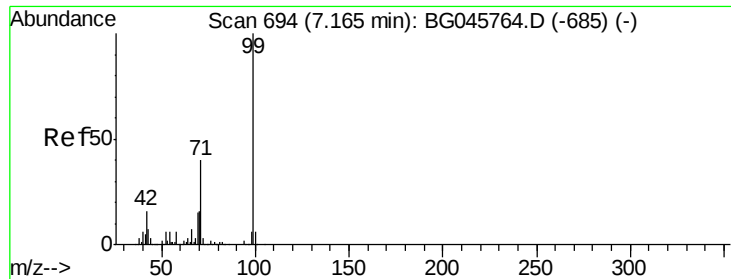

#7

Phenol-d6

Concen: 88.634 ng

RT: 7.14 min Scan# 689

Delta R.T. -0.03 min

Lab File: BG045853.D

Acq: 24 Jun 2020 20:36

Instrument :

BNA_G

ClientSampleId :

RB44767-RT


Tot Ion: 99 Resp: 414301

Ion Ratio Lower Upper




99 100

42 16.0 12.4 18.6

71 39.8 32.1 48.1

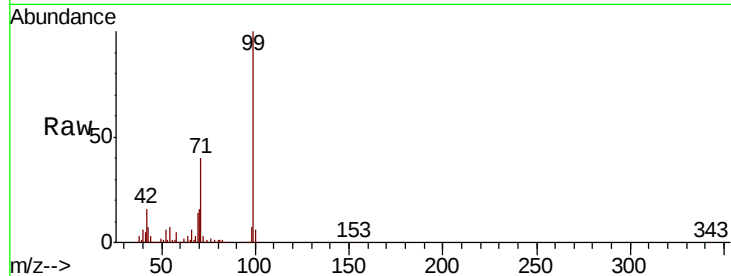

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

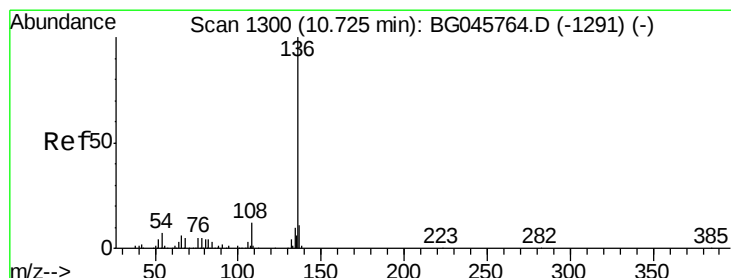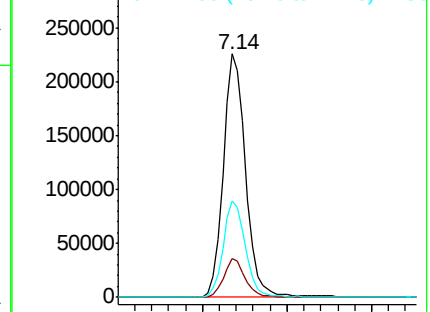

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.72 min Scan# 1300

Delta R.T. 0.00 min

Lab File: BG045853.D

Acq: 24 Jun 2020 20:36

Tgt Ion: 136 Resp: 205985


Ion Ratio Lower Upper

136 100



137 11.6 8.7 13.1


54 6.7 5.8 8.6

68 5.0 4.0 6.0

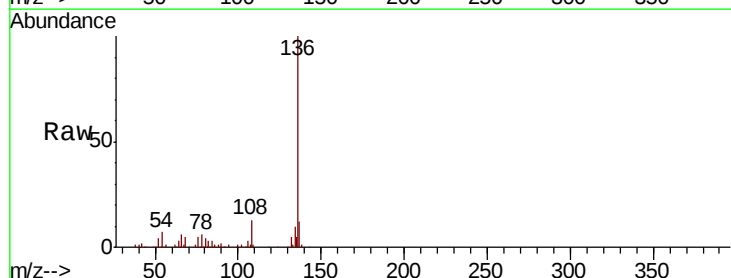

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




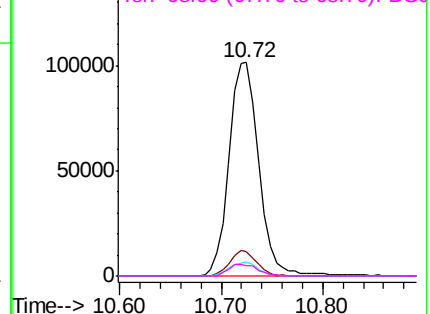




#23
 Nitrobenzene-d5
 Concen: 86.148 ng
 RT: 9.08 min Scan# 1020
 Delta R.T. -0.01 min
 Lab File: BG045853.D
 Acq: 24 Jun 2020 20:36




Instrument :
 BNA_G
 ClientSampled :
 RB44767-RT


Tot Ion	82	Resp	388437
Ion Ratio	100	Lower	Upper
128	41.4	32.5	48.7
54	40.3	31.2	46.8

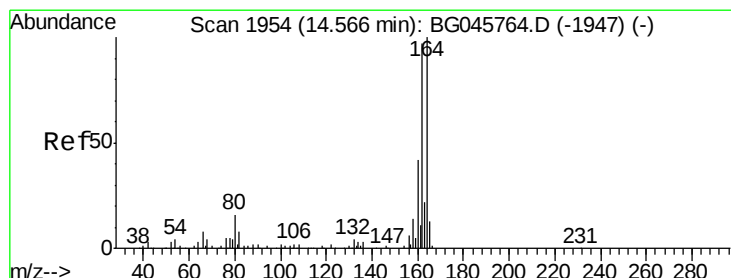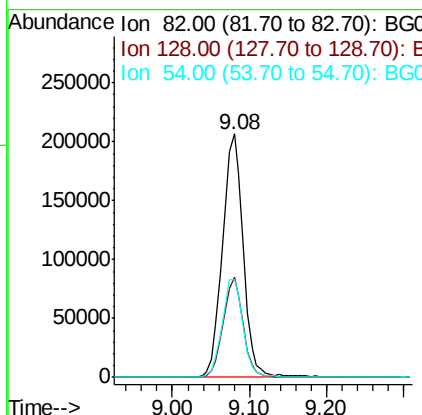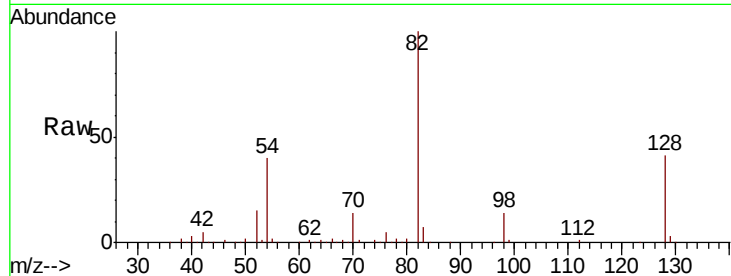

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.56 min Scan# 1953
 Delta R.T. -0.01 min
 Lab File: BG045853.D
 Acq: 24 Jun 2020 20:36

Tgt Ion	164	Resp	149123
Ion Ratio <td>100</td> <td>Lower</td> <td>Upper</td>	100	Lower	Upper
162	100.9	77.4	116.0
160	41.7	33.3	49.9

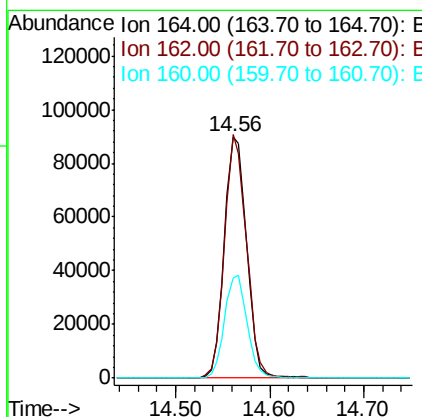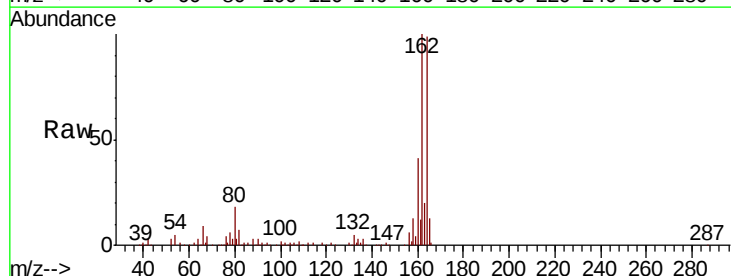


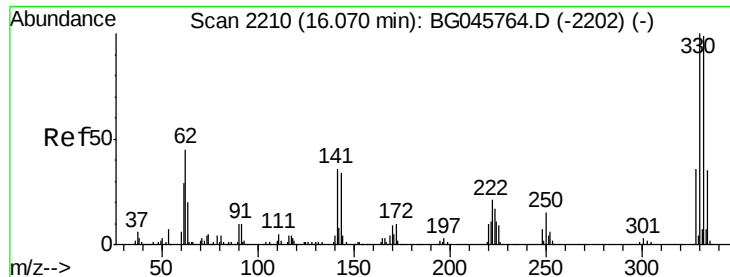

#42
 2,4,6-Tribromophenol
 Concen: 132.596 ng
 RT: 16.06 min Scan# 2209
 Delta R.T. -0.01 min
 Lab File: BG045853.D
 Acq: 24 Jun 2020 20:36

Instrument :
 BNA_G
 ClientSampleId :
 RB44767-RT

Tot Ion	Ratio	Lower	Upper
330	100		
332	99.1	78.6	117.8
141	34.8	28.2	42.4



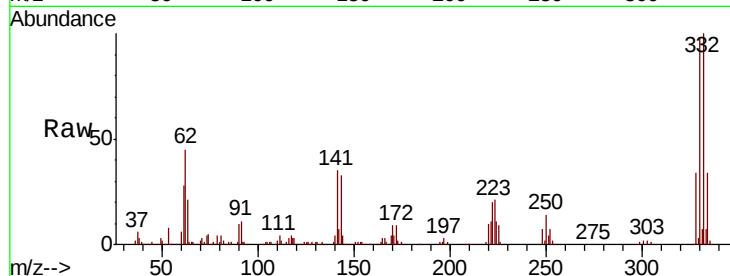


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

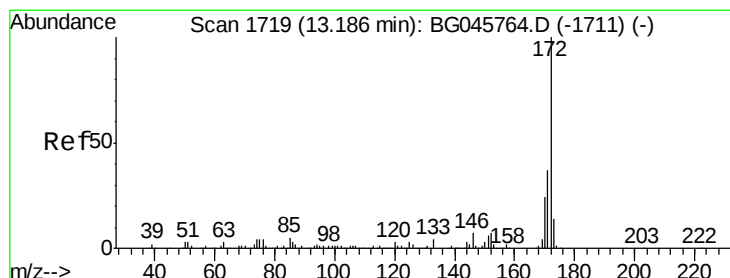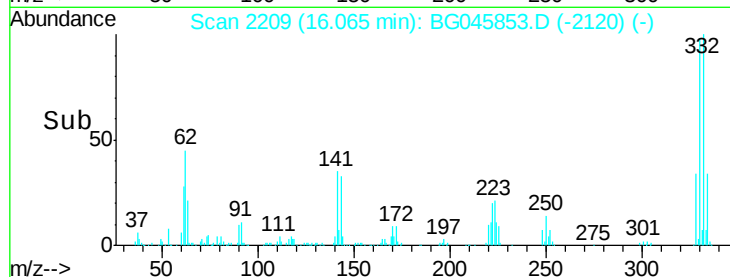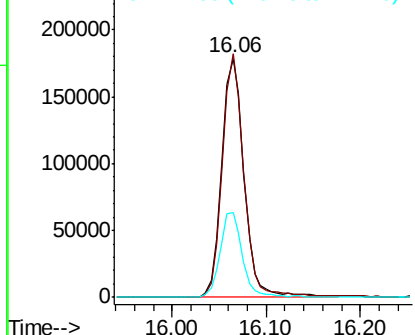

#45
 2-Fluorobiphenyl
 Concen: 89.332 ng
 RT: 13.19 min Scan# 1719
 Delta R.T. 0.00 min
 Lab File: BG045853.D
 Acq: 24 Jun 2020 20:36

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	29.9	44.9
170	23.8	19.3	28.9


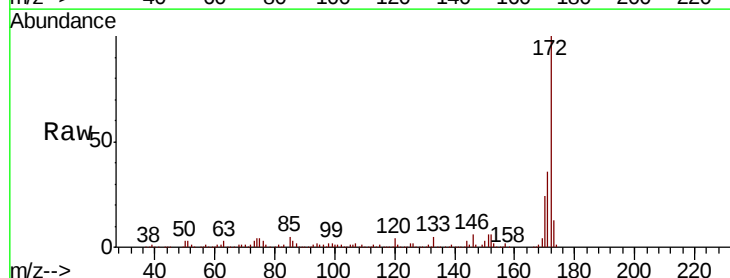



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

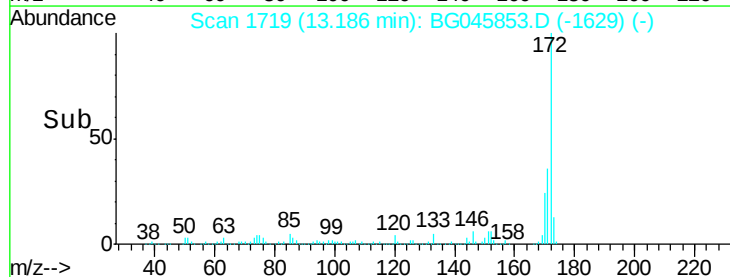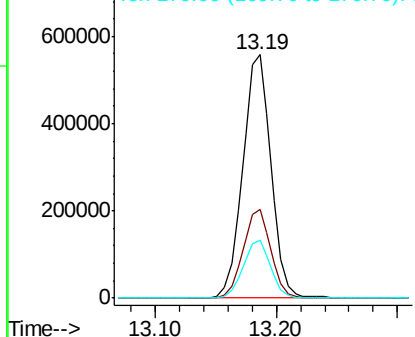

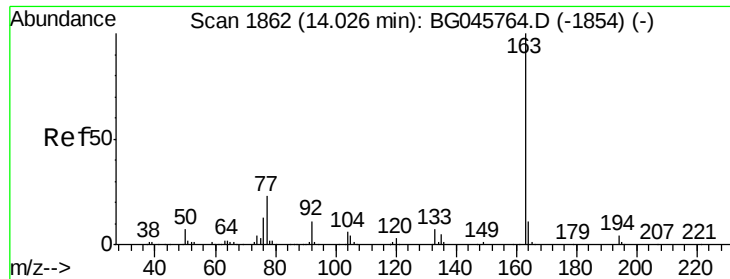

#50

Dimethylphthalate

Concen: 4.078 ng

RT: 14.02 min Scan# 1861

Delta R.T. -0.01 min

Lab File: BG045853.D

Acq: 24 Jun 2020 20:36

Instrument :

BNA_G

ClientSampleId :

RB44767-RT


Tot Ion:163 Resp: 47635

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0




164 8.9 8.9 13.3

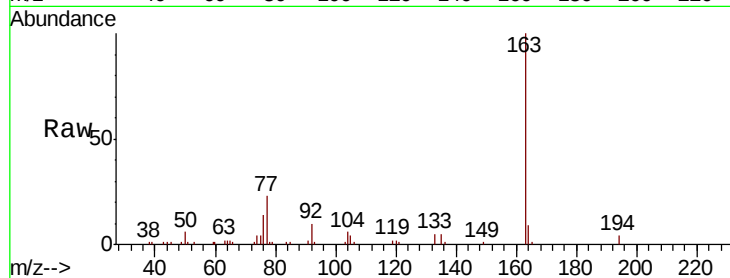

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

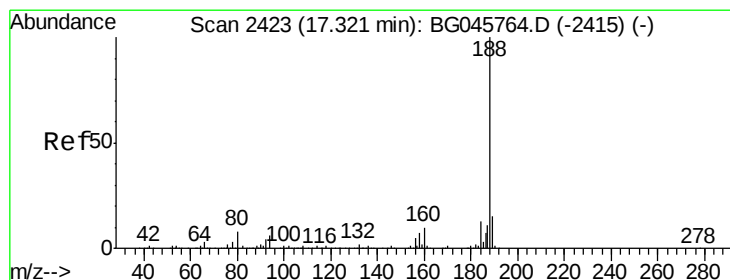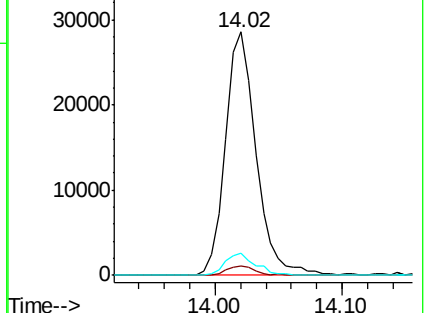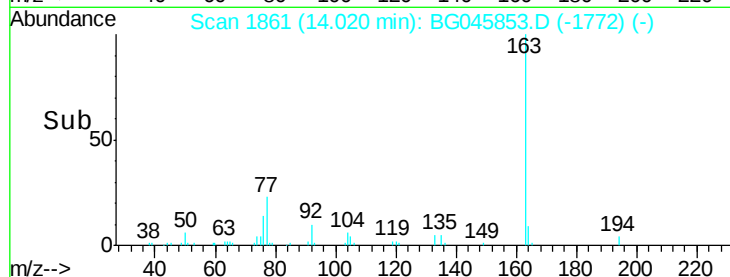

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.32 min Scan# 2422

Delta R.T. -0.01 min

Lab File: BG045853.D

Acq: 24 Jun 2020 20:36


Tgt Ion:188 Resp: 340716

Ion Ratio Lower Upper

188 100

94 6.0 5.1 7.7



80 7.4 6.2 9.4

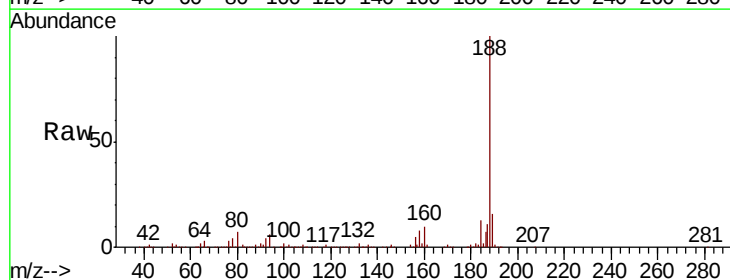


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

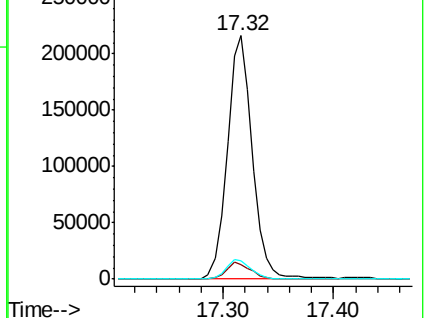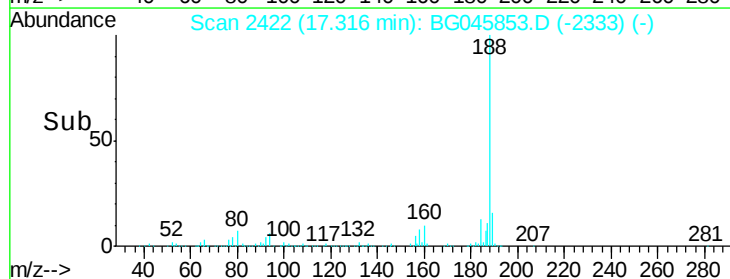



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.57 min Scan# 3147

Delta R.T. -0.01 min

Lab File: BG045853.D

Acq: 24 Jun 2020 20:36

Instrument :

BNA_G

ClientSampleId :

RB44767-RT


Tot Ion:240 Resp: 331889

Ion Ratio Lower Upper

240 100

120 5.4 5.0 7.4




236 25.6 20.6 30.8

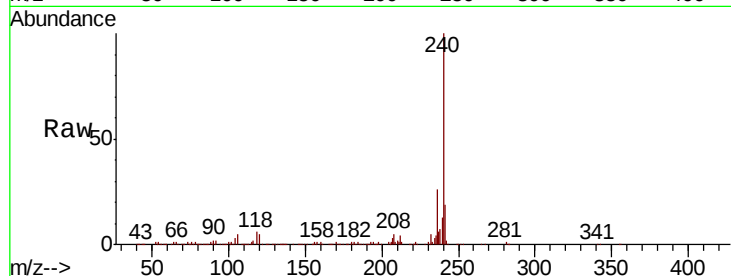

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

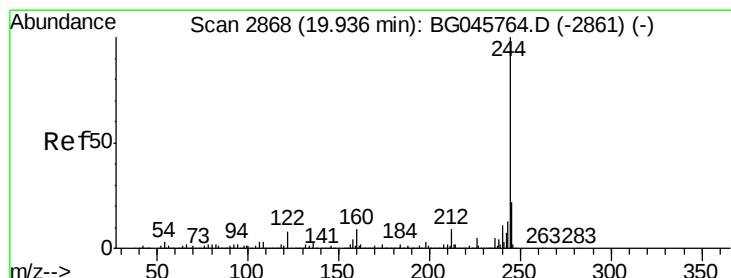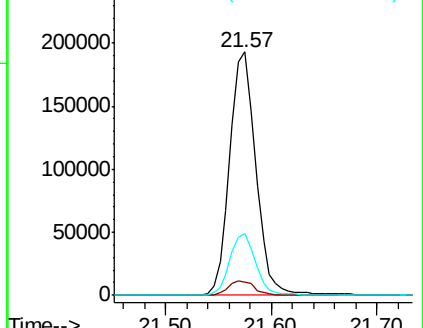

#79

Terphenyl-d14

Concen: 96.825 ng

RT: 19.94 min Scan# 2868

Delta R.T. 0.00 min

Lab File: BG045853.D

Acq: 24 Jun 2020 20:36


Tgt Ion:244 Resp: 1585680

Ion Ratio Lower Upper

244 100

212 8.8 7.2 10.8



122 8.3 6.4 9.6

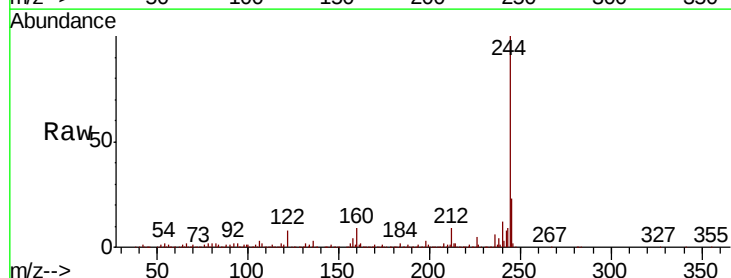


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

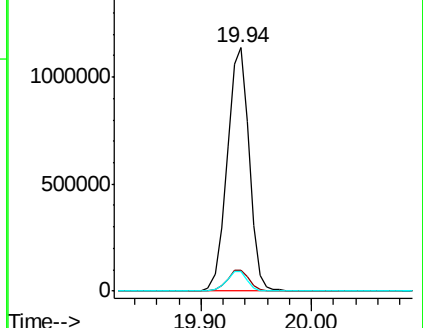

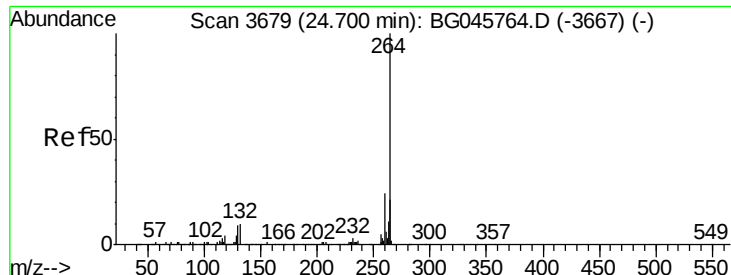

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.70 min Scan# 3679
Delta R.T. 0.00 min
Lab File: BG045853.D
Acq: 24 Jun 2020 20:36

Instrument :
BNA_G
ClientSampleId :
RB44767-RT

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.4	19.0	28.4
265	22.0	17.4	26.0

