
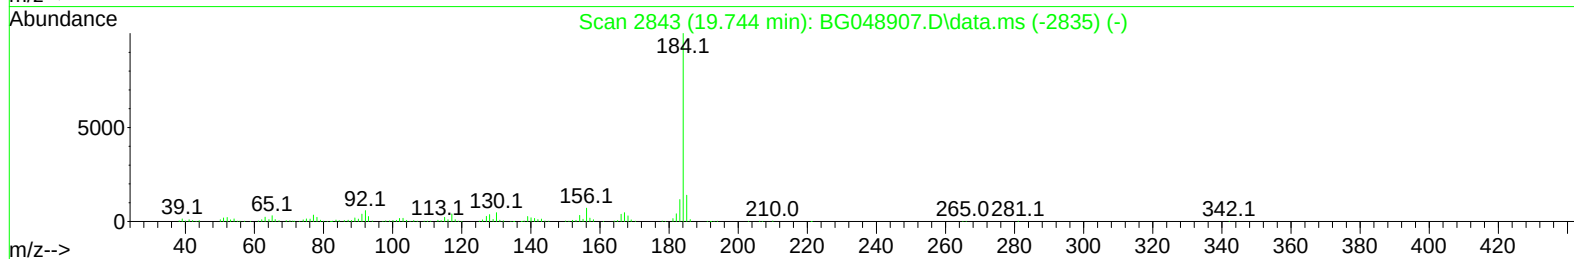
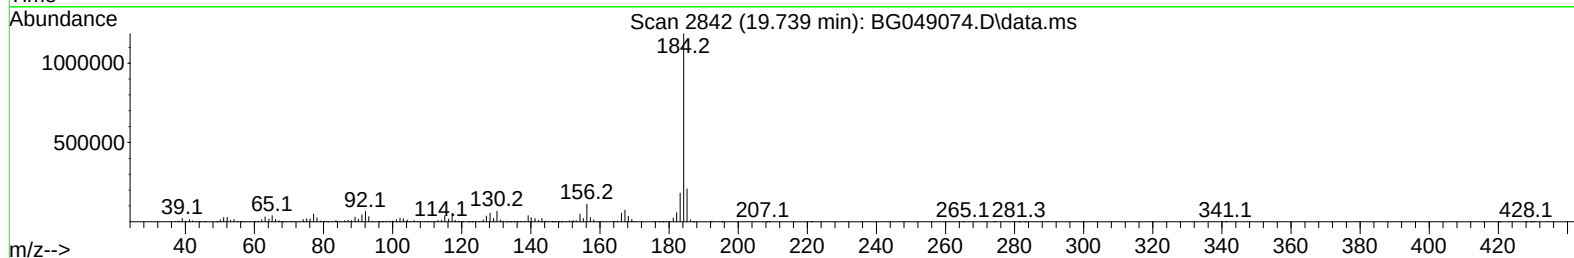


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062421\
Data File : BG049074.D
Acq On : 24 Jun 2021 9:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 10:57:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

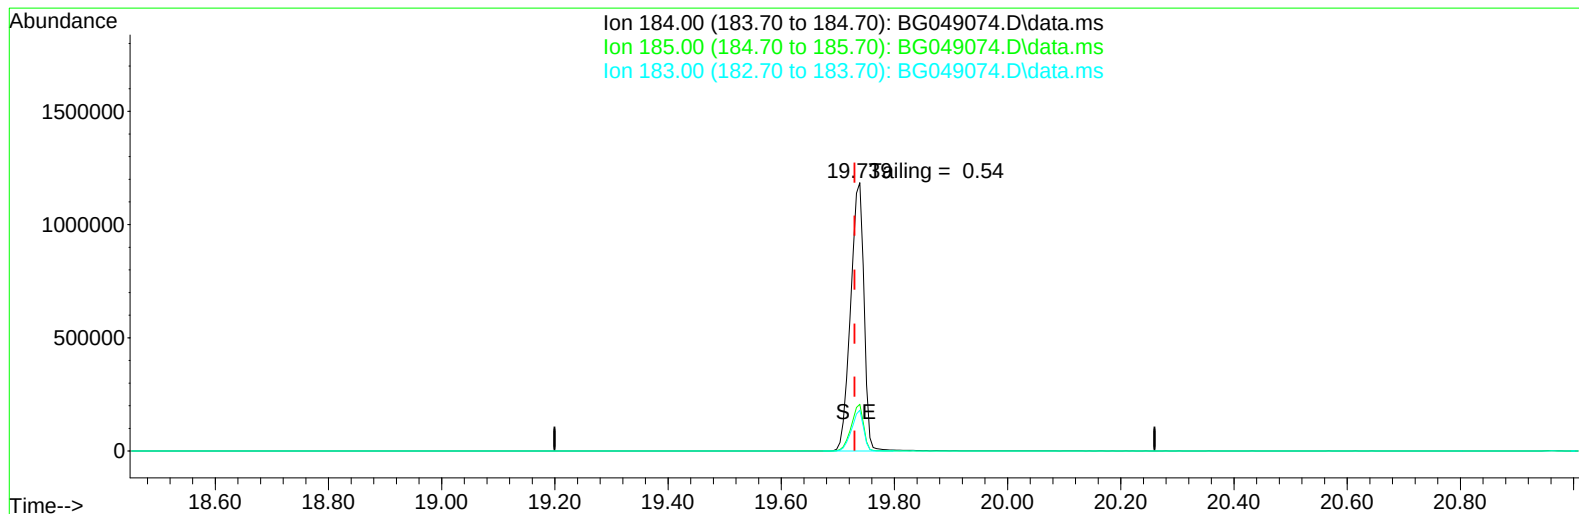




TIC: BG049074.D\data.ms

(77) Benzidine**19.739min (+ 0.010) 563676.62 ng****response 1953101**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	17.44#
183.00	11.70	15.22#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062421\
Data File : BG049074.D
Acq On : 24 Jun 2021 9:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 10:57:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

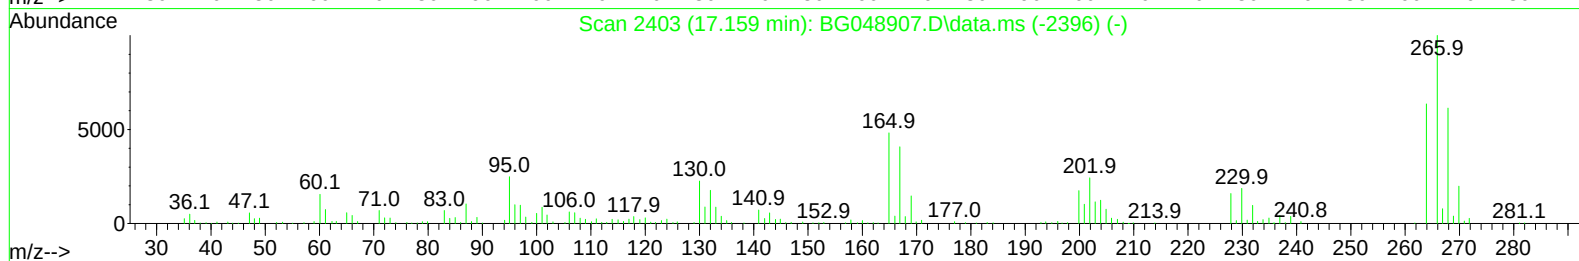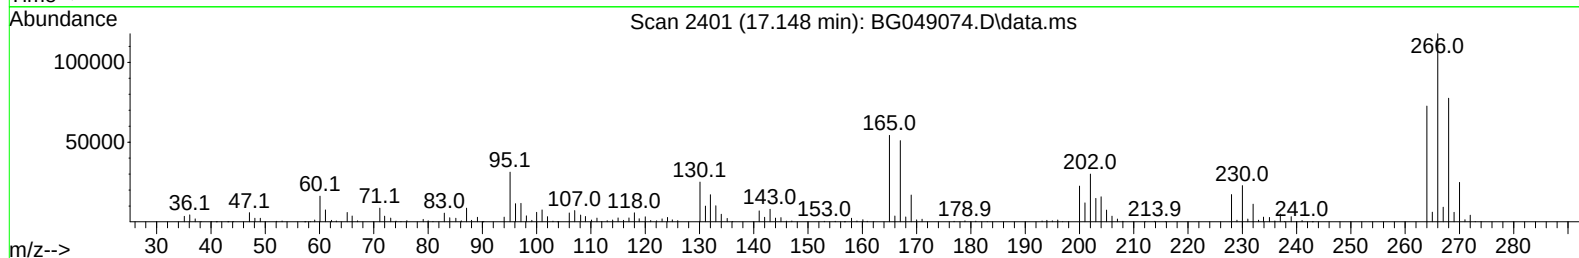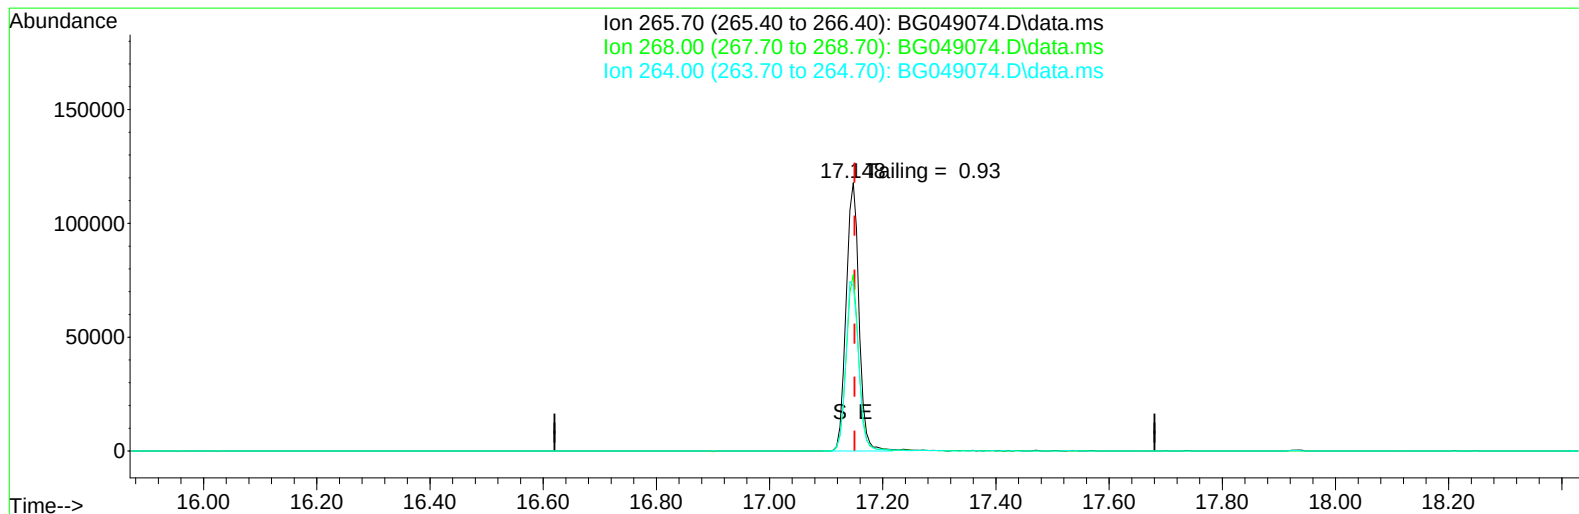

TIC: BG049074.D\data.ms

(70) Pentachlorophenol (C)

17.148min (-0.002) 0.00 ng

response 186491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	65.75
264.00	61.30	61.54
0.00	0.00	0.00