
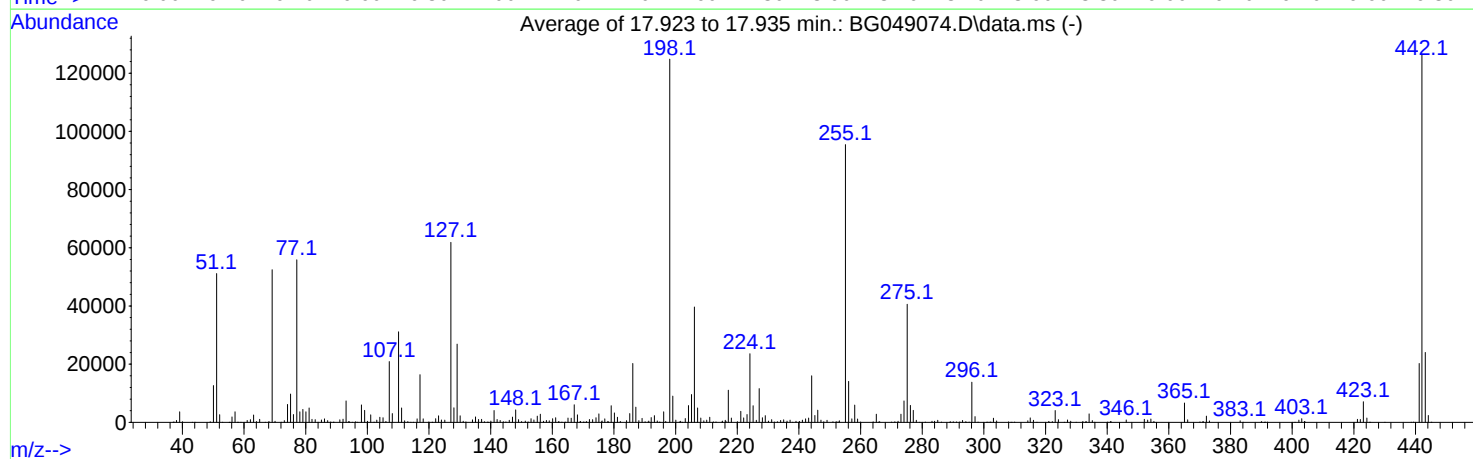


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062421\
 Data File : BG049074.D
 Acq On : 24 Jun 2021 9:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 24 11:02:36 2021

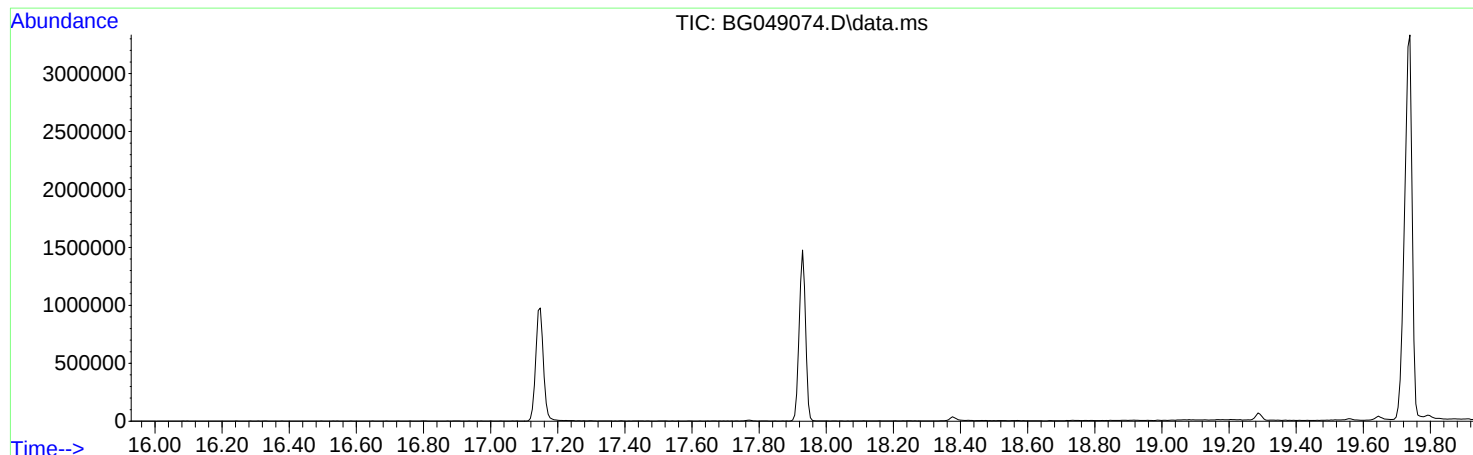




AutoFind: Scans 2533, 2534, 2535; Background Corrected with Scan 2526

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	51125	PASS
68	69	0.00	2	0.6	324	PASS
69	198	0.00	100	42.0	52485	PASS
70	69	0.00	2	0.7	375	PASS
127	198	10	80	49.6	61875	PASS
197	198	0.00	2	0.3	357	PASS
198	198	100	100	100.0	124824	PASS
199	198	5	9	7.2	8998	PASS
275	198	10	60	32.5	40579	PASS
365	198	1	100	5.3	6649	PASS
441	198	0.01	100	16.2	20233	PASS
442	442	100	100	100.0	126411	PASS
443	442	15	24	19.0	24013	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062421\
Data File : BG049074.D
Acq On : 24 Jun 2021 9:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 24 10:57:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

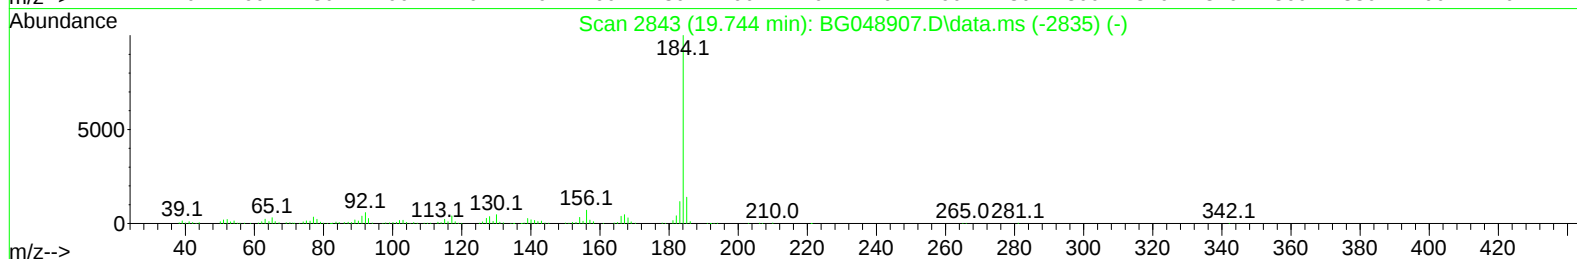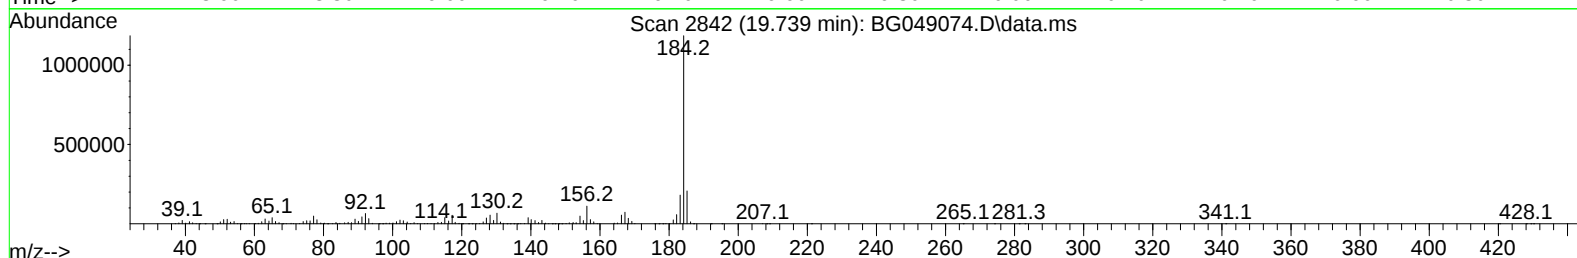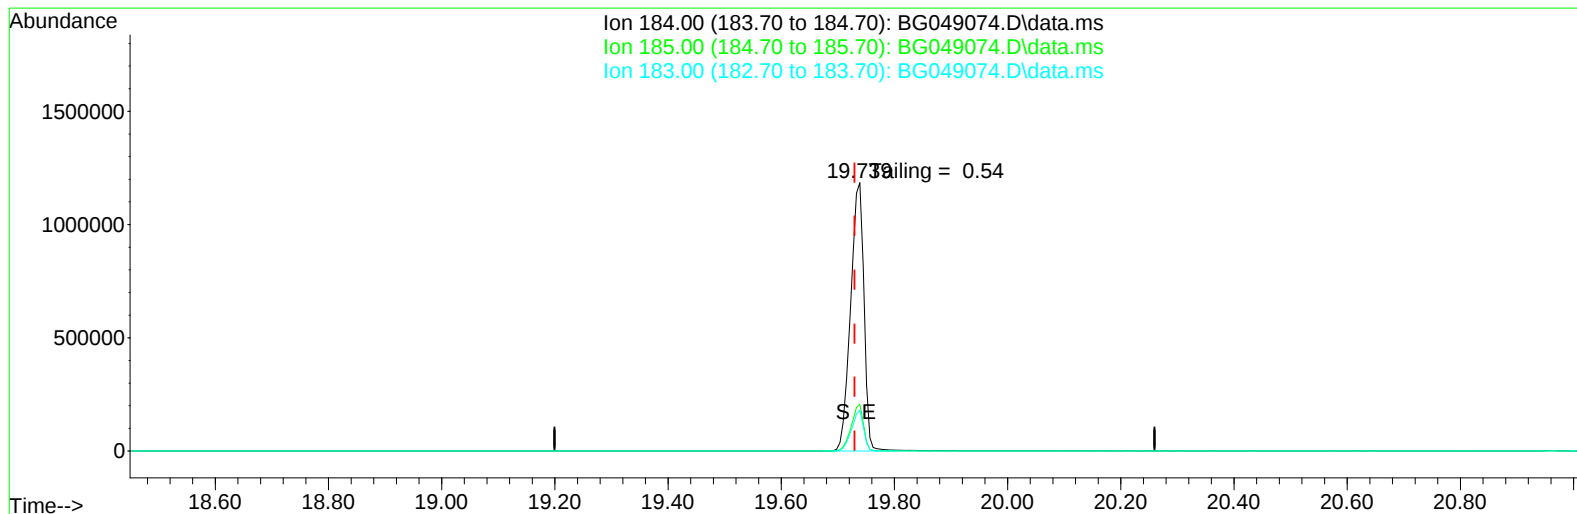

TIC: BG049074.D\data.ms

(77) Benzidine

19.739min (+ 0.010) 563676.62 ng




response 1953101

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	17.44#
183.00	11.70	15.22#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062421\
 Data File : BG049074.D
 Acq On : 24 Jun 2021 9:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 24 10:57:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 16 12:04:50 2021
 Response via : Initial Calibration

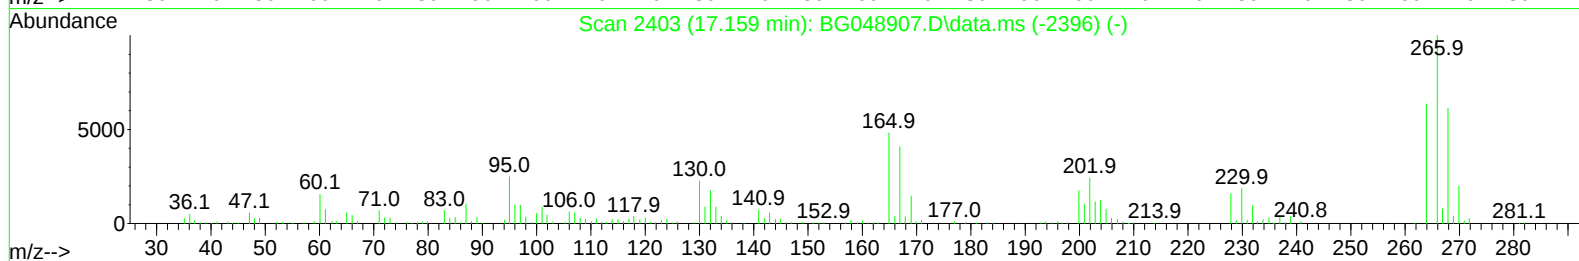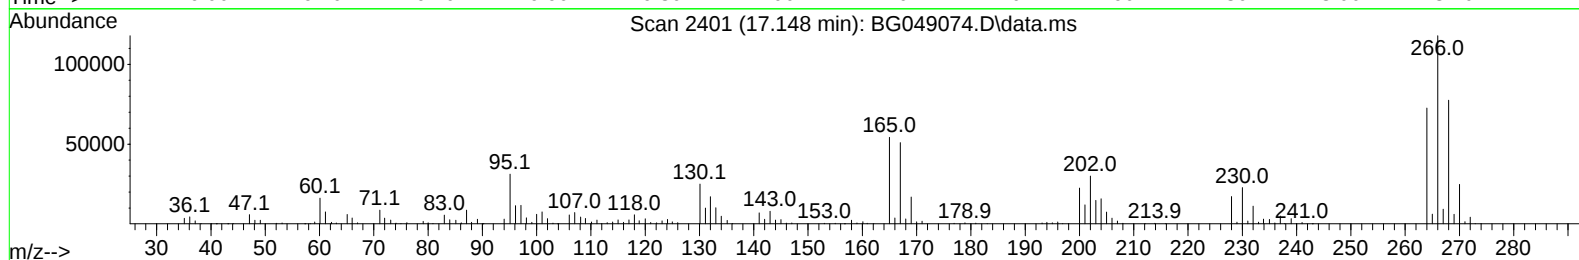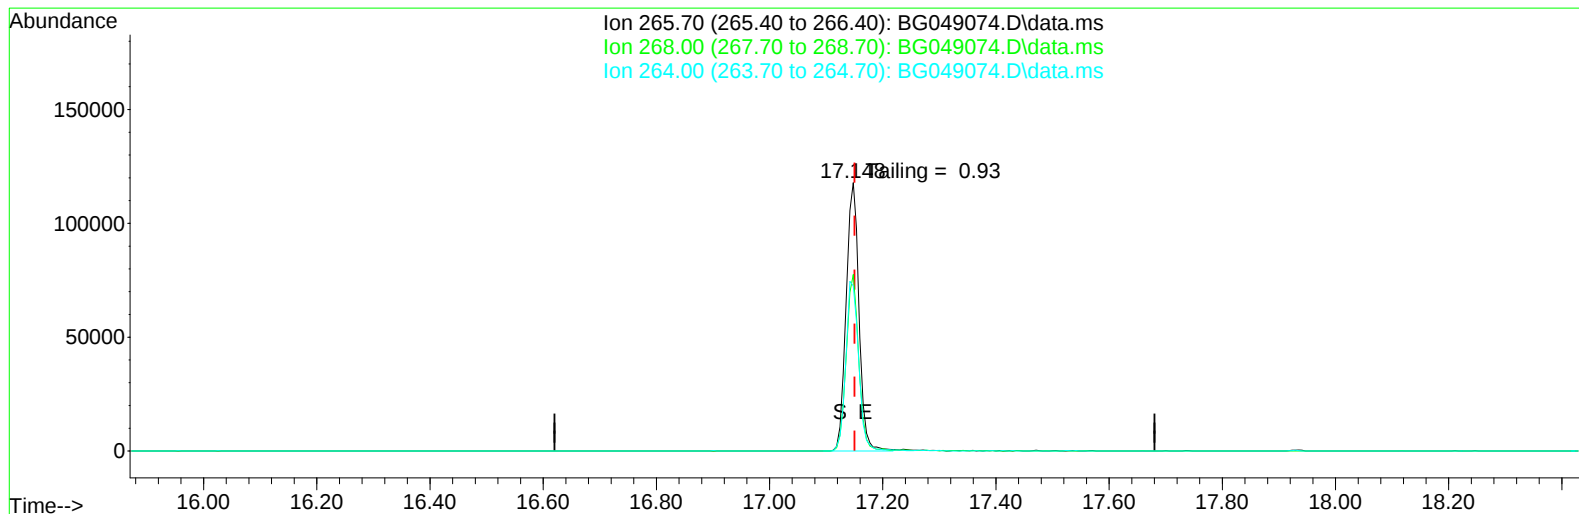

TIC: BG049074.D\data.ms

(70) Pentachlorophenol (C)

17.148min (-0.002) 0.00 ng

response 186491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	65.75
264.00	61.30	61.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/24/2021	BNA_G	BG049074.D
Compound Name	Response	Retention Time
DDT	326275	13.41
DDD	5513	13.11
DDE	455	12.77
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5968	332243	1.80