

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
 Data File : BG061708.D
 Acq On : 25 Jun 2024 18:37
 Operator : MA/JU
 Sample : P2873-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0SH7

Quant Time: Jun 25 23:07:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 05:03:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.077	152	53935	20.000	ng/ul	0.00
20) Naphthalene-d8	10.885	136	294079	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.698	164	227557	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.442	188	567683	20.000	ng/ul	0.00
79) Chrysene-d12	21.708	240	469105	20.000	ng/ul	0.00
88) Perylene-d12	24.933	264	562597	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.464	96	10198	6.830	ng/uL	0.00
4) Pyridine-d5	3.887	84	82472	18.270	ng/ul	0.00
7) Phenol-d5	7.213	99	227602	38.872	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.395	67	142335	38.996	ng/ul	0.00
11) 2-Chlorophenol-d4	7.601	132	156620	38.980	ng/ul	0.00
15) 4-Methylphenol-d8	8.770	113	188191	41.576	ng/ul	0.00
21) Nitrobenzene-d5	9.240	128	88628	44.385	ng/ul	0.00
24) 2-Nitrophenol-d4	9.957	143	104147	51.498	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.497	165	196797	41.096	ng/ul	0.00
31) 4-Chloroaniline-d4	11.014	131	235529	32.486	ng/ul	0.00
46) Dimethylphthalate-d6	14.105	166	728425	41.597	ng/ul	0.00
49) Acenaphthylene-d8	14.399	160	829020	43.198	ng/ul	0.00
54) 4-Nitrophenol-d4	14.875	143	121714	40.471	ng/ul	0.00
60) Fluorene-d10	15.691	176	684039	44.620	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.797	200	104523	43.059	ng/ul	0.00
73) Anthracene-d10	17.542	188	1081594	41.740	ng/ul	0.00
81) Pyrene-d10	19.822	212	1160266	44.279	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.716	264	1162603	43.267	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.764	70	6044	1.510 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
Data File : BG061708.D
Acq On : 25 Jun 2024 18:37
Operator : MA/JU
Sample : P2873-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0SH7


Quant Time: Jun 25 23:07:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

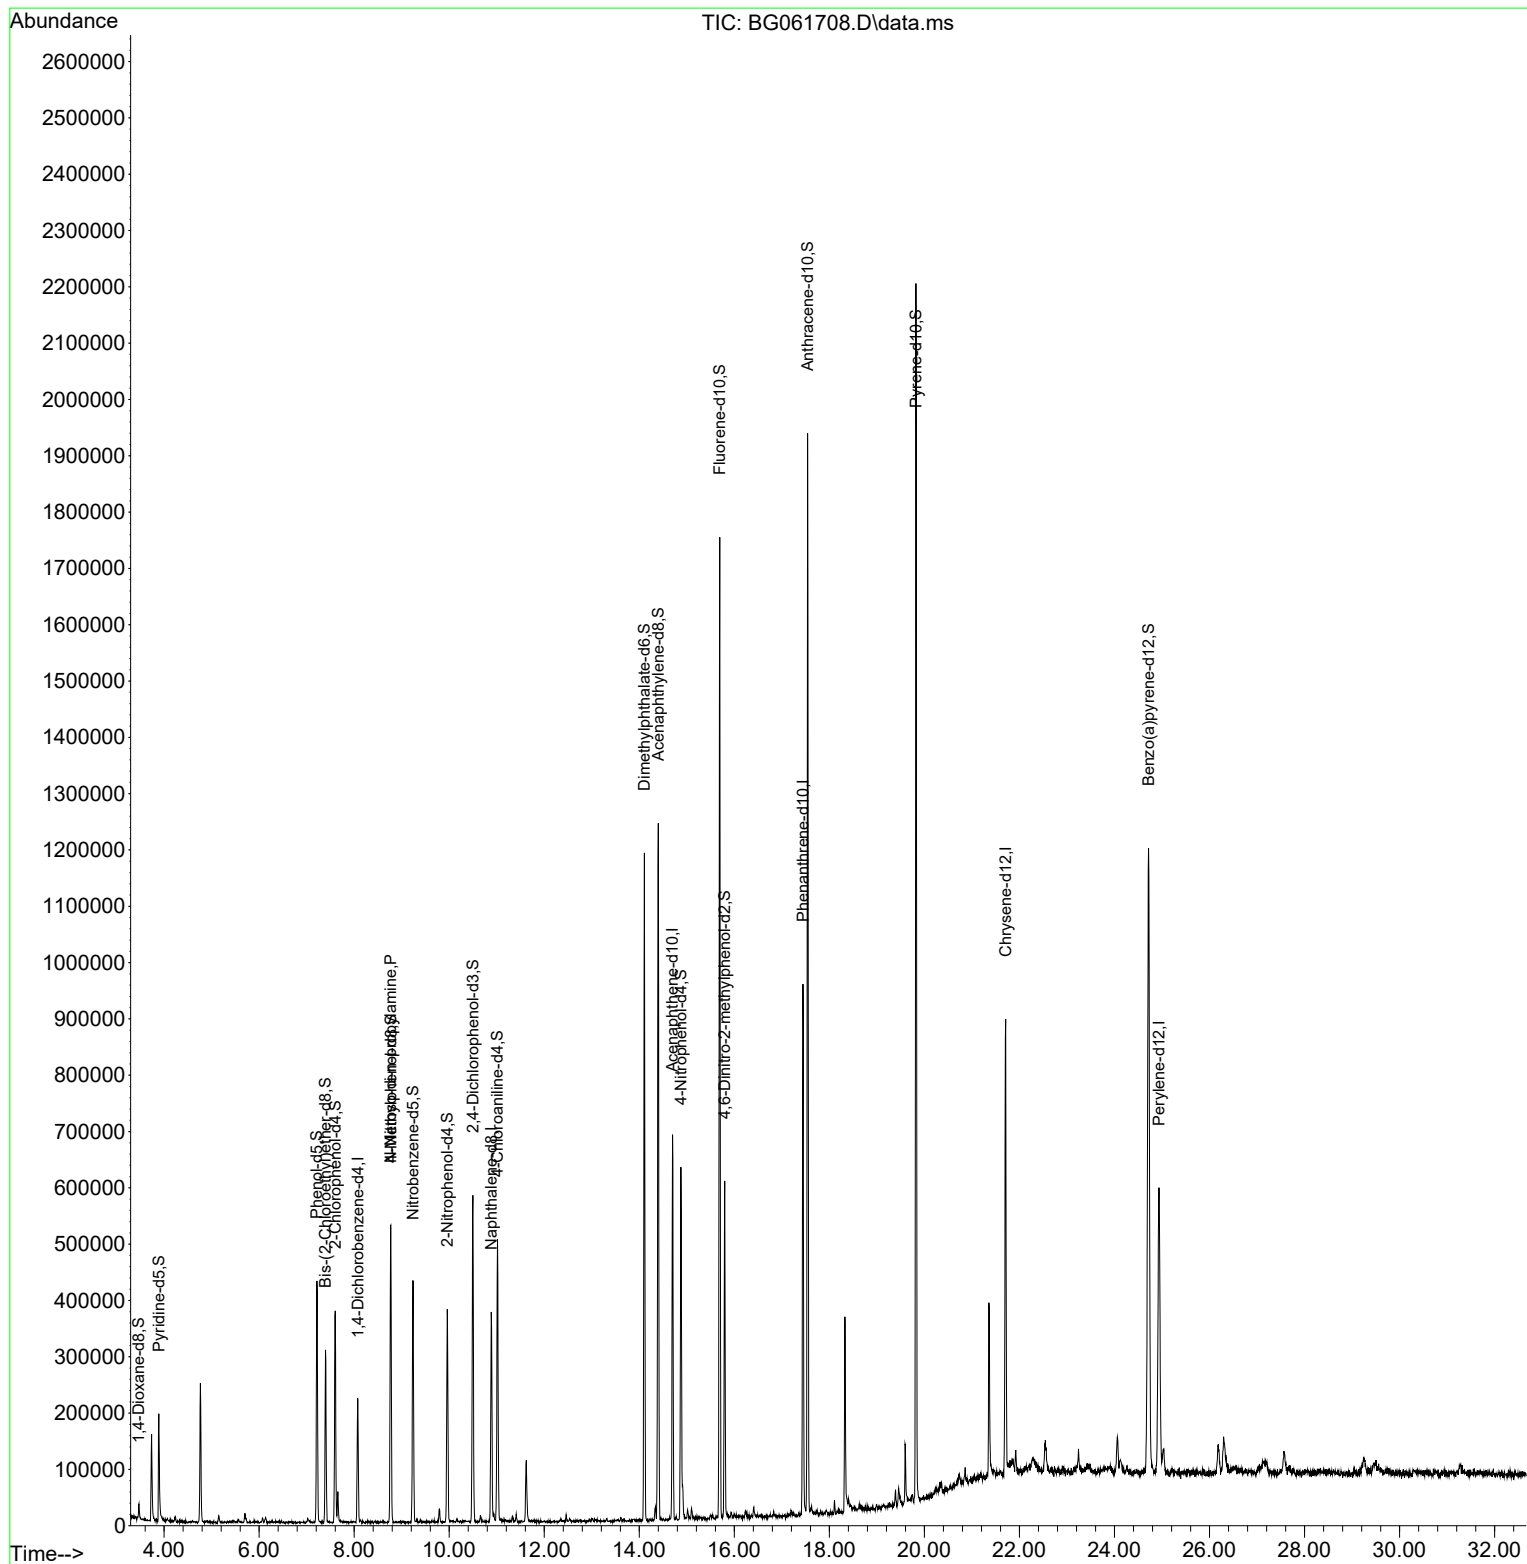

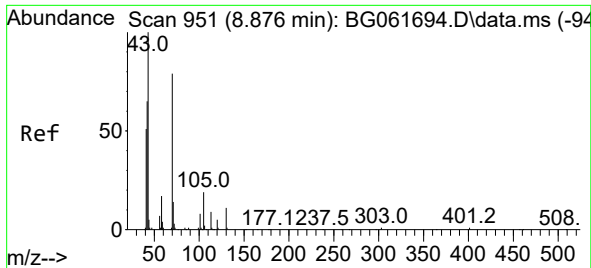

#17
N-Nitroso-di-n-propylamine
Concen: 1.510 ng/ul
RT: 8.764 min Scan# 91
Delta R.T. -0.117 min
Lab File: BG061708.D
Acq: 25 Jun 2024 18:37

Instrument :
BNA_G
ClientSampleId :
C0SH7

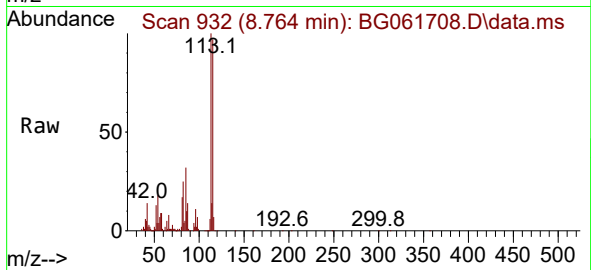

Tgt Ion: 70	Resp:	6044
Ion	Ratio	Lower Upper
70	100	
42	428.7	62.7 94.1#
101	0.0	5.8 8.8#
130	0.0	13.3 19.9#

