

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
 Data File : BG061716.D
 Acq On : 26 Jun 2024 00:05
 Operator : MA/JU
 Sample : P2873-16
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0SK4

Quant Time: Jun 26 01:08:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 05:03:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.070	152	46009	20.000	ng/u1	0.00
20) Naphthalene-d8	10.884	136	239783	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.698	164	191564	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.442	188	485107	20.000	ng/u1	0.00
79) Chrysene-d12	21.701	240	396246	20.000	ng/u1	-0.01
88) Perylene-d12	24.933	264	469291	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.464	96	7058	5.542	ng/uL	0.00
4) Pyridine-d5	3.887	84	98981	25.704	ng/u1	0.00
7) Phenol-d5	7.218	99	155345	31.102	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.394	67	105664	33.936	ng/u1	0.00
11) 2-Chlorophenol-d4	7.600	132	104852	30.591	ng/u1	0.00
15) 4-Methylphenol-d8	8.763	113	127640	33.057	ng/u1	0.00
21) Nitrobenzene-d5	9.239	128	57046	35.038	ng/u1	0.00
24) 2-Nitrophenol-d4	9.956	143	66947	40.599	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.491	165	129113	33.067	ng/u1	0.00
31) 4-Chloroaniline-d4	11.014	131	170671	28.871	ng/u1	0.00
46) Dimethylphthalate-d6	14.104	166	453781	30.782	ng/u1	0.00
49) Acenaphthylene-d8	14.392	160	519159	32.135	ng/u1	0.00
54) 4-Nitrophenol-d4	14.874	143	77961	30.793	ng/u1	0.00
60) Fluorene-d10	15.691	176	422683	32.752	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.796	200	59583	28.724	ng/u1	0.00
73) Anthracene-d10	17.541	188	686256	30.992	ng/u1	0.00
81) Pyrene-d10	19.821	212	740004	33.434	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.709	264	753824	33.632	ng/u1	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.601	149	16147	1.105	ng/u1#	Qvalue 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
Data File : BG061716.D
Acq On : 26 Jun 2024 00:05
Operator : MA/JU
Sample : P2873-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0SK4

Quant Time: Jun 26 01:08:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

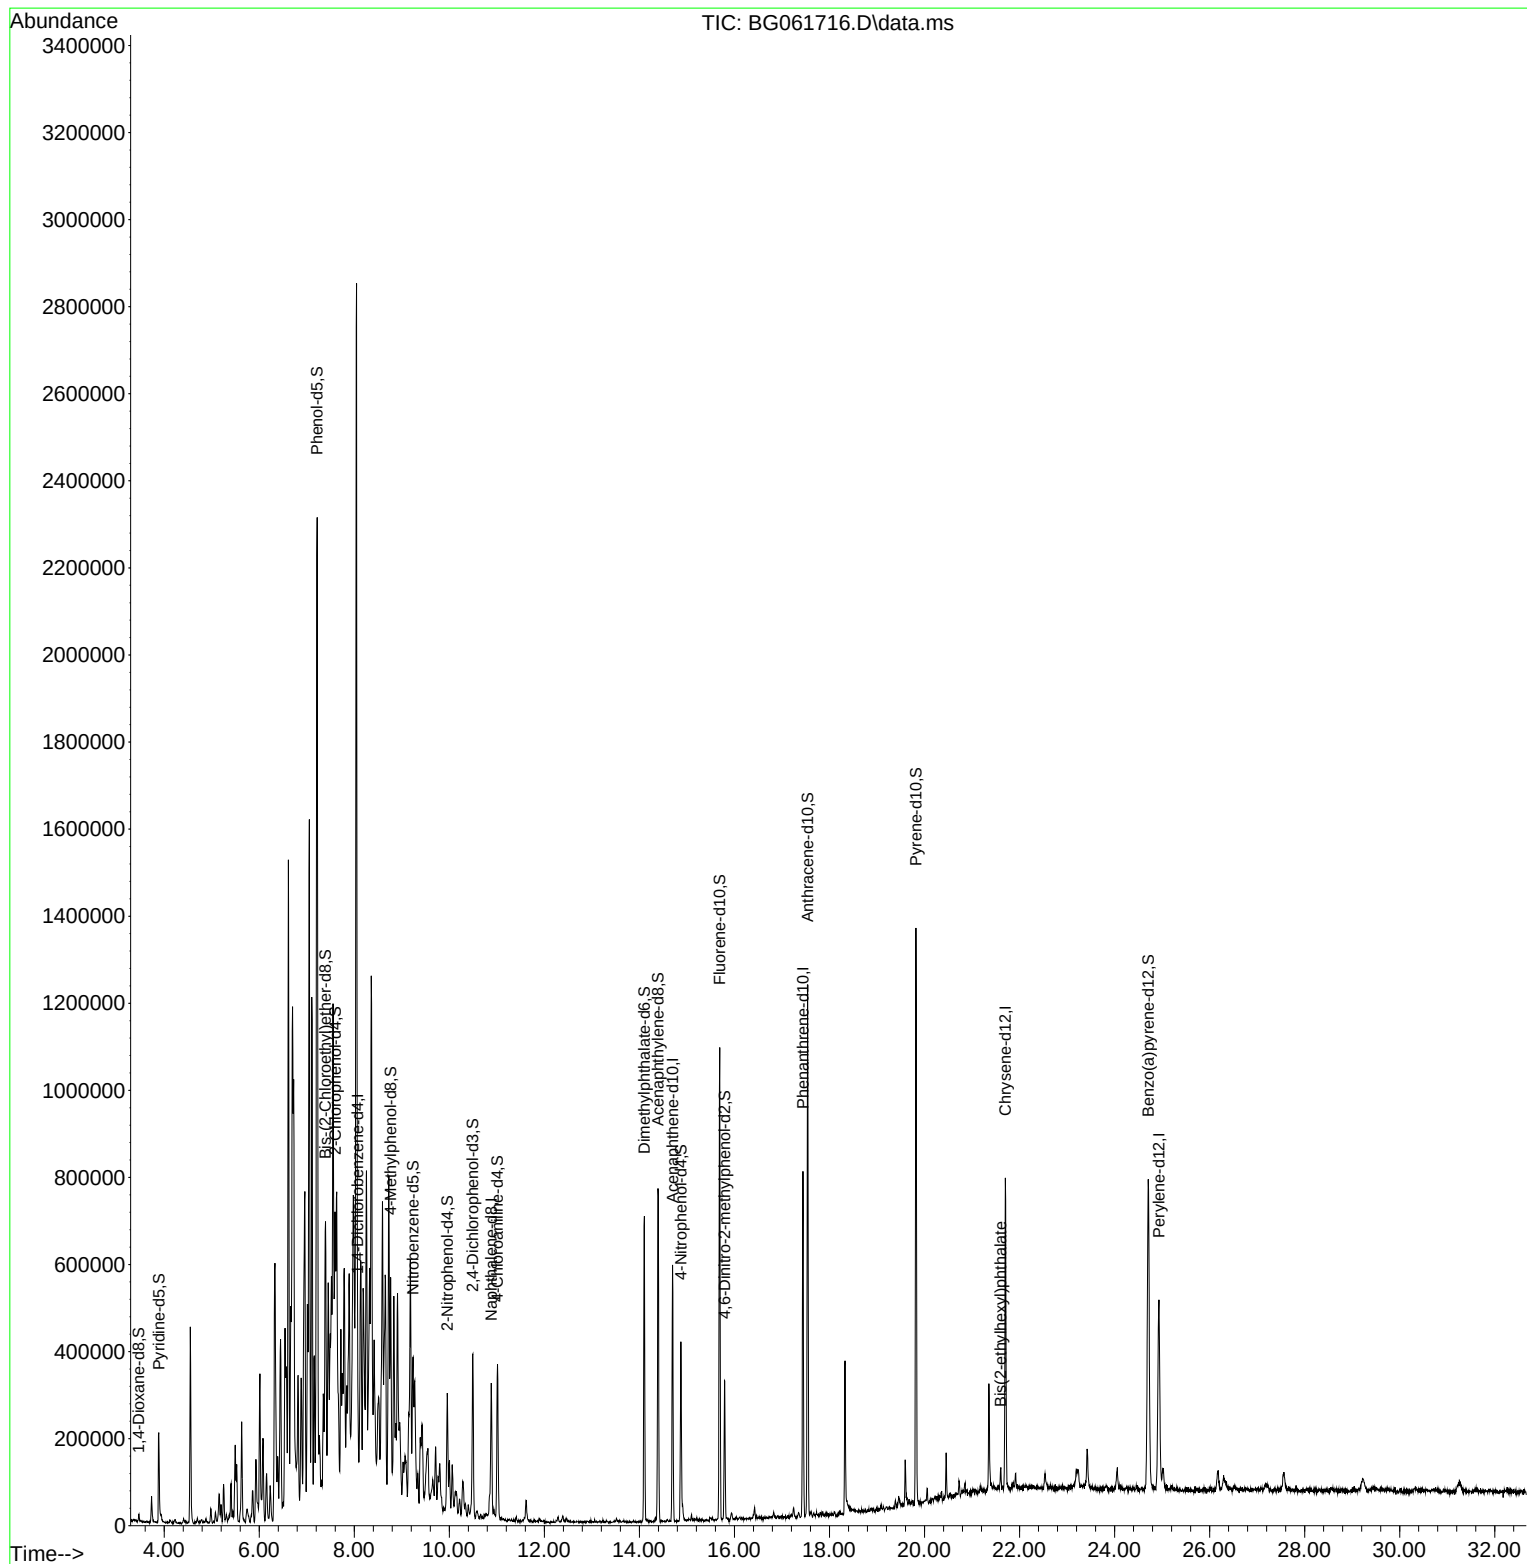

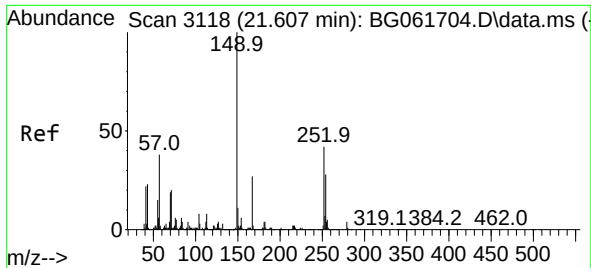

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.105 ng/ul
 RT: 21.601 min Scan# 3117
 Delta R.T. -0.024 min
 Lab File: BG061716.D
 Acq: 26 Jun 2024 00:05

Instrument :
 BNA_G
 ClientSampleId :
 C0SK4

Tgt Ion:149 Resp: 16147
 Ion Ratio Lower Upper
 149 100
 167 36.2 20.5 30.7#
 279 7.3 2.9 4.3#

