

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
 Data File : BG061669.D
 Acq On : 24 Jun 2024 10:18
 Operator : MA/JU
 Sample : PB161483BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK483

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.475	27	32	39	rVB4	21493	32803	1.37%	0.138%
2	3.657	61	63	66	rBV3	3068	3675	0.15%	0.015%
3	3.828	91	92	95	rVB2	3671	3584	0.15%	0.015%
4	3.887	99	102	118	rVV	254958	415108	17.29%	1.746%
5	4.069	131	133	137	rBV3	4426	5243	0.22%	0.022%
6	4.233	158	161	165	rVB4	7029	10401	0.43%	0.044%
7	5.085	304	306	308	rBV2	3899	3651	0.15%	0.015%
8	5.132	311	314	316	rVB	4554	4870	0.20%	0.020%
9	5.191	322	324	327	rBV4	3095	3782	0.16%	0.016%
10	5.297	339	342	344	rVB	3272	3630	0.15%	0.015%
11	5.667	401	405	408	rBV2	2932	3660	0.15%	0.015%
12	6.225	499	500	506	rBV2	2643	3730	0.16%	0.016%
13	6.301	510	513	515	rBV4	4521	6507	0.27%	0.027%
14	6.648	568	572	575	rBV2	3986	6962	0.29%	0.029%
15	7.077	641	645	648	rVB2	3483	5521	0.23%	0.023%
16	7.218	660	669	677	rBV	285151	486488	20.27%	2.046%
17	7.400	693	700	709	rVB	208097	342871	14.28%	1.442%
18	7.476	712	713	718	rVB3	3049	3435	0.14%	0.014%
19	7.518	718	720	723	rVB3	3446	3580	0.15%	0.015%
20	7.600	727	734	741	rBV	248358	422779	17.61%	1.778%
21	8.076	808	815	822	rVB	205917	348968	14.54%	1.468%
22	8.264	844	847	849	rBV2	3542	3835	0.16%	0.016%
23	8.346	858	861	862	rBV2	4016	4310	0.18%	0.018%
24	8.769	925	933	940	rVB	360121	610038	25.41%	2.566%
25	9.239	1006	1013	1021	rBV2	288830	501746	20.90%	2.110%
26	9.674	1086	1087	1090	rBV2	3153	3437	0.14%	0.014%
27	9.868	1115	1120	1123	rBV2	3730	6247	0.26%	0.026%
28	9.962	1129	1136	1143	rBV2	239996	423570	17.64%	1.782%
29	10.496	1220	1227	1237	rVB	357146	628523	26.18%	2.644%
30	10.632	1248	1250	1253	rVB	3944	3800	0.16%	0.016%
31	10.890	1286	1294	1303	rVB	343287	620427	25.84%	2.610%
32	11.019	1308	1316	1323	rVV	406652	722627	30.10%	3.039%
33	11.207	1346	1348	1351	rVB	3241	3444	0.14%	0.014%
34	11.266	1354	1358	1362	rVB3	2918	4407	0.18%	0.019%
35	11.630	1418	1420	1423	rBV2	4113	5346	0.22%	0.022%
36	12.018	1482	1486	1488	rVB2	2457	3552	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
 Data File : BG061669.D
 Acq On : 24 Jun 2024 10:18
 Operator : MA/JU
 Sample : PB161483BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK483

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	12.159	1506	1510	1513	rBV2	3364	4458	0.19%	0.019%
38	12.194	1514	1516	1520	rVB2	3899	3949	0.16%	0.017%
39	12.371	1542	1546	1553	rVB2	4113	8895	0.37%	0.037%
40	12.424	1553	1555	1558	rBV	3197	3948	0.16%	0.017%
41	12.471	1558	1563	1566	rBV3	8624	14193	0.59%	0.060%
42	12.535	1571	1574	1577	rBV	3143	4120	0.17%	0.017%
43	12.764	1611	1613	1617	rVB	3356	4182	0.17%	0.018%
44	12.847	1625	1627	1629	rBV	3368	3500	0.15%	0.015%
45	13.499	1735	1738	1739	rBV2	2786	3333	0.14%	0.014%
46	13.663	1763	1766	1767	rBV	4304	4360	0.18%	0.018%
47	14.110	1834	1842	1848	rBV	867507	1219752	50.81%	5.130%
48	14.398	1885	1891	1900	rVB	850018	1342804	55.94%	5.648%
49	14.462	1900	1902	1905	rBV2	2888	3693	0.15%	0.016%
50	14.703	1937	1943	1950	rVV	686100	1047328	43.63%	4.405%
51	14.774	1953	1955	1957	rVB2	6808	5264	0.22%	0.022%
52	14.874	1966	1972	1981	rBV	476850	752039	31.33%	3.163%
53	15.520	2081	2082	2086	rBV2	4001	4404	0.18%	0.019%
54	15.579	2090	2092	2095	rVB3	4895	3968	0.17%	0.017%
55	15.696	2104	2112	2117	rBV	1184160	1790311	74.58%	7.530%
56	15.796	2123	2129	2137	rVB	404450	594142	24.75%	2.499%
57	15.990	2158	2162	2165	rVB3	3215	3610	0.15%	0.015%
58	16.072	2174	2176	2180	rBV2	3161	3409	0.14%	0.014%
59	16.249	2204	2206	2207	rBV	5026	3391	0.14%	0.014%
60	16.554	2257	2258	2261	rBV3	4912	3867	0.16%	0.016%
61	16.736	2285	2289	2290	rBV2	4560	6237	0.26%	0.026%
62	16.865	2309	2311	2316	rVB3	3392	4125	0.17%	0.017%
63	16.924	2319	2321	2324	rBV	5357	6770	0.28%	0.028%
64	17.242	2374	2375	2379	rVB2	5836	3376	0.14%	0.014%
65	17.447	2403	2410	2416	rBV	967899	1476869	61.52%	6.212%
66	17.547	2420	2427	2434	rVV2	1416616	2098299	87.41%	8.826%
67	17.806	2468	2471	2473	rBV3	4936	5183	0.22%	0.022%
68	17.841	2475	2477	2480	rVV2	3914	3636	0.15%	0.015%
69	17.864	2480	2481	2483	rVB2	9182	3709	0.15%	0.016%
70	17.894	2483	2486	2489	rBV	5461	7520	0.31%	0.032%
71	18.105	2520	2522	2523	rBV2	7001	4325	0.18%	0.018%
72	18.387	2568	2570	2572	rBV3	5838	4430	0.18%	0.019%
73	19.392	2738	2741	2746	rVB4	27132	38113	1.59%	0.160%
74	19.827	2809	2815	2825	rBV	1699784	2400619	100.00%	10.097%
75	21.713	3129	3136	3141	rBV2	869400	1463836	60.98%	6.157%
76	24.721	3639	3648	3659	rVB3	800285	2234323	93.07%	9.398%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
Data File : BG061669.D
Acq On : 24 Jun 2024 10:18
Operator : MA/JU
Sample : PB161483BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK483

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Title : SVOA CALIBRATION

77	24.944	3677	3686	3696	rVB2	535142	1513751	63.06%	6.367%
----	--------	------	------	------	------	--------	---------	--------	--------




Sum of corrected areas: 23774598

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
Data File : BG061669.D
Acq On : 24 Jun 2024 10:18
Operator : MA/JU
Sample : PB161483BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK483

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

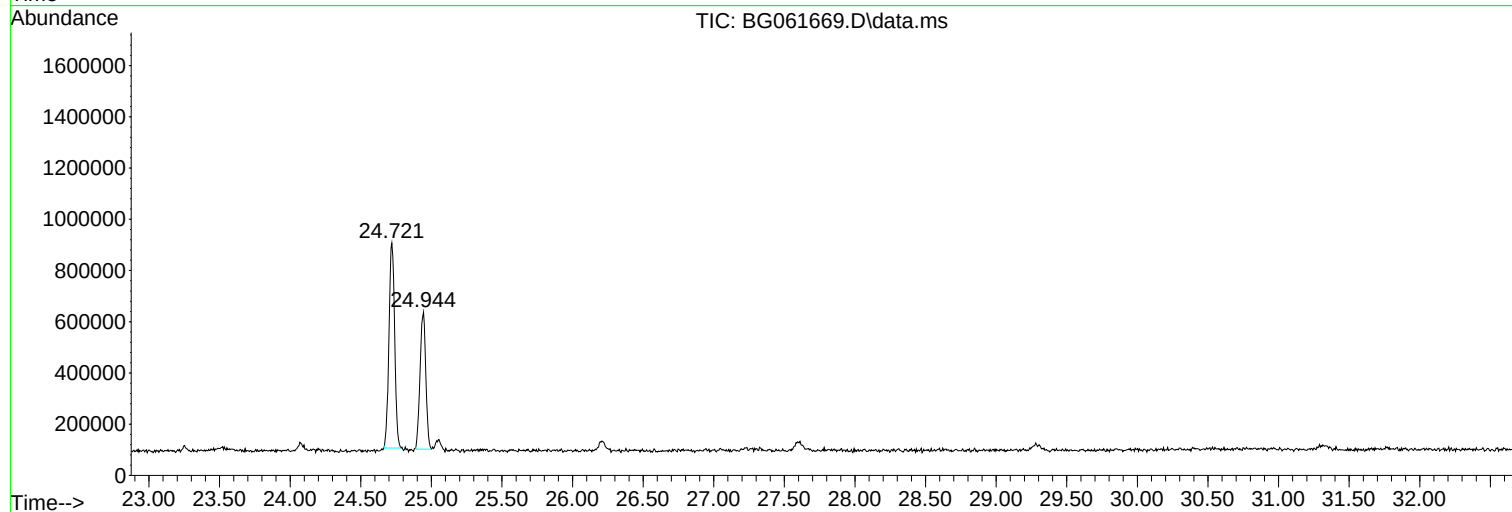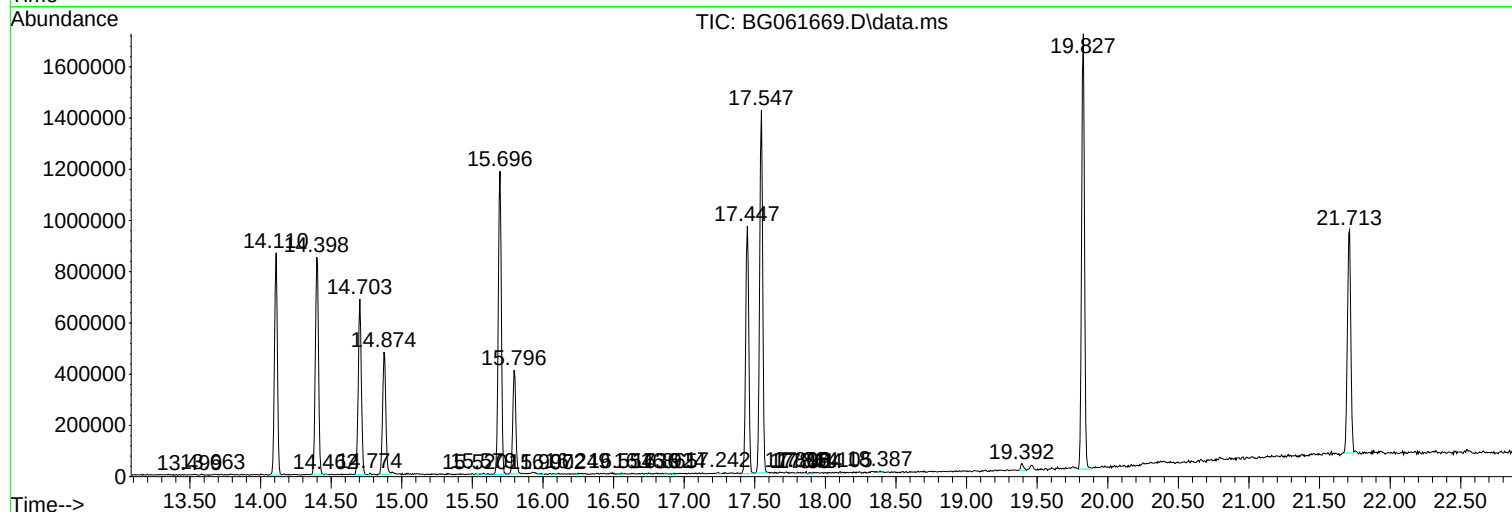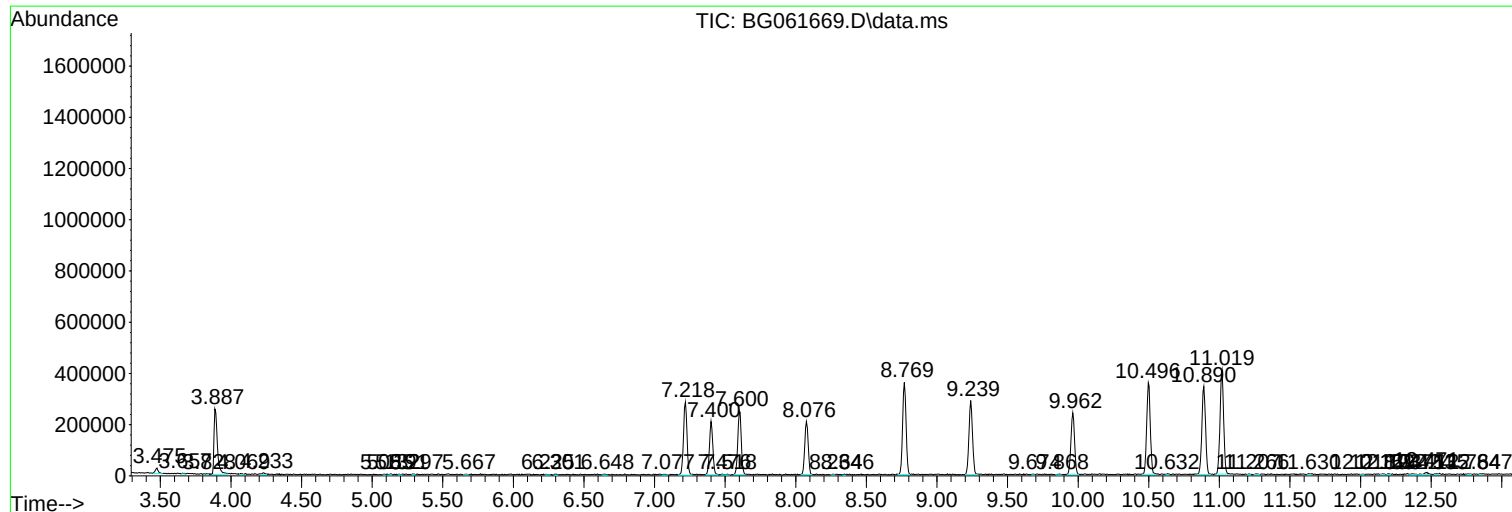

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
Data File : BG061669.D
Acq On : 24 Jun 2024 10:18
Operator : MA/JU
Sample : PB161483BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK483

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
Data File : BG061669.D
Acq On : 24 Jun 2024 10:18
Operator : MA/JU
Sample : PB161483BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK483

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------