

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
 Data File : BG061679.D
 Acq On : 24 Jun 2024 17:34
 Operator : MA/JU
 Sample : PB161484BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK484

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061679.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.470	27	31	38	rBV2	23811	37321	1.64%	0.165%
2	3.828	90	92	94	rVB2	4312	3707	0.16%	0.016%
3	3.863	94	98	99	rVV2	3913	4571	0.20%	0.020%
4	3.887	99	102	116	rVV	310225	499202	22.00%	2.211%
5	3.998	119	121	124	rVB3	5358	5002	0.22%	0.022%
6	4.034	124	127	134	rBV6	5919	10336	0.46%	0.046%
7	4.233	157	161	163	rBV2	4646	7095	0.31%	0.031%
8	4.392	185	188	189	rVB2	4075	3287	0.14%	0.015%
9	5.074	300	304	306	rBV3	2403	3371	0.15%	0.015%
10	5.250	329	334	335	rBV4	3915	4828	0.21%	0.021%
11	5.461	368	370	372	rVB2	4139	3494	0.15%	0.015%
12	5.497	372	376	379	rBV3	3969	7000	0.31%	0.031%
13	5.738	416	417	422	rVB3	3018	3868	0.17%	0.017%
14	5.790	422	426	427	rBV3	3814	3257	0.14%	0.014%
15	5.943	448	452	453	rBV2	2770	3294	0.15%	0.015%
16	6.002	459	462	464	rBV2	2828	3647	0.16%	0.016%
17	6.137	484	485	487	rBV2	4596	3774	0.17%	0.017%
18	6.266	505	507	510	rVB4	3858	4622	0.20%	0.020%
19	7.030	634	637	638	rBV	3525	4078	0.18%	0.018%
20	7.136	653	655	659	rBV3	2411	3238	0.14%	0.014%
21	7.218	662	669	678	rVB	340994	571733	25.20%	2.532%
22	7.400	692	700	708	rVB	234123	385716	17.00%	1.708%
23	7.600	726	734	741	rBV	300484	506903	22.34%	2.245%
24	7.659	743	744	748	rVB3	4428	4003	0.18%	0.018%
25	7.688	748	749	753	rBV2	3989	4042	0.18%	0.018%
26	7.776	760	764	765	rVB4	3646	3517	0.15%	0.016%
27	7.982	794	799	800	rVB3	3271	3833	0.17%	0.017%
28	8.011	800	804	805	rBV	3591	3317	0.15%	0.015%
29	8.076	807	815	821	rVV2	222219	353808	15.59%	1.567%
30	8.669	912	916	920	rVB2	4382	7796	0.34%	0.035%
31	8.769	925	933	942	rVV2	399725	685618	30.21%	3.037%
32	9.028	974	977	980	rVB3	2475	3431	0.15%	0.015%
33	9.057	980	982	985	rBV2	3378	4041	0.18%	0.018%
34	9.104	987	990	992	rVB	3554	3658	0.16%	0.016%
35	9.239	1005	1013	1020	rBV	306717	543174	23.94%	2.406%
36	9.322	1024	1027	1029	rBV2	2110	3111	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
 Data File : BG061679.D
 Acq On : 24 Jun 2024 17:34
 Operator : MA/JU
 Sample : PB161484BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK484

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	9.416	1041	1043	1045	rVB3	4116	3400	0.15%	0.015%
38	9.439	1045	1047	1048	rBV	3395	3161	0.14%	0.014%
39	9.527	1060	1062	1065	rBV2	3264	3382	0.15%	0.015%
40	9.604	1073	1075	1079	rVB2	2986	3731	0.16%	0.017%
41	9.639	1079	1081	1085	rBV4	2721	3808	0.17%	0.017%
42	9.962	1128	1136	1144	rBV	267071	472994	20.84%	2.095%
43	10.156	1166	1169	1170	rBV3	3558	3307	0.15%	0.015%
44	10.185	1173	1174	1176	rBV2	4799	3180	0.14%	0.014%
45	10.285	1188	1191	1192	rBV2	3011	3418	0.15%	0.015%
46	10.497	1218	1227	1235	rBV2	402755	702315	30.95%	3.111%
47	10.890	1287	1294	1301	rBV2	310005	561325	24.74%	2.486%
48	10.955	1301	1305	1306	rVB2	4836	3782	0.17%	0.017%
49	11.020	1308	1316	1324	rBV	411193	753002	33.18%	3.335%
50	11.648	1421	1423	1424	rBV2	5208	3864	0.17%	0.017%
51	11.924	1468	1470	1474	rBV3	2959	3256	0.14%	0.014%
52	12.206	1514	1518	1520	rBV2	2871	3429	0.15%	0.015%
53	12.471	1556	1563	1565	rBV3	9414	13809	0.61%	0.061%
54	12.530	1570	1573	1574	rBV2	4276	3310	0.15%	0.015%
55	12.588	1580	1583	1586	rBV2	2457	3490	0.15%	0.015%
56	12.900	1633	1636	1639	rBV	3824	6454	0.28%	0.029%
57	13.053	1660	1662	1664	rBV	3317	3256	0.14%	0.014%
58	13.376	1715	1717	1719	rBV2	3339	3394	0.15%	0.015%
59	13.446	1724	1729	1732	rBV3	4485	9042	0.40%	0.040%
60	13.523	1740	1742	1745	rVB	3497	3514	0.15%	0.016%
61	13.558	1745	1748	1750	rVB	4057	4223	0.19%	0.019%
62	13.681	1765	1769	1772	rVB3	4548	6428	0.28%	0.028%
63	13.763	1781	1783	1787	rBV3	2849	4136	0.18%	0.018%
64	13.799	1787	1789	1792	rVB3	3024	3402	0.15%	0.015%
65	14.110	1835	1842	1848	rVB	733321	1070169	47.16%	4.740%
66	14.398	1884	1891	1900	rVB2	814607	1292664	56.97%	5.725%
67	14.704	1937	1943	1949	rVB	534999	821565	36.21%	3.639%
68	14.874	1965	1972	1982	rBV	449112	735058	32.39%	3.256%
69	15.027	1997	1998	2004	rVB2	5154	6795	0.30%	0.030%
70	15.150	2017	2019	2022	rVB3	5108	5941	0.26%	0.026%
71	15.185	2022	2025	2026	rBV	3840	4332	0.19%	0.019%
72	15.432	2065	2067	2071	rBV3	4352	6081	0.27%	0.027%
73	15.691	2104	2111	2120	rBV	1085891	1676742	73.89%	7.427%
74	15.796	2123	2129	2135	rBV	360765	530682	23.39%	2.350%
75	15.932	2150	2152	2155	rVB4	6600	7482	0.33%	0.033%
76	15.984	2160	2161	2164	rVB3	5136	3527	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
 Data File : BG061679.D
 Acq On : 24 Jun 2024 17:34
 Operator : MA/JU
 Sample : PB161484BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK484

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

77	16.043	2169	2171	2173	rBV2	4198	3277	0.14%	0.015%
78	16.319	2217	2218	2222	rVB	4460	3958	0.17%	0.018%
79	16.372	2224	2227	2229	rBV2	5942	5329	0.23%	0.024%
80	16.590	2260	2264	2265	rBV3	4781	5359	0.24%	0.024%
81	16.619	2267	2269	2271	rVV	3672	3213	0.14%	0.014%
82	16.654	2273	2275	2277	rBV	3945	3437	0.15%	0.015%
83	16.854	2307	2309	2312	rBV2	6201	4682	0.21%	0.021%
84	16.977	2329	2330	2333	rBV3	3748	3989	0.18%	0.018%
85	17.018	2335	2337	2338	rVB2	5217	3309	0.15%	0.015%
86	17.095	2346	2350	2355	rBV7	5771	9768	0.43%	0.043%
87	17.171	2359	2363	2365	rBV3	4747	6674	0.29%	0.030%
88	17.359	2393	2395	2397	rVB2	5201	3671	0.16%	0.016%
89	17.447	2403	2410	2416	rBV	749958	1140990	50.28%	5.054%
90	17.547	2420	2427	2436	rBV	1297798	1973834	86.99%	8.742%
91	17.665	2446	2447	2450	rBV3	6691	8145	0.36%	0.036%
92	18.111	2520	2523	2526	rBV5	6350	8633	0.38%	0.038%
93	18.223	2540	2542	2545	rBV3	5263	4875	0.21%	0.022%
94	18.481	2585	2586	2588	rVB	6046	3239	0.14%	0.014%
95	19.392	2738	2741	2746	rVB6	17693	25600	1.13%	0.113%
96	19.463	2749	2753	2755	rBV4	15463	19863	0.88%	0.088%
97	19.827	2809	2815	2823	rBV	1509668	2221103	97.88%	9.838%
98	21.707	3130	3135	3143	rVB2	711044	1153067	50.81%	5.107%
99	24.721	3639	3648	3660	rVB2	794850	2269164	100.00%	10.051%
100	24.939	3678	3685	3696	rVB3	441398	1228743	54.15%	5.442%




Sum of corrected areas: 22577465

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
Data File : BG061679.D
Acq On : 24 Jun 2024 17:34
Operator : MA/JU
Sample : PB161484BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK484

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

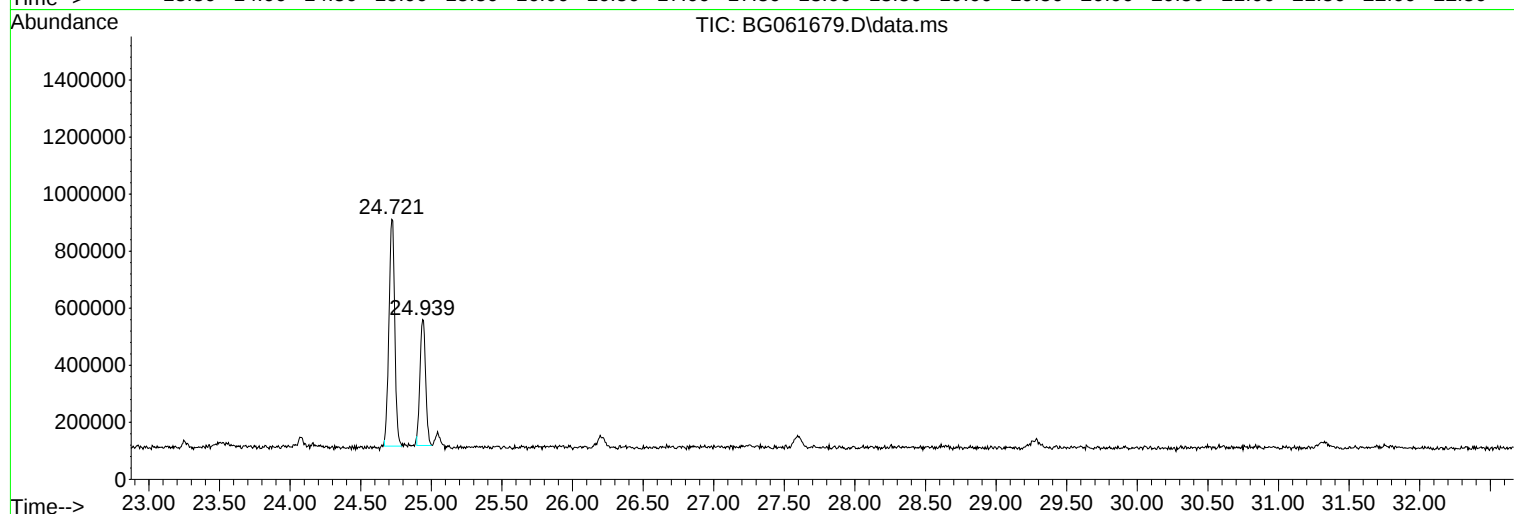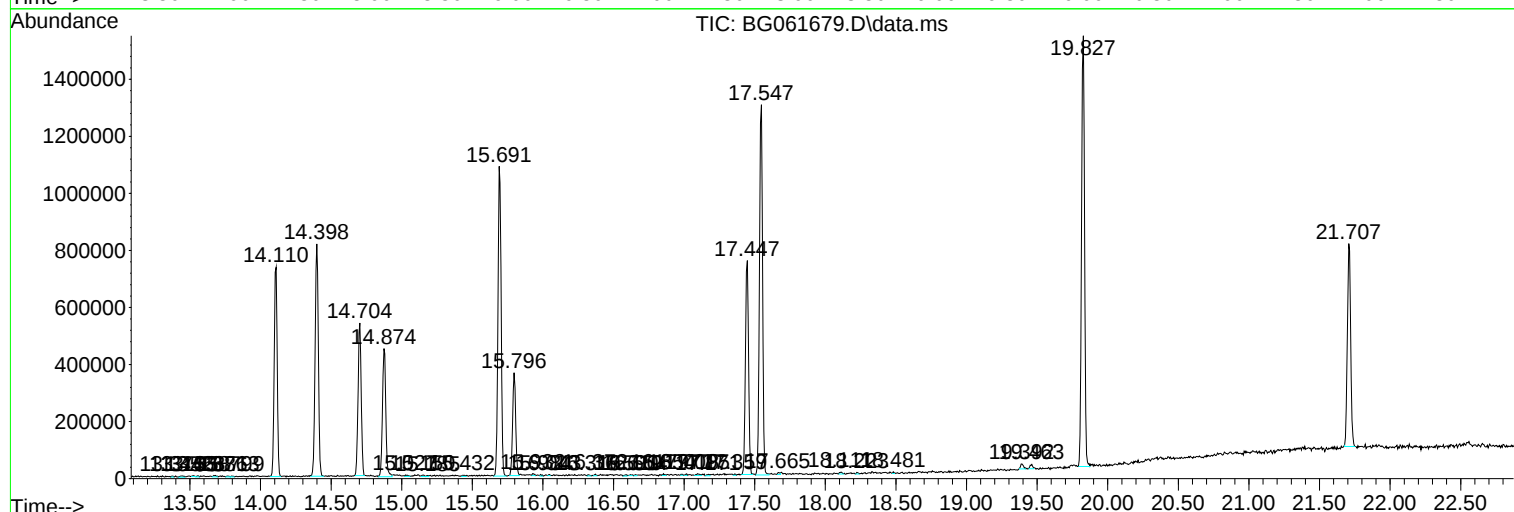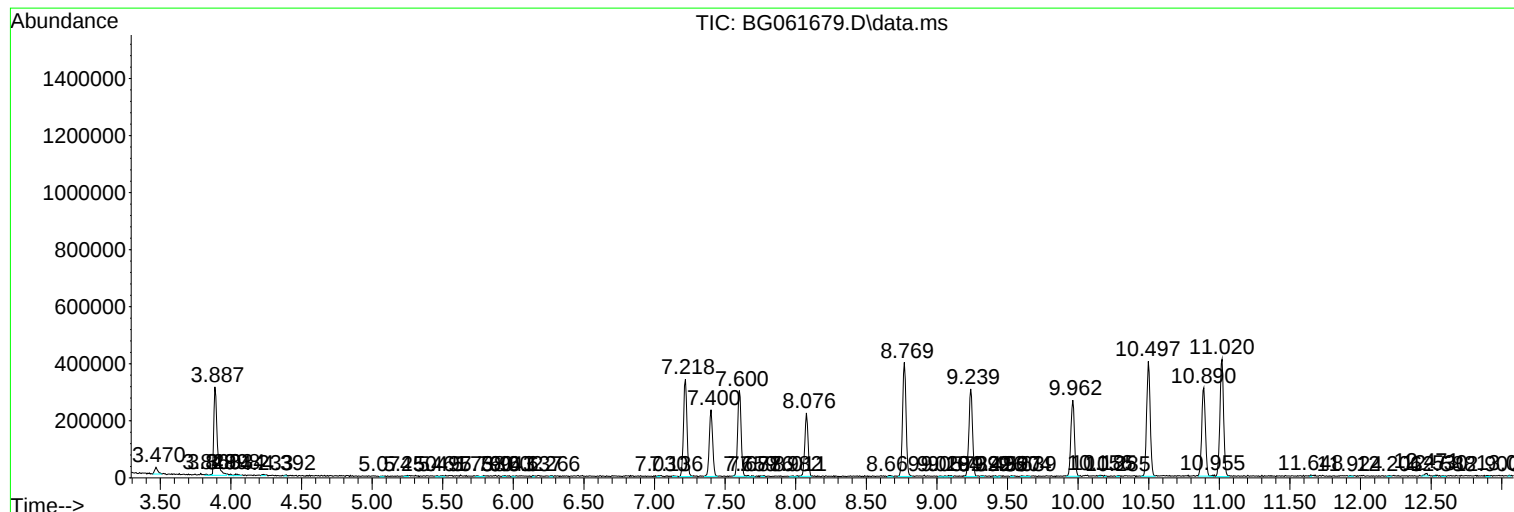

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
Data File : BG061679.D
Acq On : 24 Jun 2024 17:34
Operator : MA/JU
Sample : PB161484BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK484

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
Data File : BG061679.D
Acq On : 24 Jun 2024 17:34
Operator : MA/JU
Sample : PB161484BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK484

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc