

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
 Data File : BG061705.D
 Acq On : 25 Jun 2024 16:34
 Operator : MA/JU
 Sample : PB161517BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK517

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061705.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.470	27	31	36	rBV4	23434	35250	1.63%	0.155%
2	3.888	98	102	109	rBV	262752	411910	19.08%	1.813%
3	4.040	126	128	130	rVB2	4940	4755	0.22%	0.021%
4	4.064	130	132	134	rBV3	4612	4306	0.20%	0.019%
5	4.111	138	140	141	rBV	6228	3879	0.18%	0.017%
6	4.217	156	158	159	rBV2	4786	3537	0.16%	0.016%
7	4.446	194	197	198	rBV2	4726	3958	0.18%	0.017%
8	4.504	205	207	212	rVB3	3045	3789	0.18%	0.017%
9	4.669	231	235	238	rBV5	4855	4241	0.20%	0.019%
10	5.245	331	333	335	rBV2	3076	3165	0.15%	0.014%
11	5.298	340	342	345	rVB4	3940	3608	0.17%	0.016%
12	5.462	368	370	373	rBV3	4249	3236	0.15%	0.014%
13	5.503	376	377	382	rBV4	2875	3342	0.15%	0.015%
14	5.697	407	410	412	rBV3	4518	4278	0.20%	0.019%
15	5.797	424	427	430	rVB4	2605	3996	0.19%	0.018%
16	6.079	472	475	477	rBV2	3148	4674	0.22%	0.021%
17	6.255	501	505	508	rBV4	2260	3204	0.15%	0.014%
18	6.537	550	553	556	rBV2	1980	3235	0.15%	0.014%
19	6.608	561	565	568	rVB4	5167	5661	0.26%	0.025%
20	7.031	633	637	638	rBV4	4083	3187	0.15%	0.014%
21	7.213	658	668	677	rBV	296993	517133	23.95%	2.276%
22	7.395	693	699	708	rVB	205325	341792	15.83%	1.504%
23	7.595	726	733	740	rBV	255499	443418	20.54%	1.952%
24	7.994	800	801	806	rVB2	2978	3463	0.16%	0.015%
25	8.071	806	814	821	rBV	246250	408431	18.92%	1.798%
26	8.382	865	867	871	rVB3	2703	3484	0.16%	0.015%
27	8.764	926	932	942	rBV	354007	608333	28.18%	2.678%
28	9.158	996	999	1001	rBV2	3183	3992	0.18%	0.018%
29	9.234	1005	1012	1020	rVB	276451	481986	22.32%	2.122%
30	9.381	1034	1037	1039	rBV2	3173	4034	0.19%	0.018%
31	9.428	1043	1045	1049	rVB3	4394	4636	0.21%	0.020%
32	9.734	1094	1097	1100	rVB2	3855	4421	0.20%	0.019%
33	9.957	1128	1135	1146	rBV	238651	422610	19.57%	1.860%
34	10.057	1149	1152	1155	rVV4	3258	3862	0.18%	0.017%
35	10.092	1155	1158	1161	rVB3	3081	3702	0.17%	0.016%
36	10.168	1169	1171	1175	rVB2	4909	3793	0.18%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
 Data File : BG061705.D
 Acq On : 25 Jun 2024 16:34
 Operator : MA/JU
 Sample : PB161517BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK517

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	10.492	1219	1226	1234	rVV	360098	643551	29.81%	2.833%
38	10.885	1285	1293	1302	rVB	378396	676693	31.34%	2.979%
39	10.956	1302	1305	1307	rBV4	2889	3337	0.15%	0.015%
40	11.014	1307	1315	1324	rVV2	386490	671970	31.12%	2.958%

41	11.249	1353	1355	1358	rBV3	3510	3786	0.18%	0.017%
42	11.296	1360	1363	1365	rBV3	4598	4545	0.21%	0.020%
43	11.508	1397	1399	1401	rBV	3308	3284	0.15%	0.014%
44	12.019	1484	1486	1489	rVB2	3321	3690	0.17%	0.016%
45	12.143	1505	1507	1510	rVB	4042	3318	0.15%	0.015%

46	12.331	1538	1539	1542	rVB3	6065	4292	0.20%	0.019%
47	12.378	1542	1547	1550	rBV3	4757	6889	0.32%	0.030%
48	12.413	1550	1553	1557	rBV3	3358	5966	0.28%	0.026%
49	12.454	1557	1560	1566	rVV3	7532	12501	0.58%	0.055%
50	12.560	1576	1578	1584	rBV2	6870	8952	0.41%	0.039%

51	12.683	1596	1599	1602	rBV	2473	3739	0.17%	0.016%
52	13.212	1685	1689	1692	rVB5	4151	5195	0.24%	0.023%
53	13.300	1702	1704	1709	rVB4	3285	4229	0.20%	0.019%
54	13.470	1731	1733	1736	rBV2	3651	3584	0.17%	0.016%
55	13.512	1738	1740	1743	rVB3	3664	4064	0.19%	0.018%

56	13.600	1750	1755	1756	rBV2	4466	5175	0.24%	0.023%
57	13.658	1764	1765	1768	rBV3	4249	3678	0.17%	0.016%
58	13.752	1779	1781	1784	rBV2	4086	3909	0.18%	0.017%
59	13.982	1818	1820	1823	rVB	5332	3677	0.17%	0.016%
60	14.005	1823	1824	1832	rVB3	4040	6896	0.32%	0.030%

61	14.105	1832	1841	1847	rBV	686280	987610	45.74%	4.347%
62	14.158	1848	1850	1853	rVB	4286	3124	0.14%	0.014%
63	14.399	1884	1891	1899	rVB	723951	1184912	54.88%	5.216%
64	14.698	1936	1942	1950	rVB	649351	1020211	47.25%	4.491%
65	14.875	1965	1972	1982	rBV	434859	682783	31.62%	3.005%

66	14.957	1984	1986	1987	rVV2	7258	5122	0.24%	0.023%
67	15.110	2010	2012	2015	rBV4	4293	5410	0.25%	0.024%
68	15.245	2031	2035	2037	rBV2	3675	4445	0.21%	0.020%
69	15.427	2065	2066	2070	rVB4	3446	3304	0.15%	0.015%
70	15.550	2084	2087	2090	rVB5	3710	4116	0.19%	0.018%

71	15.603	2095	2096	2101	rVB4	3472	3385	0.16%	0.015%
72	15.691	2104	2111	2118	rVB	1033095	1578401	73.11%	6.948%
73	15.744	2118	2120	2122	rBV3	6023	5965	0.28%	0.026%
74	15.797	2122	2129	2137	rVV	344828	528037	24.46%	2.324%
75	15.891	2143	2145	2147	rVB2	6070	4163	0.19%	0.018%

76	15.926	2149	2151	2157	rBV4	8835	13769	0.64%	0.061%
----	--------	------	------	------	------	------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
 Data File : BG061705.D
 Acq On : 25 Jun 2024 16:34
 Operator : MA/JU
 Sample : PB161517BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK517

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

77	16.103	2177	2181	2183	rBV4	4036	5520	0.26%	0.024%
78	16.167	2190	2192	2194	rBV	3747	4001	0.19%	0.018%
79	16.208	2197	2199	2202	rBV3	4275	4736	0.22%	0.021%
80	16.255	2204	2207	2208	rBV3	3193	3118	0.14%	0.014%
81	16.314	2215	2217	2220	rBV3	2829	3106	0.14%	0.014%
82	16.461	2238	2242	2244	rBV4	4378	4971	0.23%	0.022%
83	16.831	2303	2305	2308	rBV3	3513	3961	0.18%	0.017%
84	17.213	2368	2370	2373	rBV2	6075	6827	0.32%	0.030%
85	17.319	2384	2388	2389	rBV2	4117	4762	0.22%	0.021%
86	17.442	2403	2409	2418	rVB	976188	1463338	67.78%	6.441%
87	17.542	2419	2426	2434	rVB	1255334	1886328	87.37%	8.303%
88	17.677	2445	2449	2454	rBV4	5867	11987	0.56%	0.053%
89	17.765	2463	2464	2467	rBV2	4179	3284	0.15%	0.014%
90	18.053	2510	2513	2516	rBV2	7978	11142	0.52%	0.049%
91	18.153	2528	2530	2531	rBV	5600	3826	0.18%	0.017%
92	18.171	2531	2533	2534	rVB	5920	3221	0.15%	0.014%
93	18.553	2596	2598	2602	rBV4	5699	6424	0.30%	0.028%
94	18.629	2609	2611	2613	rBV2	7033	4928	0.23%	0.022%
95	19.387	2737	2740	2745	rVB6	19723	28944	1.34%	0.127%
96	19.458	2749	2752	2757	rVB2	21511	27628	1.28%	0.122%
97	19.822	2808	2814	2823	rVB	1503684	2120268	98.21%	9.333%
98	21.708	3129	3135	3145	rVB2	896421	1502636	69.60%	6.614%
99	24.716	3638	3647	3657	rVB2	773331	2159009	100.00%	9.503%
100	24.933	3676	3684	3694	rVB2	584690	1536977	71.19%	6.765%




Sum of corrected areas: 22718920

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
Data File : BG061705.D
Acq On : 25 Jun 2024 16:34
Operator : MA/JU
Sample : PB161517BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK517

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

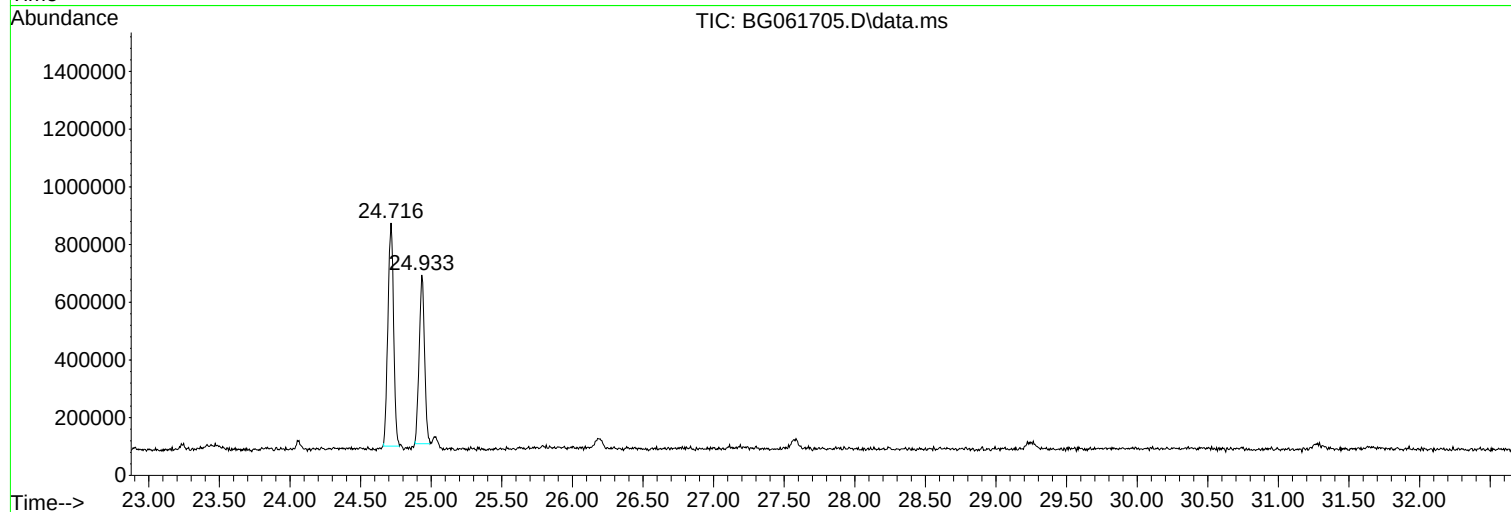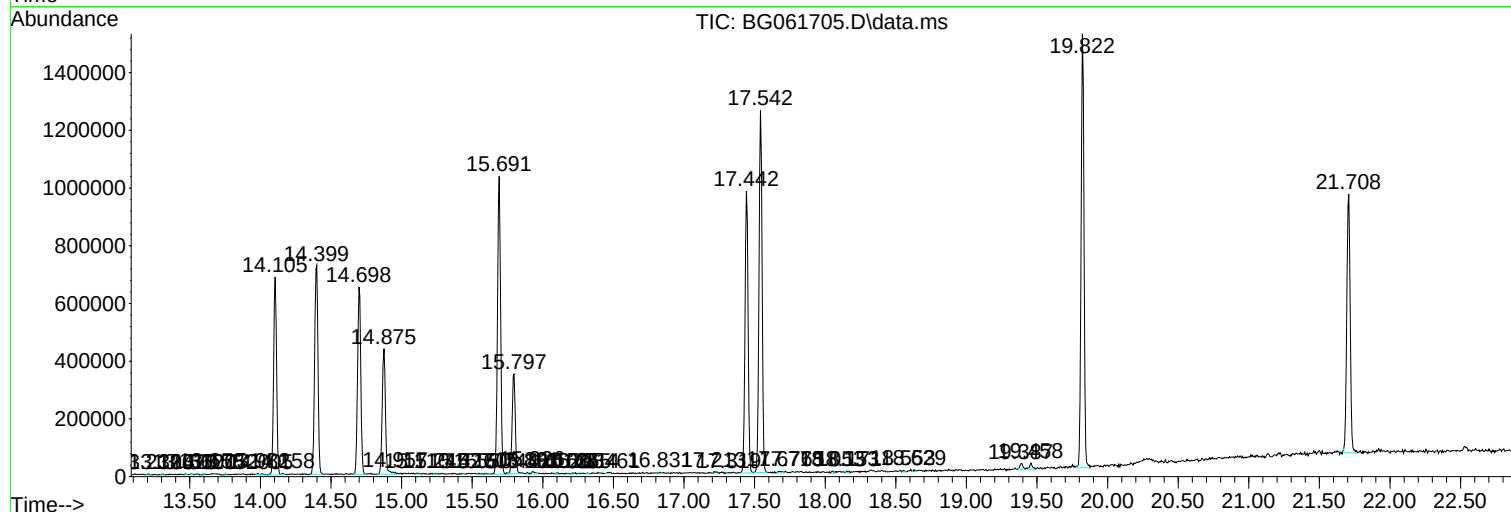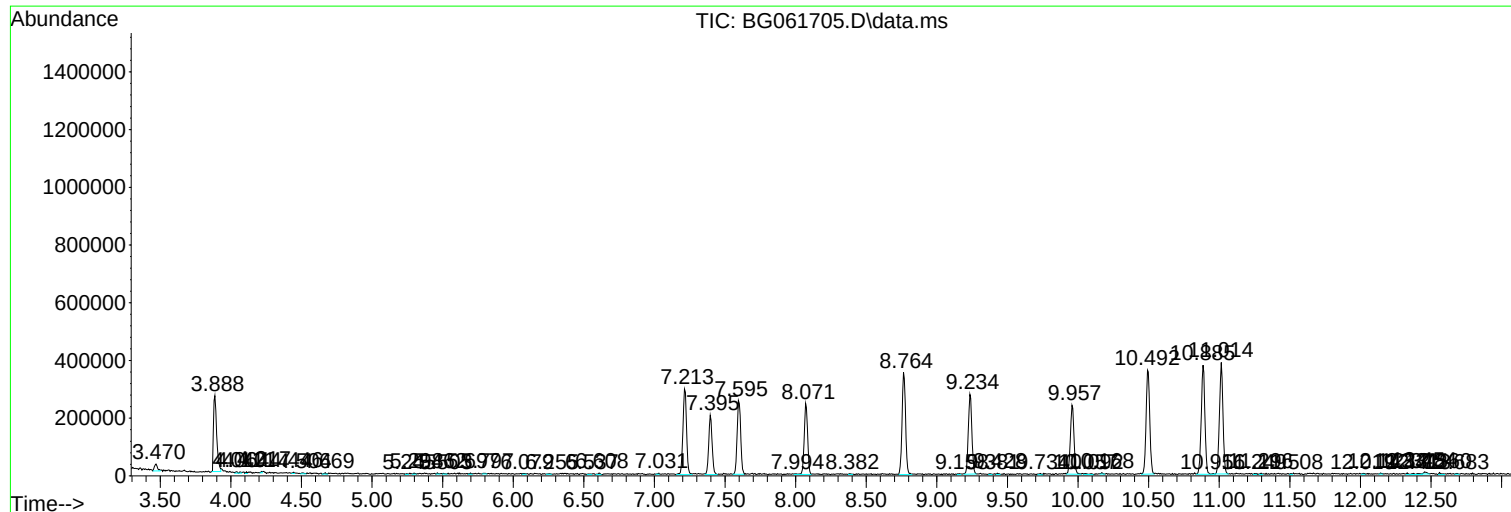

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
Data File : BG061705.D
Acq On : 25 Jun 2024 16:34
Operator : MA/JU
Sample : PB161517BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK517

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
Data File : BG061705.D
Acq On : 25 Jun 2024 16:34
Operator : MA/JU
Sample : PB161517BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK517

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------