

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
 Data File : BG061720.D
 Acq On : 26 Jun 2024 3:27
 Operator : MA/JU
 Sample : PB161523BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK583

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061720.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.465	27	30	37	rVB	22009	30003	1.19%	0.112%
2	3.753	76	79	82	rVB2	4252	3829	0.15%	0.014%
3	3.835	91	93	95	rBV3	3980	3891	0.15%	0.015%
4	3.882	97	101	113	rVV	299622	496828	19.64%	1.858%
5	4.188	150	153	155	rBV3	3180	3815	0.15%	0.014%
6	4.229	157	160	163	rVB3	8858	7936	0.31%	0.030%
7	4.499	204	206	210	rBV3	4119	4614	0.18%	0.017%
8	5.234	330	331	334	rBV	4051	3882	0.15%	0.015%
9	5.322	341	346	347	rBV3	3387	4823	0.19%	0.018%
10	5.551	384	385	389	rVB2	4394	3352	0.13%	0.013%
11	6.556	554	556	558	rBV2	3695	3572	0.14%	0.013%
12	6.738	584	587	589	rVB2	2943	3261	0.13%	0.012%
13	6.791	593	596	601	rVB2	2869	3794	0.15%	0.014%
14	7.214	659	668	678	rBV	386179	632114	24.98%	2.364%
15	7.396	689	699	708	rVB	256778	424475	16.78%	1.588%
16	7.543	720	724	725	rBV	2508	3239	0.13%	0.012%
17	7.596	725	733	741	rVV	323618	550000	21.74%	2.057%
18	8.072	806	814	822	rBV	242102	409319	16.18%	1.531%
19	8.500	886	887	892	rBV	2932	4062	0.16%	0.015%
20	8.765	925	932	941	rVB	492024	812123	32.10%	3.038%
21	8.859	945	948	950	rBV3	5459	4229	0.17%	0.016%
22	9.235	1004	1012	1019	rBV	383402	654764	25.88%	2.449%
23	9.535	1061	1063	1068	rBV2	1911	3303	0.13%	0.012%
24	9.664	1082	1085	1089	rVB	3505	4997	0.20%	0.019%
25	9.881	1119	1122	1124	rBV2	3257	4611	0.18%	0.017%
26	9.958	1126	1135	1144	rVV2	315714	569744	22.52%	2.131%
27	10.246	1179	1184	1186	rBV3	2977	3698	0.15%	0.014%
28	10.492	1219	1226	1234	rVB	483550	853316	33.73%	3.192%
29	10.886	1286	1293	1301	rVB	412359	731899	28.93%	2.738%
30	11.015	1307	1315	1324	rVB	519833	917650	36.27%	3.432%
31	11.368	1373	1375	1377	rVB2	6015	4287	0.17%	0.016%
32	11.397	1377	1380	1383	rBV2	4787	6330	0.25%	0.024%
33	11.626	1417	1419	1423	rBV3	2655	3558	0.14%	0.013%
34	11.885	1462	1463	1467	rVB2	3569	3619	0.14%	0.014%
35	12.214	1515	1519	1520	rBV	3474	3316	0.13%	0.012%
36	12.461	1557	1561	1566	rBV2	11211	17090	0.68%	0.064%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
 Data File : BG061720.D
 Acq On : 26 Jun 2024 3:27
 Operator : MA/JU
 Sample : PB161523BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK583

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	12.825	1621	1623	1626	rVB2	3874	3418	0.14%	0.013%
38	13.489	1732	1736	1737	rBV2	5566	5810	0.23%	0.022%
39	13.835	1794	1795	1802	rBV4	2664	4743	0.19%	0.018%
40	14.100	1834	1840	1850	rVB	944127	1404756	55.52%	5.254%
41	14.394	1883	1890	1898	rVB	1044860	1615507	63.85%	6.043%
42	14.699	1934	1942	1948	rVB	764747	1169862	46.24%	4.376%
43	14.787	1955	1957	1960	rVB2	5385	4332	0.17%	0.016%
44	14.875	1964	1972	1986	rBV	479726	805397	31.83%	3.013%
45	15.046	1998	2001	2002	rBV	4759	4288	0.17%	0.016%
46	15.105	2009	2011	2014	rVB4	6366	5795	0.23%	0.022%
47	15.328	2048	2049	2052	rBV2	4887	3926	0.16%	0.015%
48	15.422	2063	2065	2070	rBV2	3267	4677	0.18%	0.017%
49	15.686	2103	2110	2118	rVB	1371242	2075448	82.03%	7.763%
50	15.792	2122	2128	2137	rVB	433813	656223	25.94%	2.455%
51	15.921	2147	2150	2151	rBV2	5275	5038	0.20%	0.019%
52	16.109	2180	2182	2185	rVB2	3802	4008	0.16%	0.015%
53	16.379	2225	2228	2232	rVB2	4139	7288	0.29%	0.027%
54	16.468	2239	2243	2248	rVB4	7472	11857	0.47%	0.044%
55	16.709	2283	2284	2288	rBV	3201	3898	0.15%	0.015%
56	16.985	2328	2331	2336	rBV3	3726	6835	0.27%	0.026%
57	17.443	2401	2409	2415	rBV	966998	1466622	57.97%	5.486%
58	17.543	2419	2426	2433	rVB	1512099	2284863	90.31%	8.546%
59	18.101	2520	2521	2524	rVB3	6907	3852	0.15%	0.014%
60	18.383	2565	2569	2570	rBV3	3540	4003	0.16%	0.015%
61	18.489	2585	2587	2591	rBV2	5837	7111	0.28%	0.027%
62	18.659	2614	2616	2619	rVB4	7291	6041	0.24%	0.023%
63	19.382	2735	2739	2744	rBV5	20562	34158	1.35%	0.128%
64	19.452	2748	2751	2757	rVB3	20374	29258	1.16%	0.109%
65	19.652	2783	2785	2786	rBV2	7620	5482	0.22%	0.021%
66	19.823	2807	2814	2822	rBV	1680124	2466582	97.49%	9.226%
67	21.703	3128	3134	3140	rVB2	869337	1410830	55.76%	5.277%
68	24.711	3636	3646	3659	rVB2	898671	2530090	100.00%	9.464%
69	24.928	3674	3683	3693	rBV	535234	1487426	58.79%	5.564%




Sum of corrected areas: 26734767

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
Data File : BG061720.D
Acq On : 26 Jun 2024 3:27
Operator : MA/JU
Sample : PB161523BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK583

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

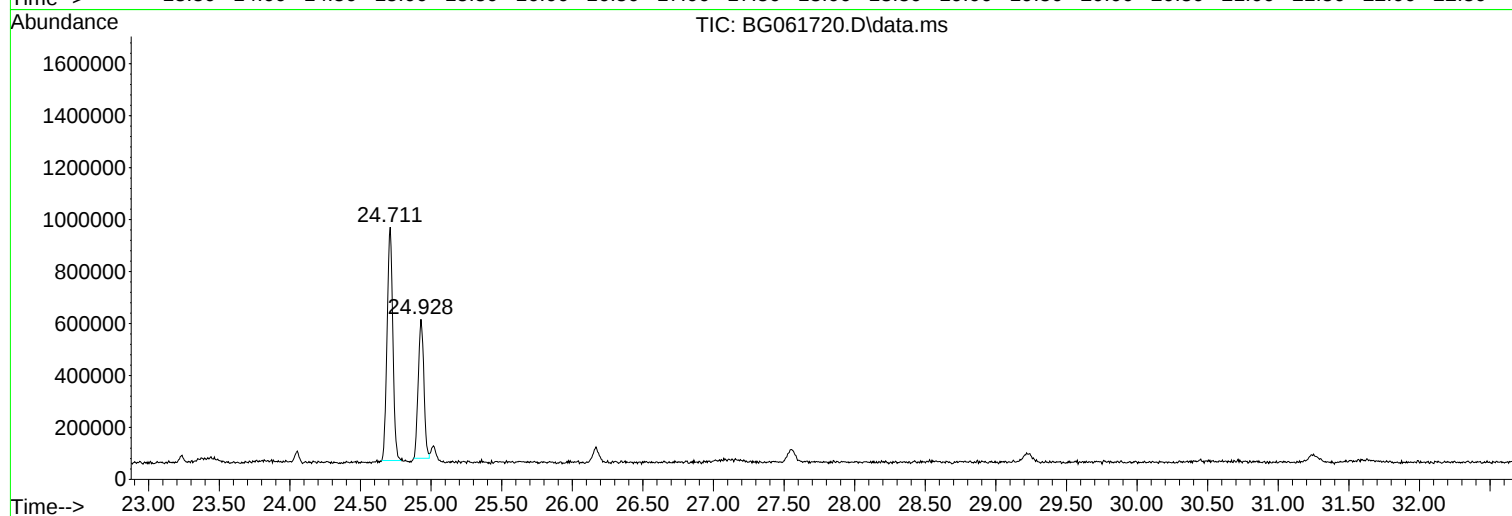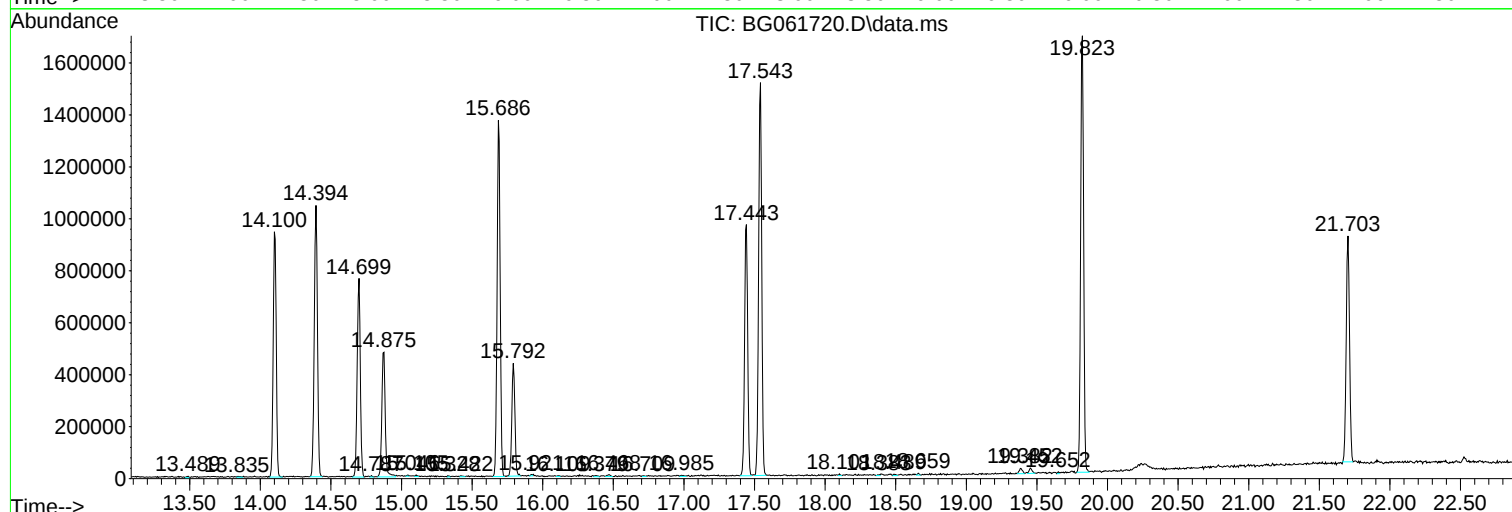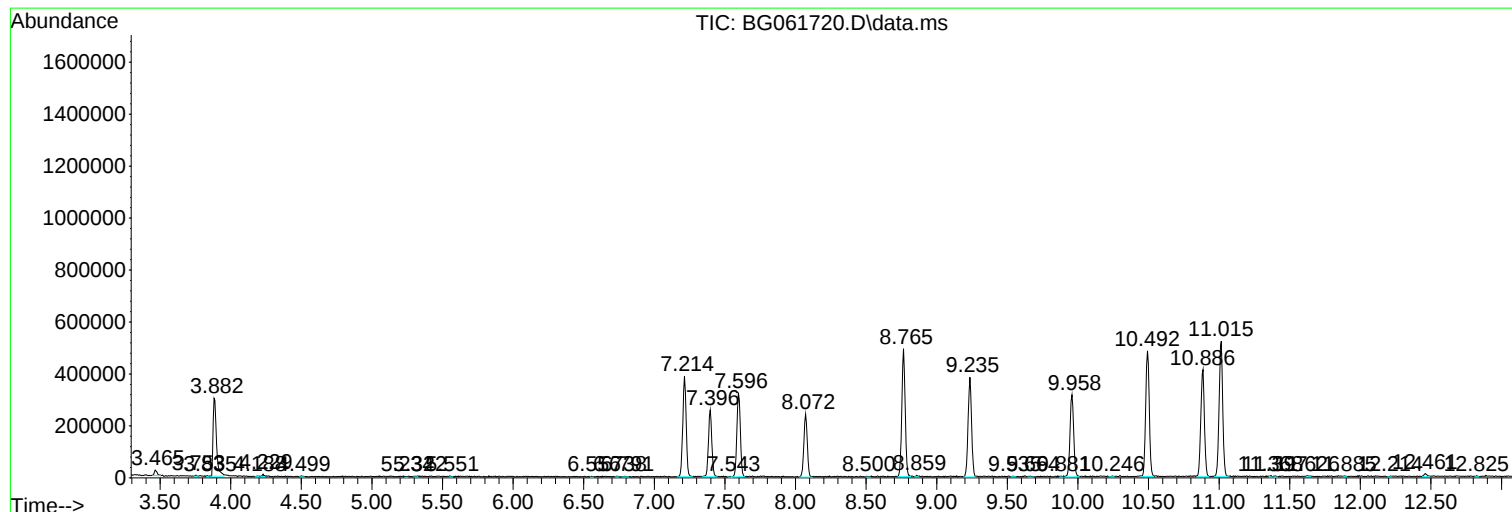

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
Data File : BG061720.D
Acq On : 26 Jun 2024 3:27
Operator : MA/JU
Sample : PB161523BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK583

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062424\
Data File : BG061720.D
Acq On : 26 Jun 2024 3:27
Operator : MA/JU
Sample : PB161523BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK583

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc