

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062516\
 Data File : BG022567.D
 Acq On : 25 Jun 2016 10:07
 Operator : UM/SJ
 Sample : H3633-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TPEMW9S

Quant Time: Jun 27 01:05:18 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 20:14:59 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	125738	20.00	ng	0.00
21) Naphthalene-d8	10.99	136	539246	20.00	ng	0.00
38) Acenaphthene-d10	14.80	164	384819	20.00	ng	0.00
63) Phenanthrene-d10	17.56	188	991014	20.00	ng	0.00
75) Chrysene-d12	21.85	240	1096624	20.00	ng	0.00
86) Perylene-d12	25.21	264	1146566	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.71	112	500533	63.85	ng	0.00
7) Phenol-d6	7.30	99	494846	44.78	ng	0.00
23) Nitrobenzene-d5	9.33	82	1078805	84.67	ng	0.00
41) 2,4,6-Tribromophenol	16.29	330	815570	134.75	ng	0.00
44) 2-Fluorobiphenyl	13.43	172	2108995	86.91	ng	0.00
78) Terphenyl-d14	20.16	244	2978988	71.97	ng	0.00
Target Compounds						
32) Benzoic acid	10.18	122	68	5.12	ng	Qvalue # 22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062516\
Data File : BG022567.D
Acq On : 25 Jun 2016 10:07
Operator : UM/SJ
Sample : H3633-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TEPMW9S

Quant Time: Jun 27 01:05:18 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

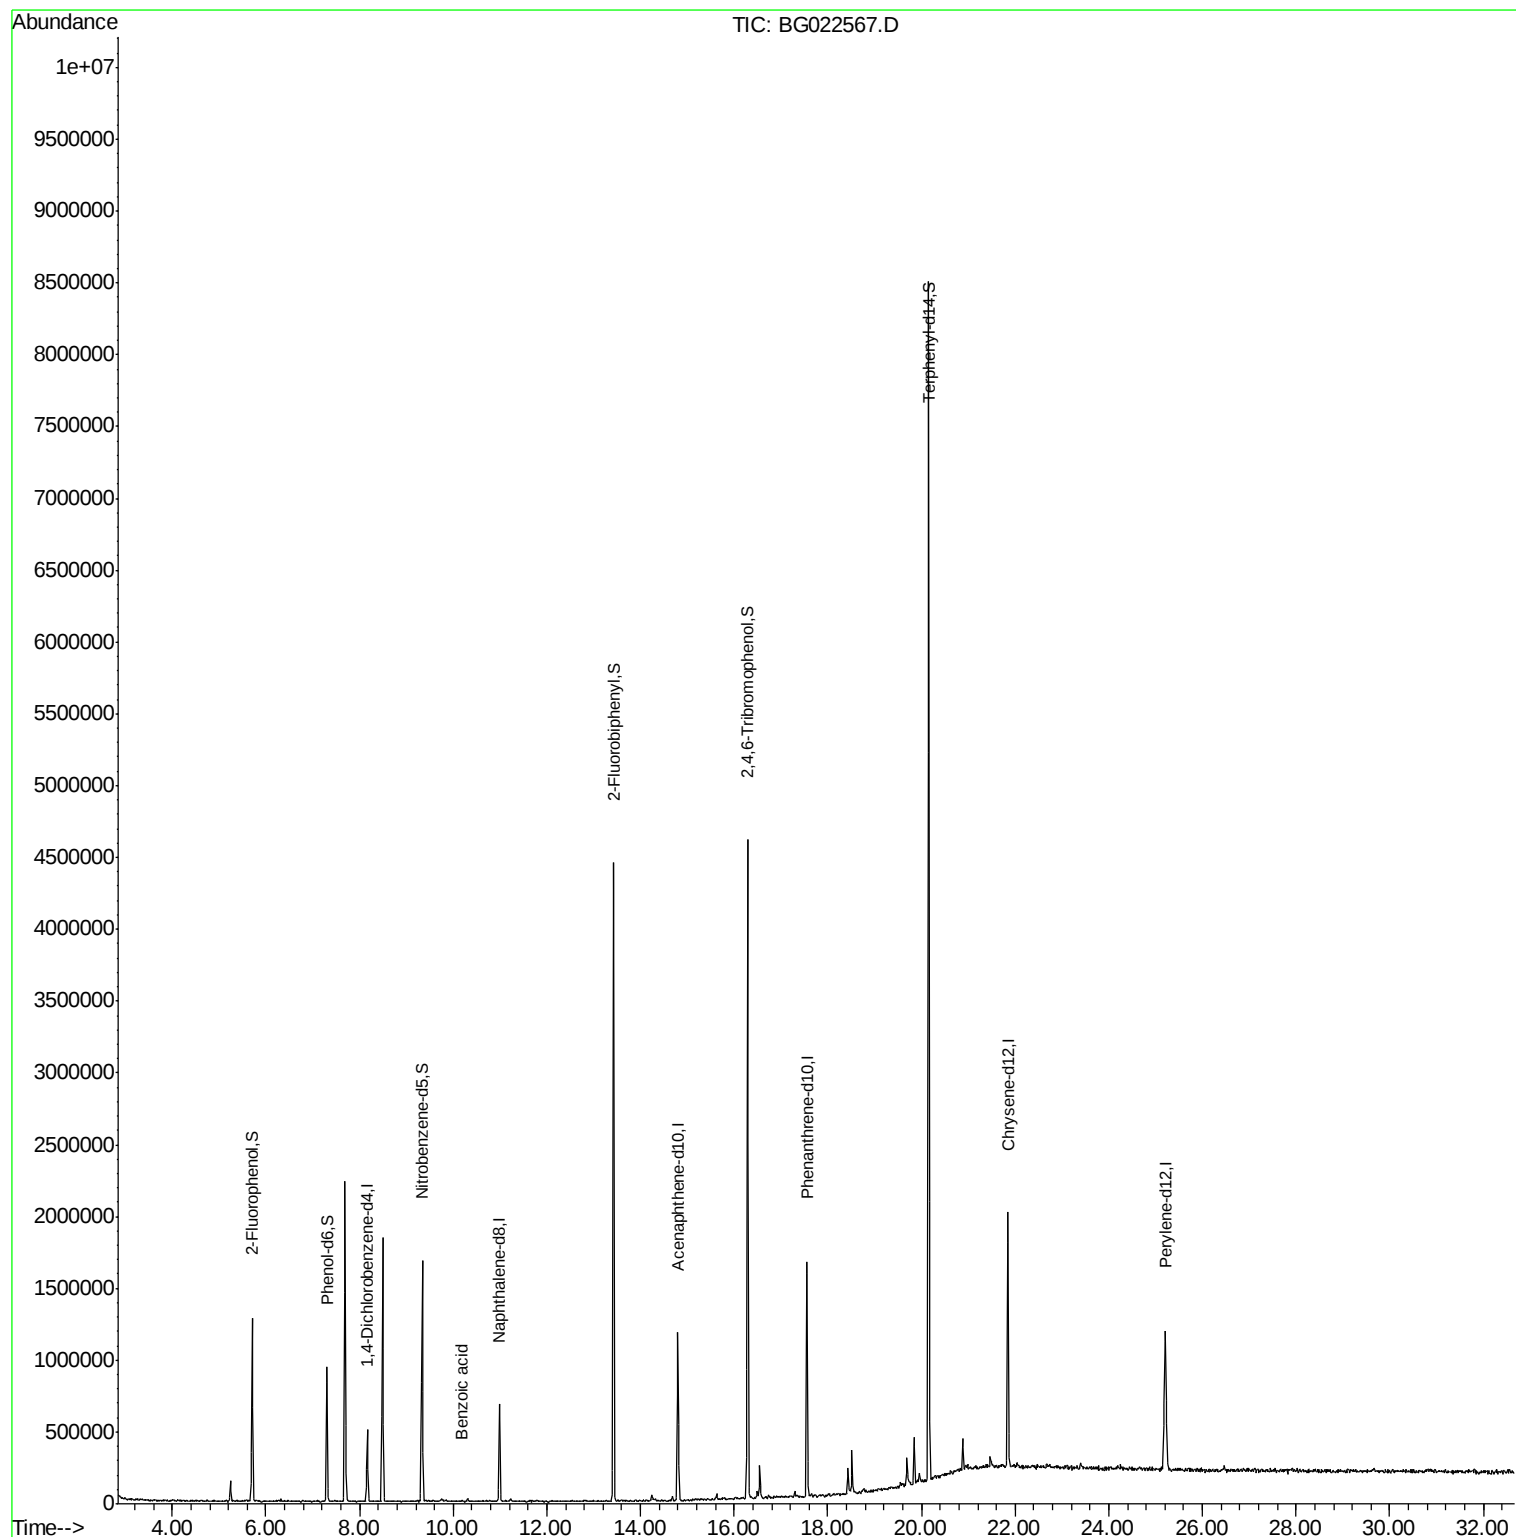

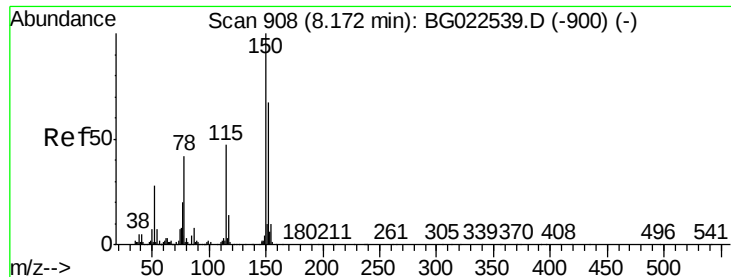

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.17 min Scan# 907

Delta R.T. -0.01 min

Lab File: BG022567.D

Acq: 25 Jun 2016 10:07

Instrument :

BNA_G

ClientSampleId :

TEPMW9S


Tgt Ion:152 Resp: 125738

Ion Ratio Lower Upper

152 100

150 156.7 144.7 217.1




115 75.2 64.0 96.0

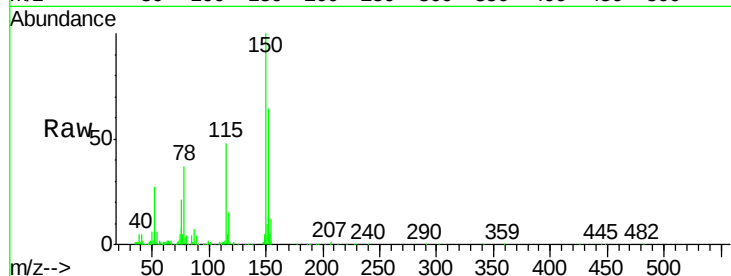

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

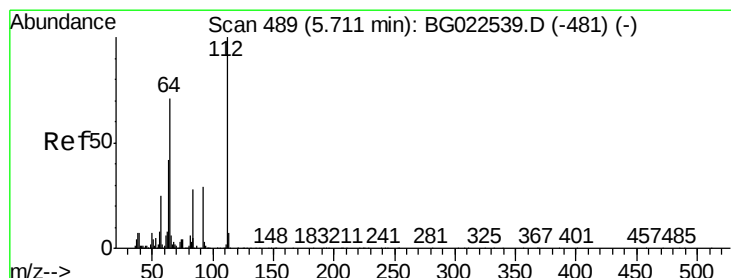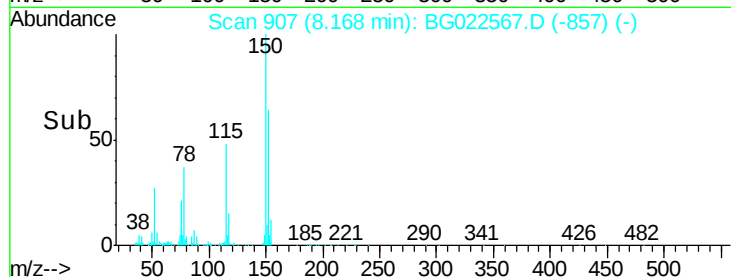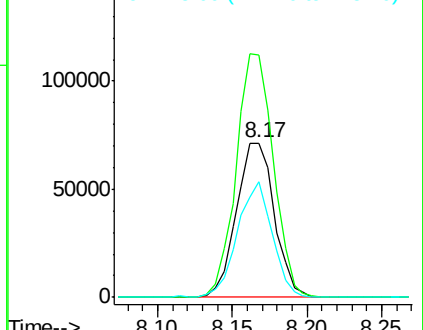

#5

2-Fluorophenol

Concen: 63.85 ng

RT: 5.71 min Scan# 488

Delta R.T. 0.00 min

Lab File: BG022567.D

Acq: 25 Jun 2016 10:07


Tgt Ion:112 Resp: 500533

Ion Ratio Lower Upper

112 100

64 67.3 59.0 88.4



63 40.6 37.8 56.8

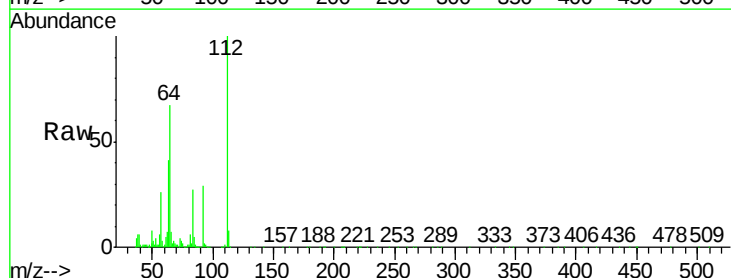

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

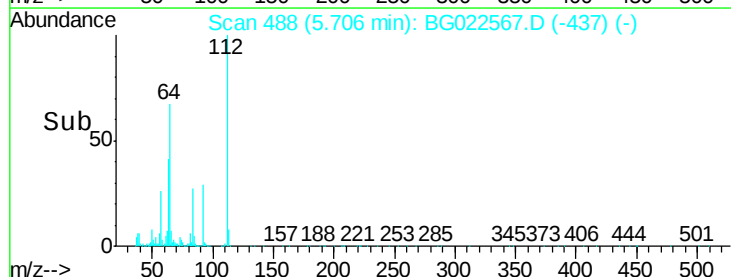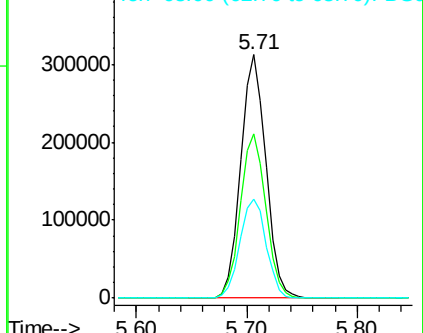



#7

Phenol-d6

Concen: 44.78 ng

RT: 7.30 min Scan# 760

Delta R.T. 0.00 min

Lab File: BG022567.D

Acq: 25 Jun 2016 10:07

Instrument :

BNA_G

ClientSampleId :

TEPMW9S


Tgt Ion: 99 Resp: 494846

Ion Ratio Lower Upper

99 100

42 21.2 17.8 26.6




71 51.9 41.5 62.3

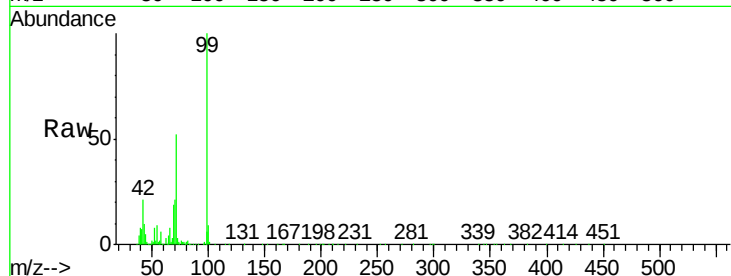

Abundance Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

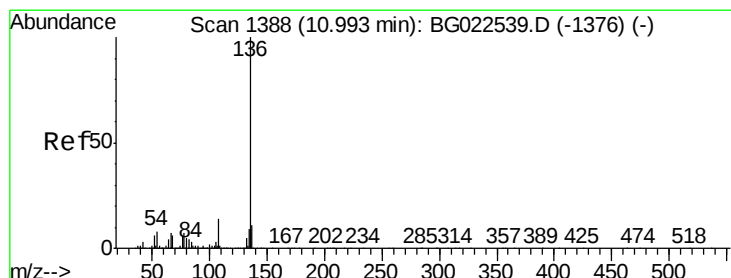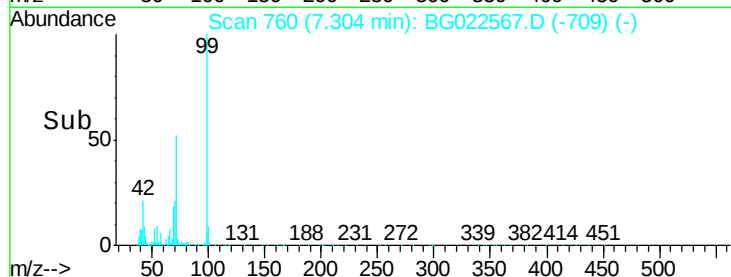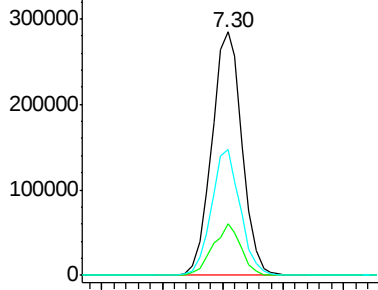

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.99 min Scan# 1387

Delta R.T. -0.01 min

Lab File: BG022567.D

Acq: 25 Jun 2016 10:07

Tgt Ion: 136 Resp: 539246


Ion Ratio Lower Upper

136 100

137 10.6 9.6 14.4

54 8.7 7.3 10.9

68 4.9 5.3 7.9#


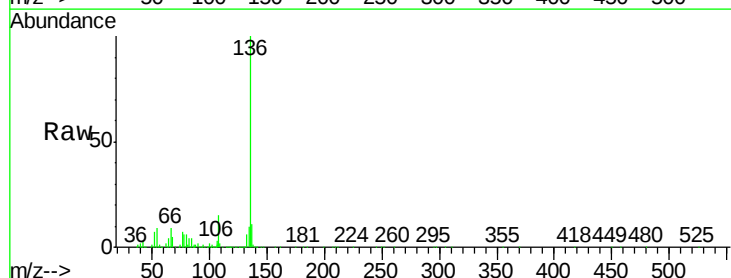



Abundance Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC



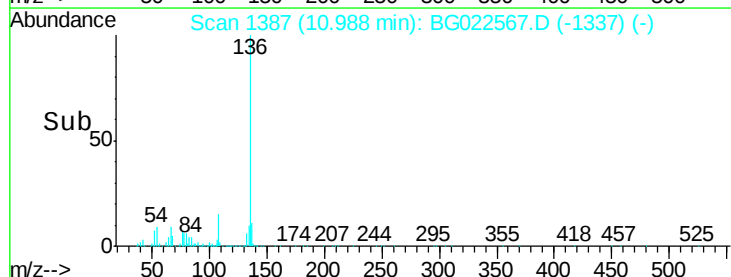
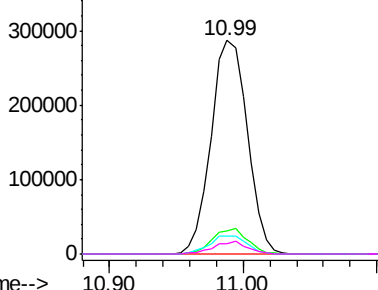


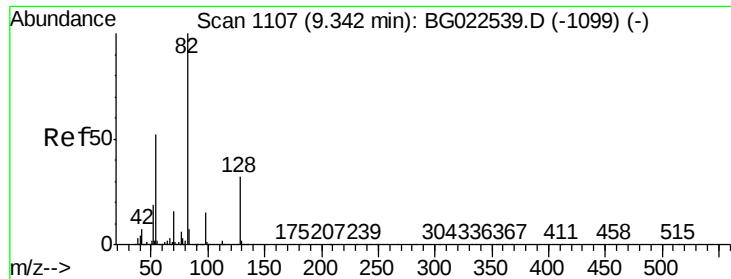

#23
Nitrobenzene-d5
Concen: 84.67 ng
RT: 9.33 min Scan# 1105
Delta R.T. -0.01 min
Lab File: BG022567.D
Acq: 25 Jun 2016 10:07




Instrument :
BNA_G
ClientSampleId :
TEPMW9S


Tgt Ion: 82 Resp: 1078805
Ion Ratio Lower Upper
82 100
128 33.0 24.4 36.6
54 51.2 41.4 62.0

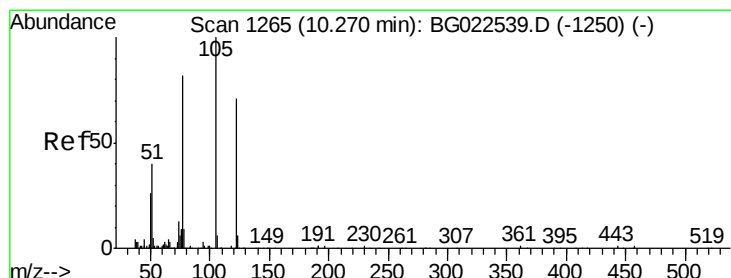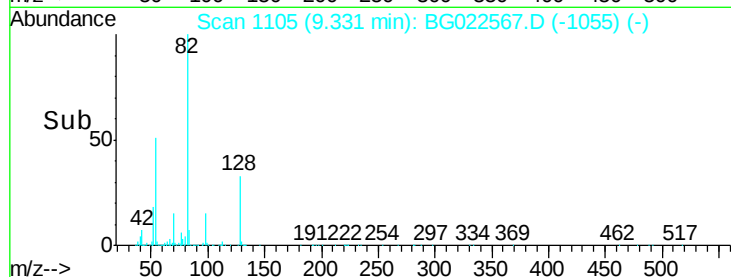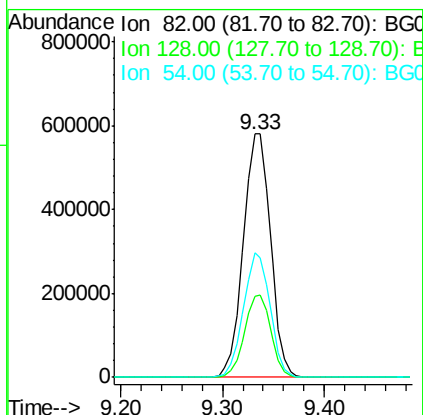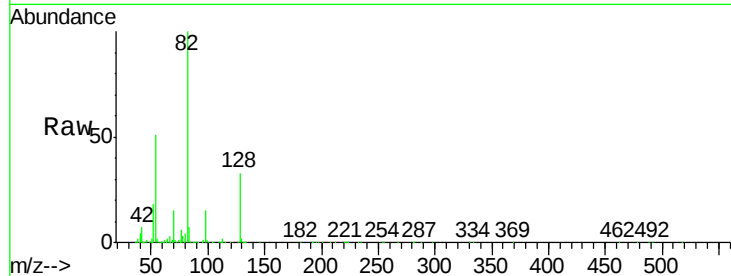

#32
Benzoic acid
Concen: 5.12 ng
RT: 10.18 min Scan# 1249
Delta R.T. -0.02 min
Lab File: BG022567.D
Acq: 25 Jun 2016 10:07

Tgt Ion: 122 Resp: 68
Ion Ratio Lower Upper
122 100
105 81.3 117.2 157.2#
77 0.0 109.2 149.2#

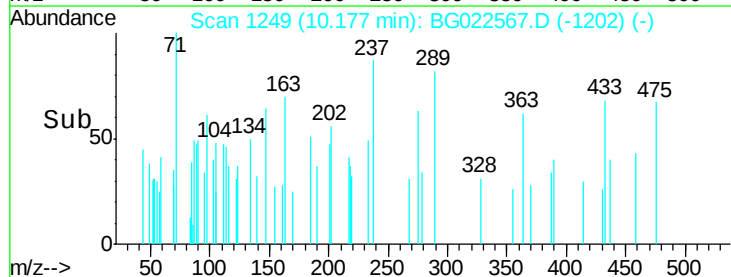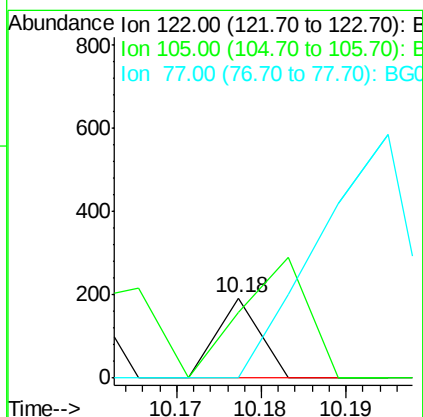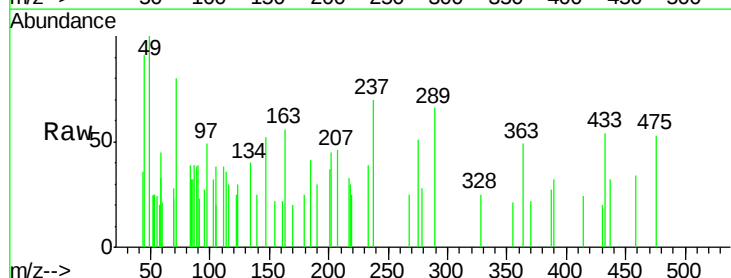

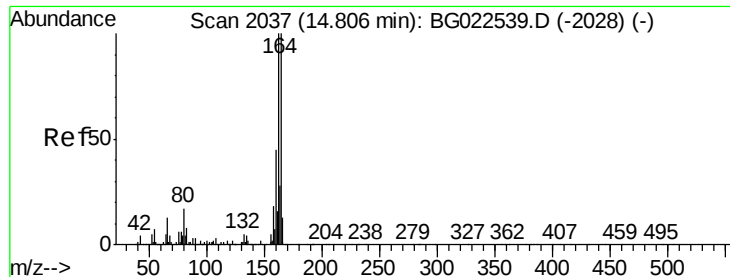

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.80 min Scan# 2036

Delta R.T. 0.00 min

Lab File: BG022567.D

Acq: 25 Jun 2016 10:07

Instrument :

BNA_G

ClientSampleId :

TEPMW9S


Tgt Ion:164 Resp: 384819

Ion Ratio Lower Upper

164 100

162 112.3 87.7 131.5




160 46.6 37.2 55.8

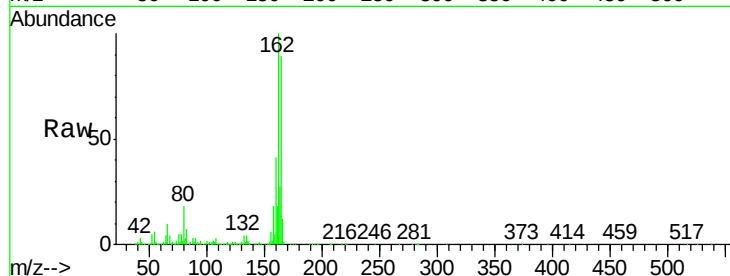

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

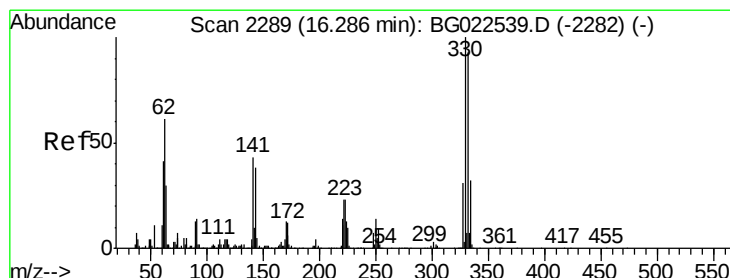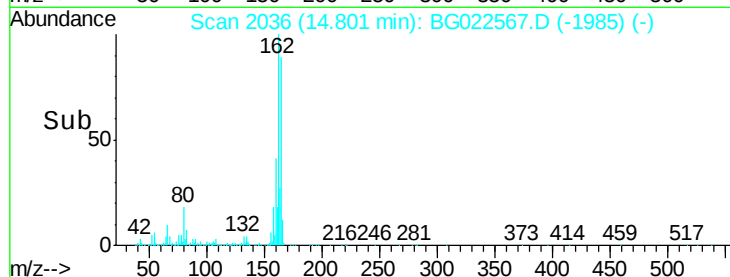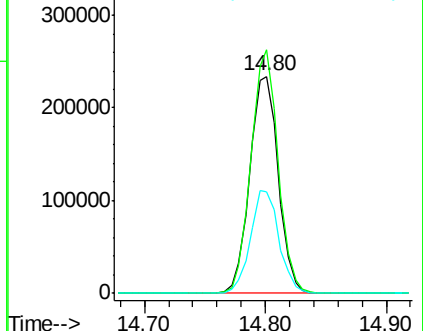

#41

2,4,6-Tribromophenol

Concen: 134.75 ng

RT: 16.29 min Scan# 2289

Delta R.T. 0.00 min

Lab File: BG022567.D

Acq: 25 Jun 2016 10:07


Tgt Ion:330 Resp: 815570

Ion Ratio Lower Upper

330 100

332 96.8 77.4 116.2



141 39.6 31.7 47.5

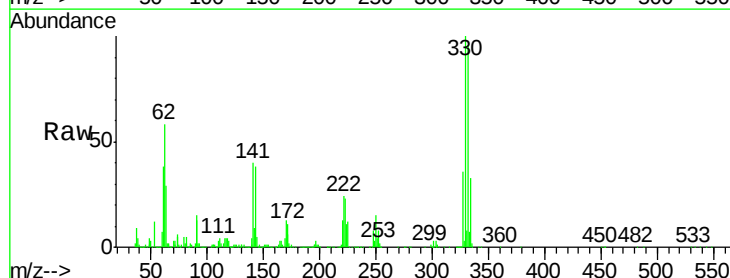


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



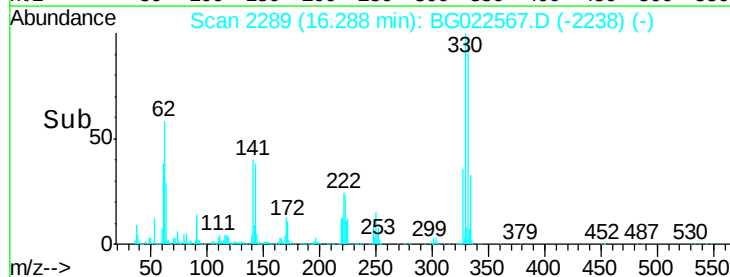
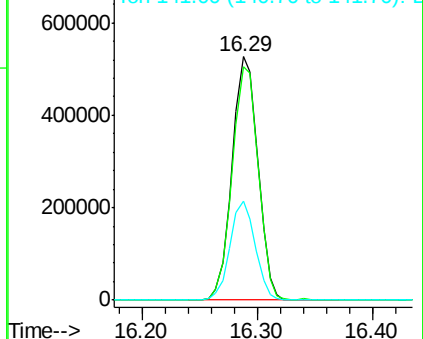


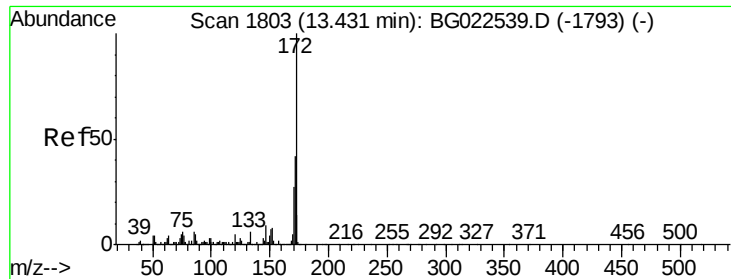

#44
 2-Fluorobiphenyl
 Concen: 86.91 ng
 RT: 13.43 min Scan# 1802
 Delta R.T. 0.00 min
 Lab File: BG022567.D
 Acq: 25 Jun 2016 10:07




Instrument :
 BNA_G
 ClientSampleId :
 TEPMW9S


Tgt Ion:172 Resp: 2108995
 Ion Ratio Lower Upper
 172 100
 171 42.9 31.6 47.4
 170 28.0 21.3 31.9

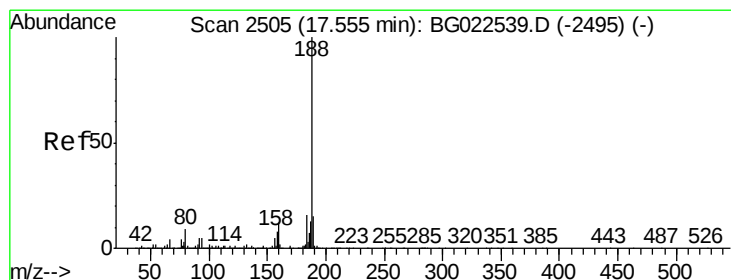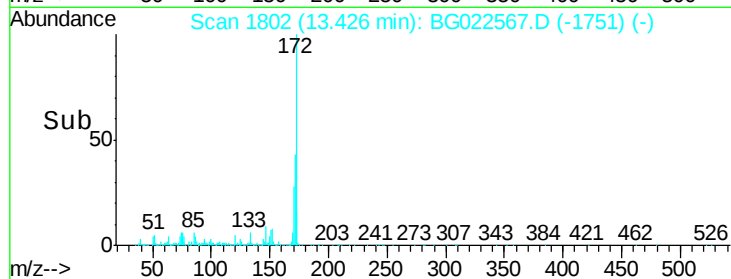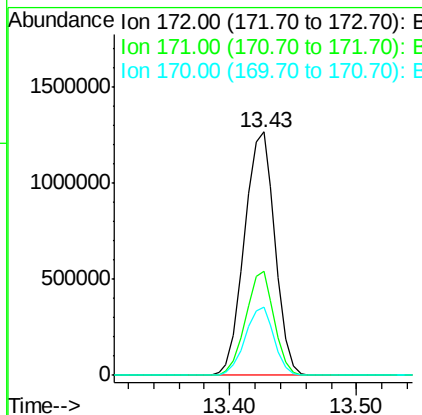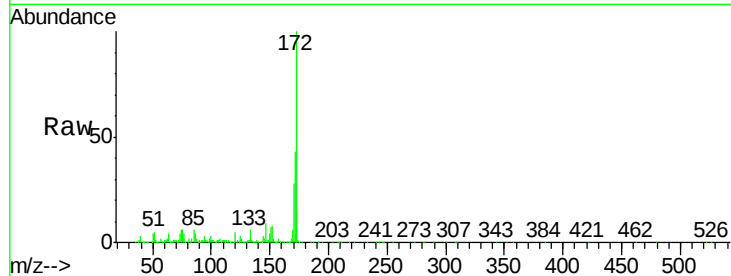

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 17.56 min Scan# 2505
 Delta R.T. 0.01 min
 Lab File: BG022567.D
 Acq: 25 Jun 2016 10:07

Tgt Ion:188 Resp: 991014
 Ion Ratio Lower Upper
 188 100
 94 7.1 5.2 7.8
 80 8.2 7.2 10.8

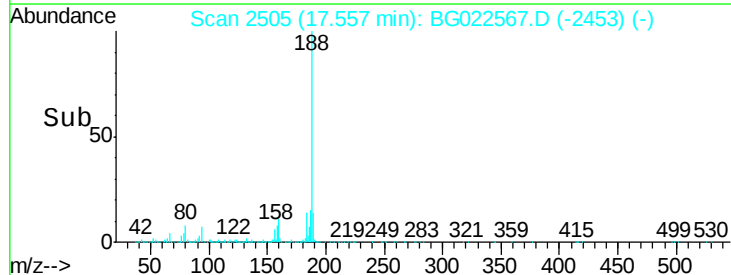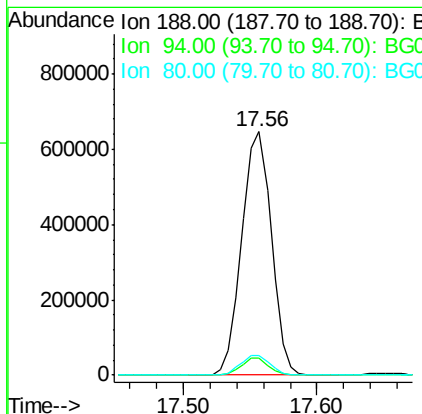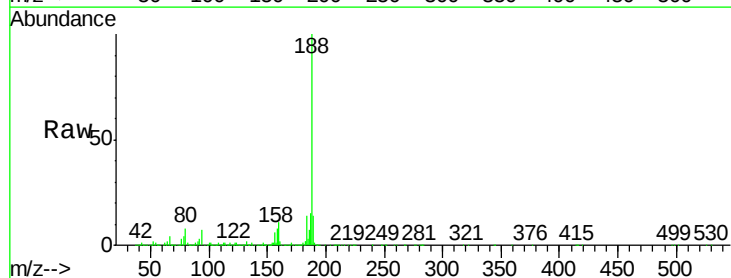

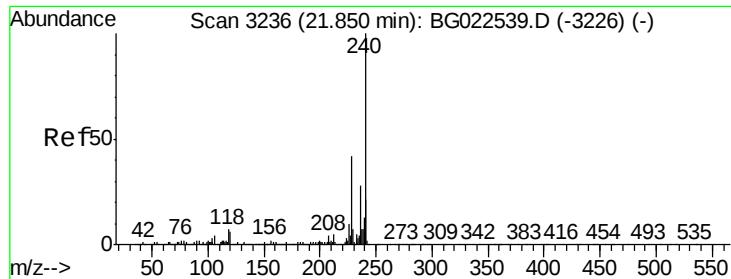

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.85 min Scan# 3235

Delta R.T. 0.00 min

Lab File: BG022567.D

Acq: 25 Jun 2016 10:07

Instrument :

BNA_G

ClientSampleId :

TEPMW9S


Tgt Ion:240 Resp: 1096624

Ion Ratio Lower Upper

240 100

120 5.7 4.1 6.1




236 26.7 21.1 31.7

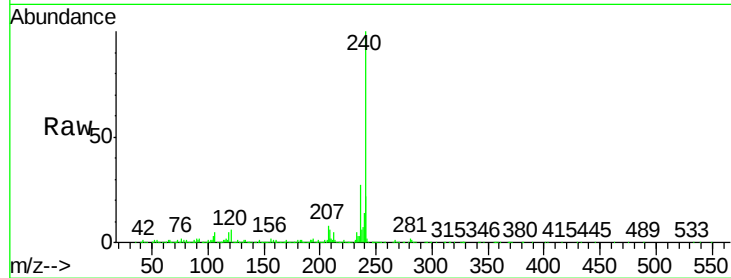

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

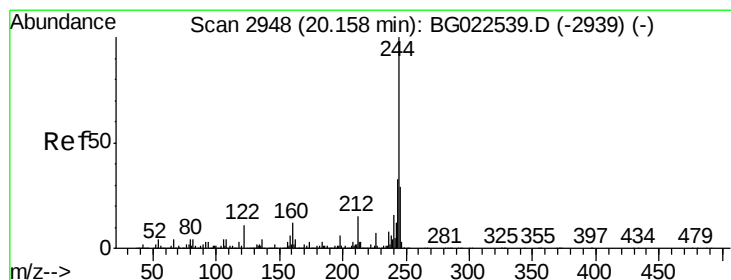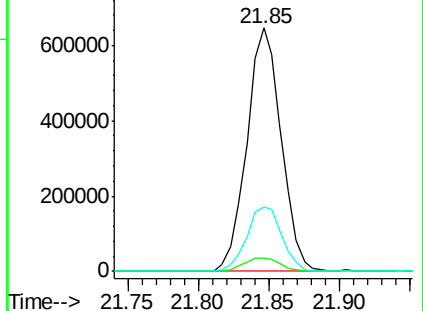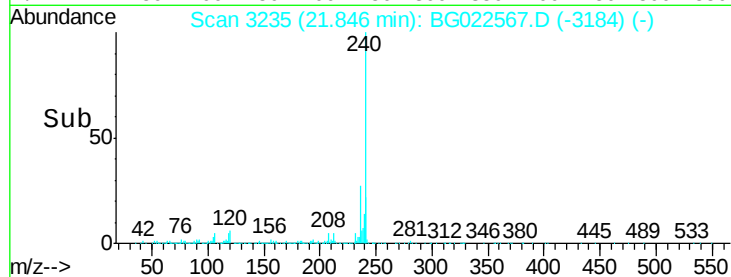

#78

Terphenyl-d14

Concen: 71.97 ng

RT: 20.16 min Scan# 2948

Delta R.T. 0.01 min

Lab File: BG022567.D

Acq: 25 Jun 2016 10:07


Tgt Ion:244 Resp: 2978988

Ion Ratio Lower Upper

244 100

212 15.1 10.8 16.2



122 10.7 8.0 12.0

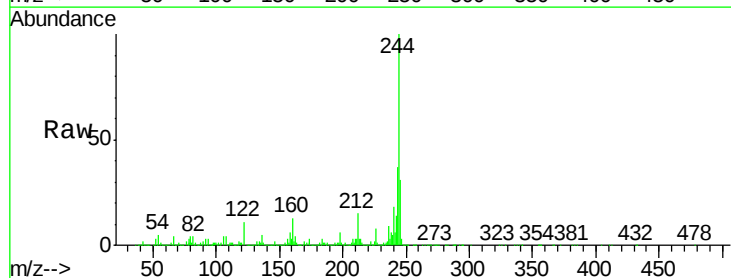


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

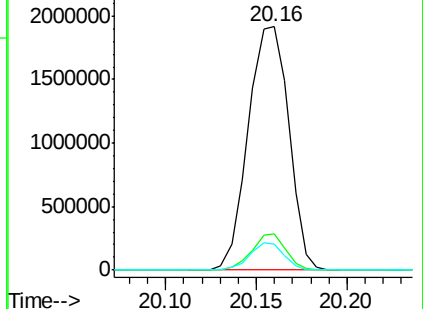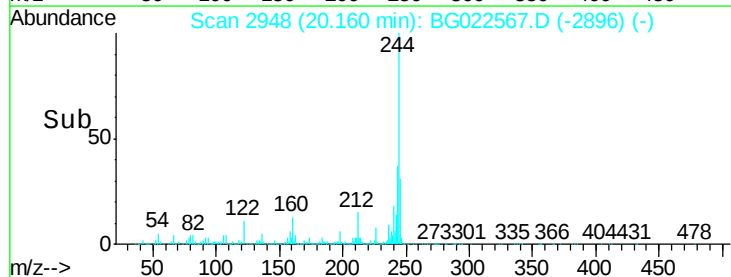

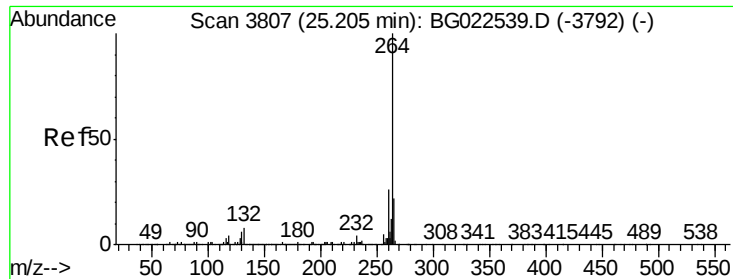

#86
Perylene-d12
Concen: 20.00 ng
RT: 25.21 min Scan# 3807
Delta R.T. 0.00 min
Lab File: BG022567.D
Acq: 25 Jun 2016 10:07

Instrument :
BNA_G
ClientSampleId :
TEPMW9S

Tgt Ion: 264 Resp: 1146566

Ion	Ratio	Lower	Upper
264	100		
260	23.6	18.4	27.6
265	21.3	18.9	28.3

