
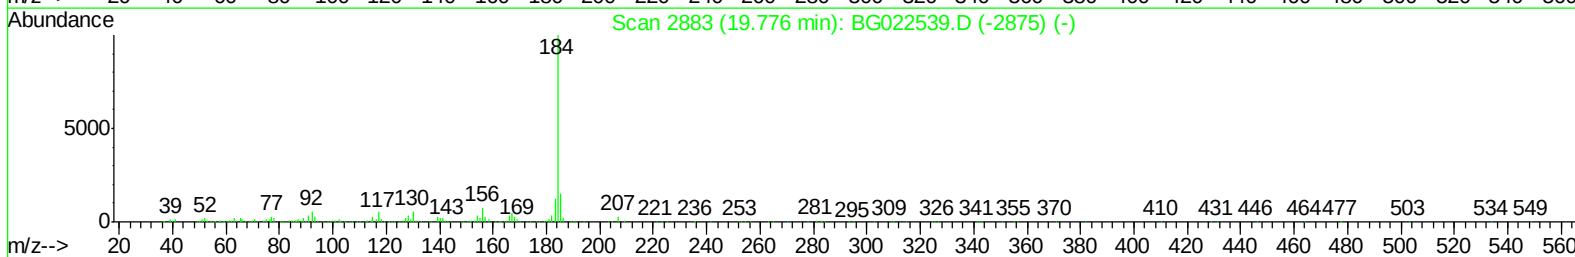
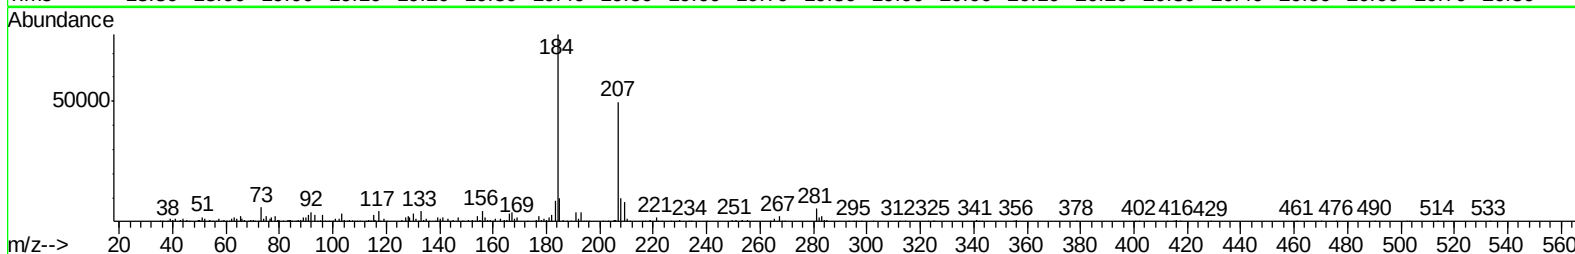


Data Path : Z:\HPCHEM1\BNA_G\Data\BG062516\
Data File : BG022535.D
Acq On : 24 Jun 2016 11:49
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 08:24:43 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

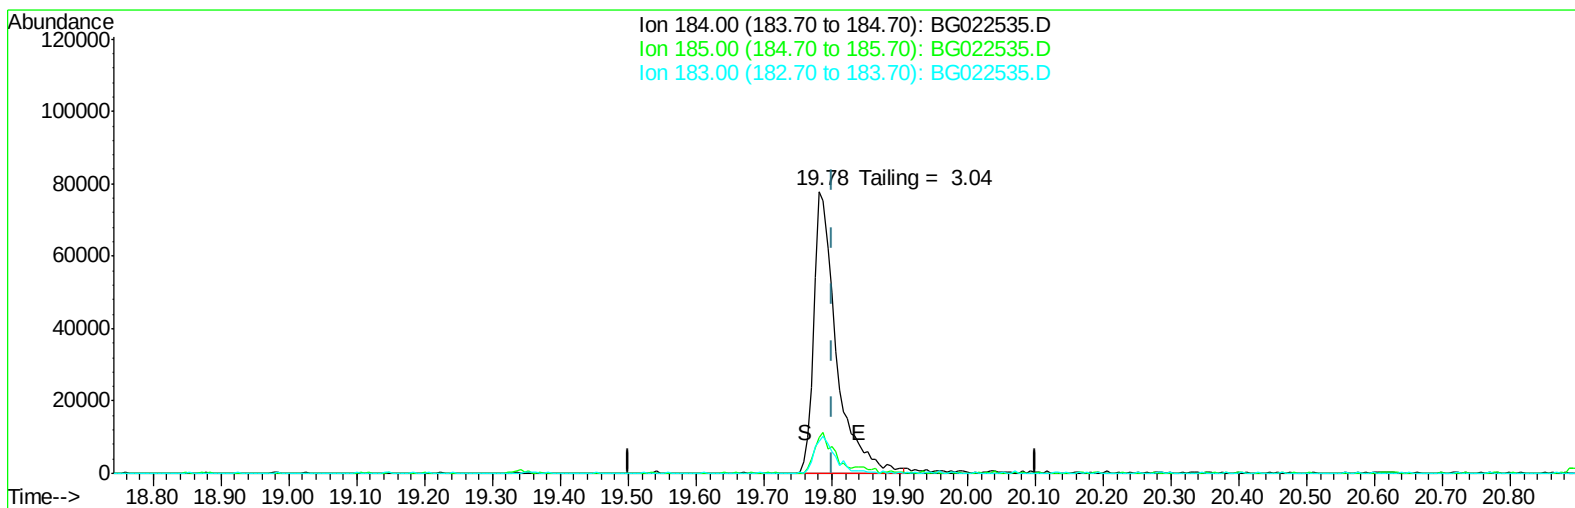

TIC: BG022535.D

(76) Benzidine




19.782min (-0.019) 113057.98ng

response 178146

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	12.58#
183.00	13.40	11.21
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG062516\
Data File : BG022535.D
Acq On : 24 Jun 2016 11:49
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 08:24:43 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

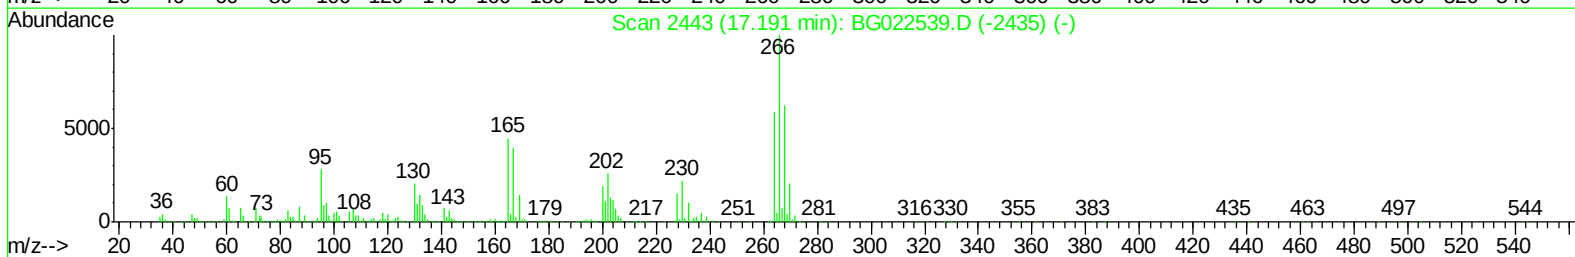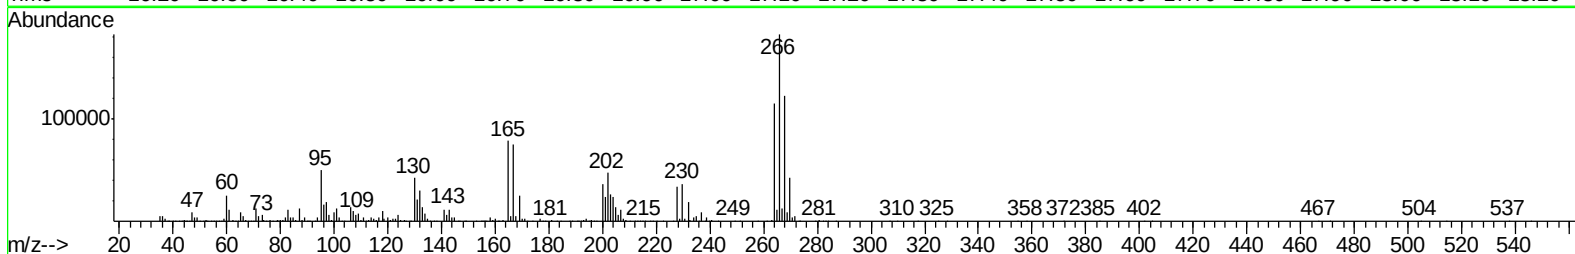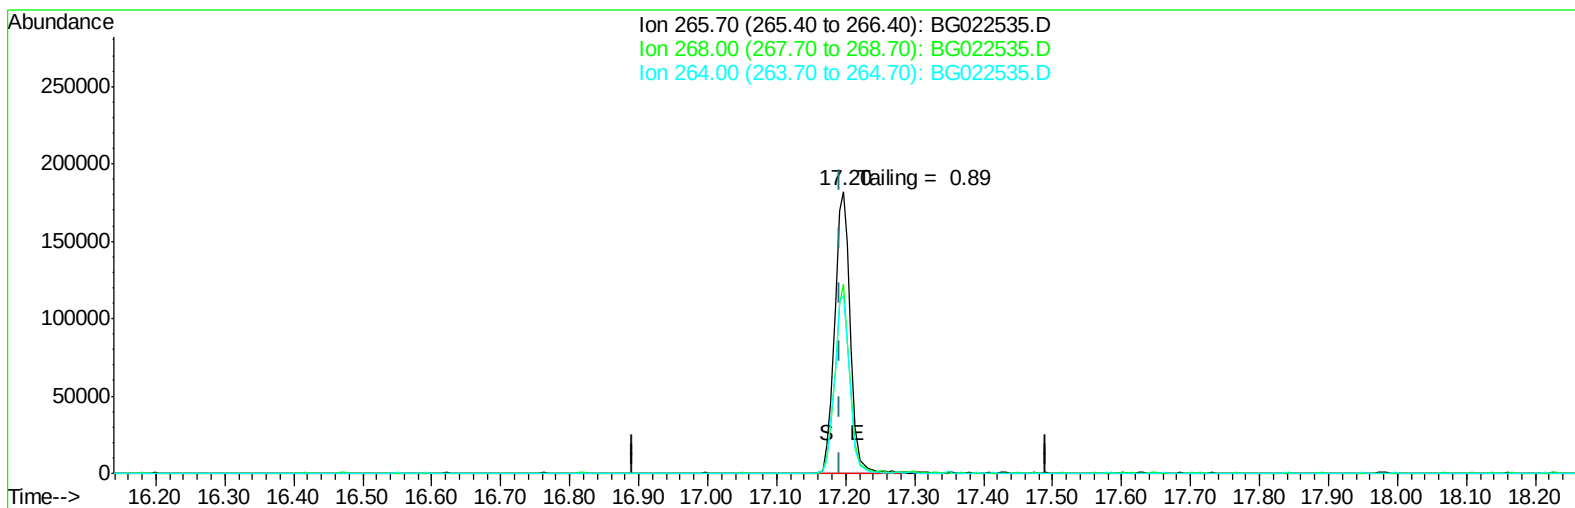

TIC: BG022535.D

(69) Pentachlorophenol (C)

17.197min (+0.005) 460893.43ng

response 287158

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	67.20
264.00	63.20	63.18
0.00	0.00	0.00