
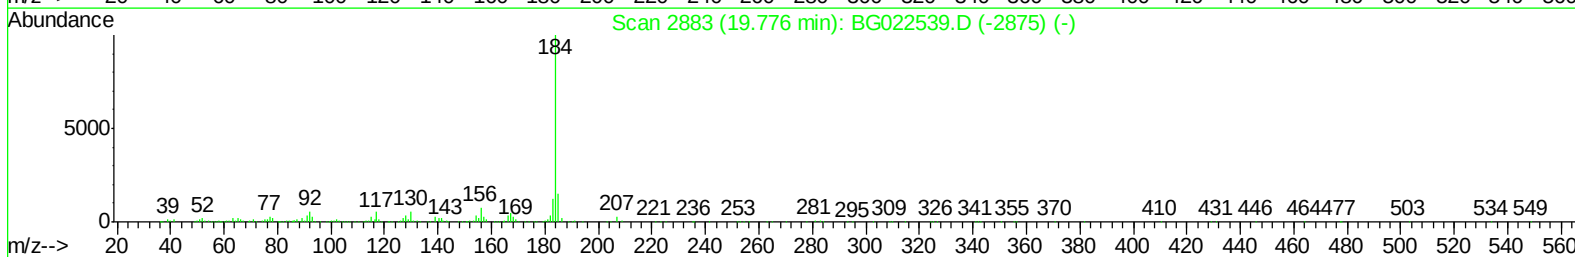
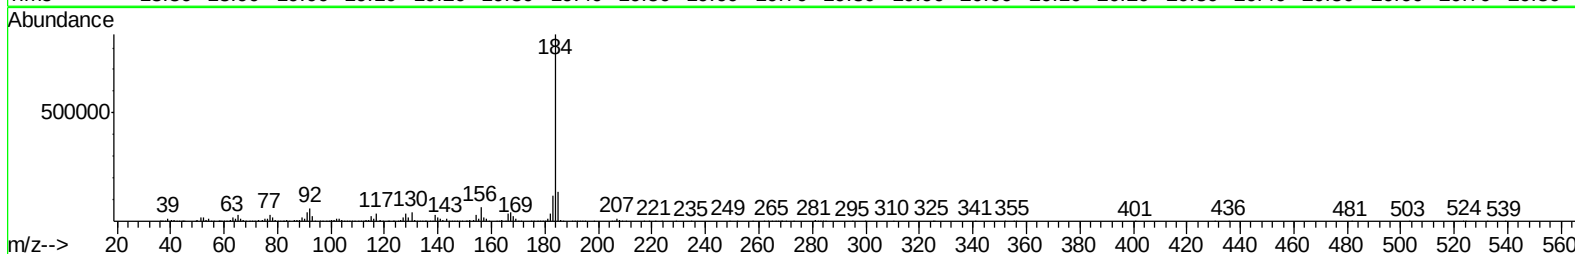


Data Path : Z:\HPCHEM1\BNA_G\Data\BG062516\
 Data File : BG022562.D
 Acq On : 25 Jun 2016 6:47
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 08:27:13 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 20:14:59 2016
 Response via : Initial Calibration

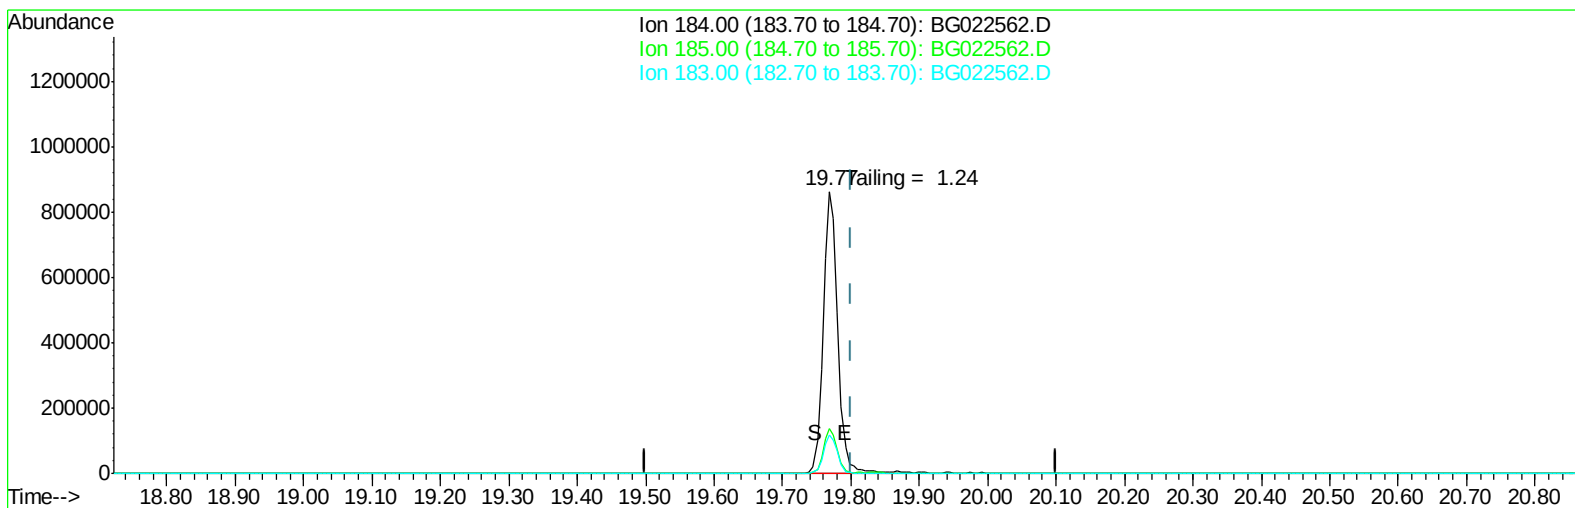

TIC: BG022562.D

(76) Benzidine




19.768min (-0.032) 141129.87ng

response 1283187

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	16.01
183.00	13.40	13.51
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG062516\
Data File : BG022562.D
Acq On : 25 Jun 2016 6:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 08:27:13 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

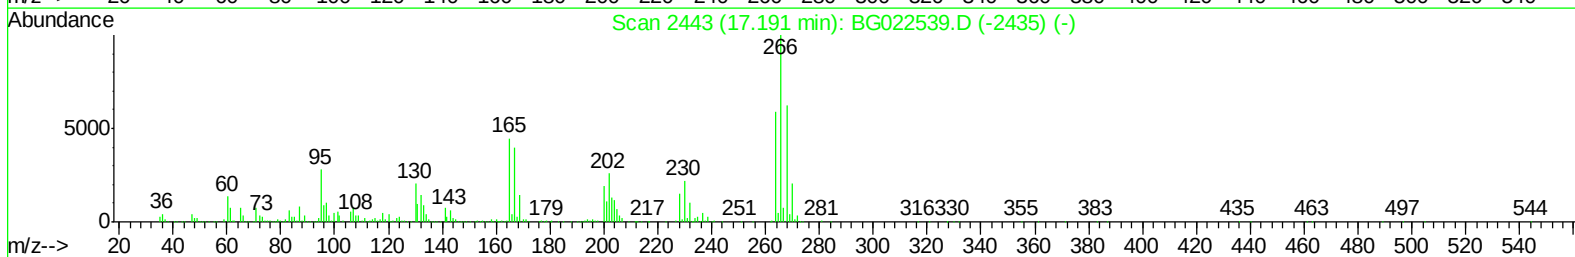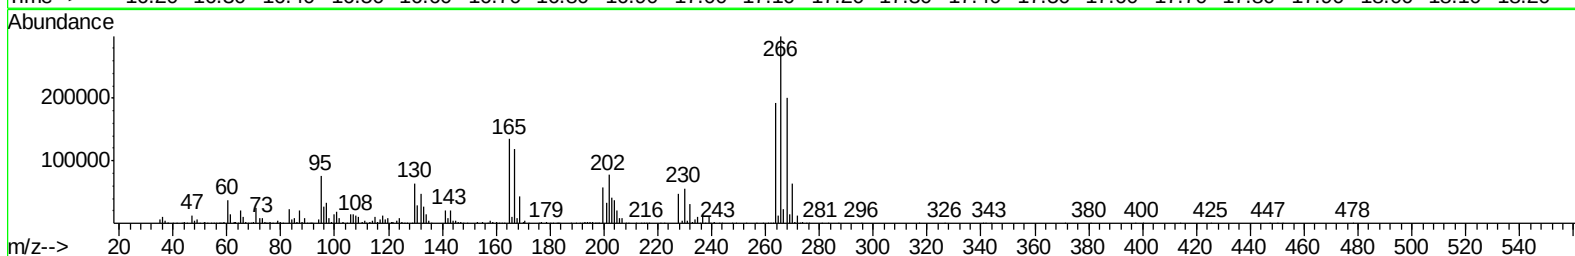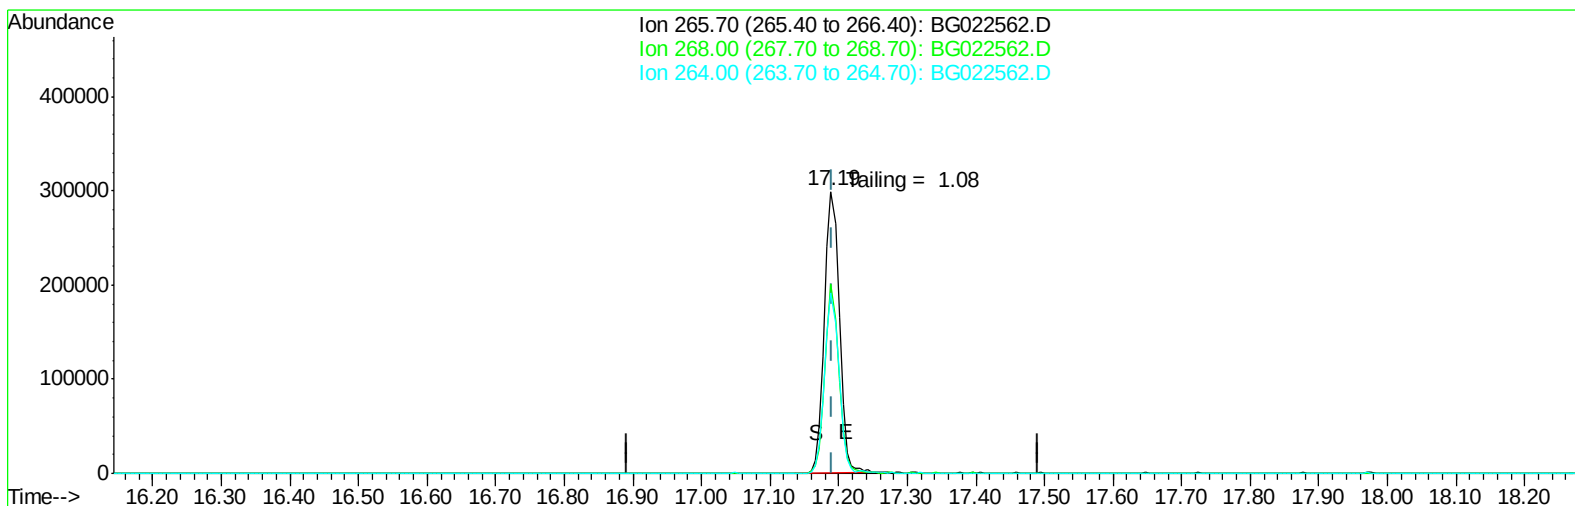

TIC: BG022562.D

(69) Pentachlorophenol (C)

17.189min (-0.003) 62114.31ng

response 454433

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	67.48
264.00	63.20	64.27
0.00	0.00	0.00