

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062516\
 Data File : BG022545.D
 Acq On : 24 Jun 2016 19:27
 Operator : UM/SJ
 Sample : H3625-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SC-STA-1501(0-4)

Quant Time: Jun 27 14:16:58 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 20:14:59 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	132928	20.00	ng	0.00
21) Naphthalene-d8	10.99	136	530209	20.00	ng	0.00
38) Acenaphthene-d10	14.81	164	287871	20.00	ng	0.00
63) Phenanthrene-d10	17.56	188	840324	20.00	ng	0.00
75) Chrysene-d12	21.84	240	803263	20.00	ng	0.00
86) Perylene-d12	25.20	264	93778	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.71	112	1086513	131.10	ng	0.00
7) Phenol-d6	7.31	99	1360835	116.49	ng	0.00
23) Nitrobenzene-d5	9.34	82	1209424	96.54	ng	0.00
41) 2,4,6-Tribromophenol	16.29	330	786876	173.79	ng	0.00
44) 2-Fluorobiphenyl	13.43	172	2159612	118.97	ng	0.00
78) Terphenyl-d14	20.16	244	3054166	100.74	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062516\
Data File : BG022545.D
Acq On : 24 Jun 2016 19:27
Operator : UM/SJ
Sample : H3625-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SC-STA-1501(0-4)

Quant Time: Jun 27 14:16:58 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

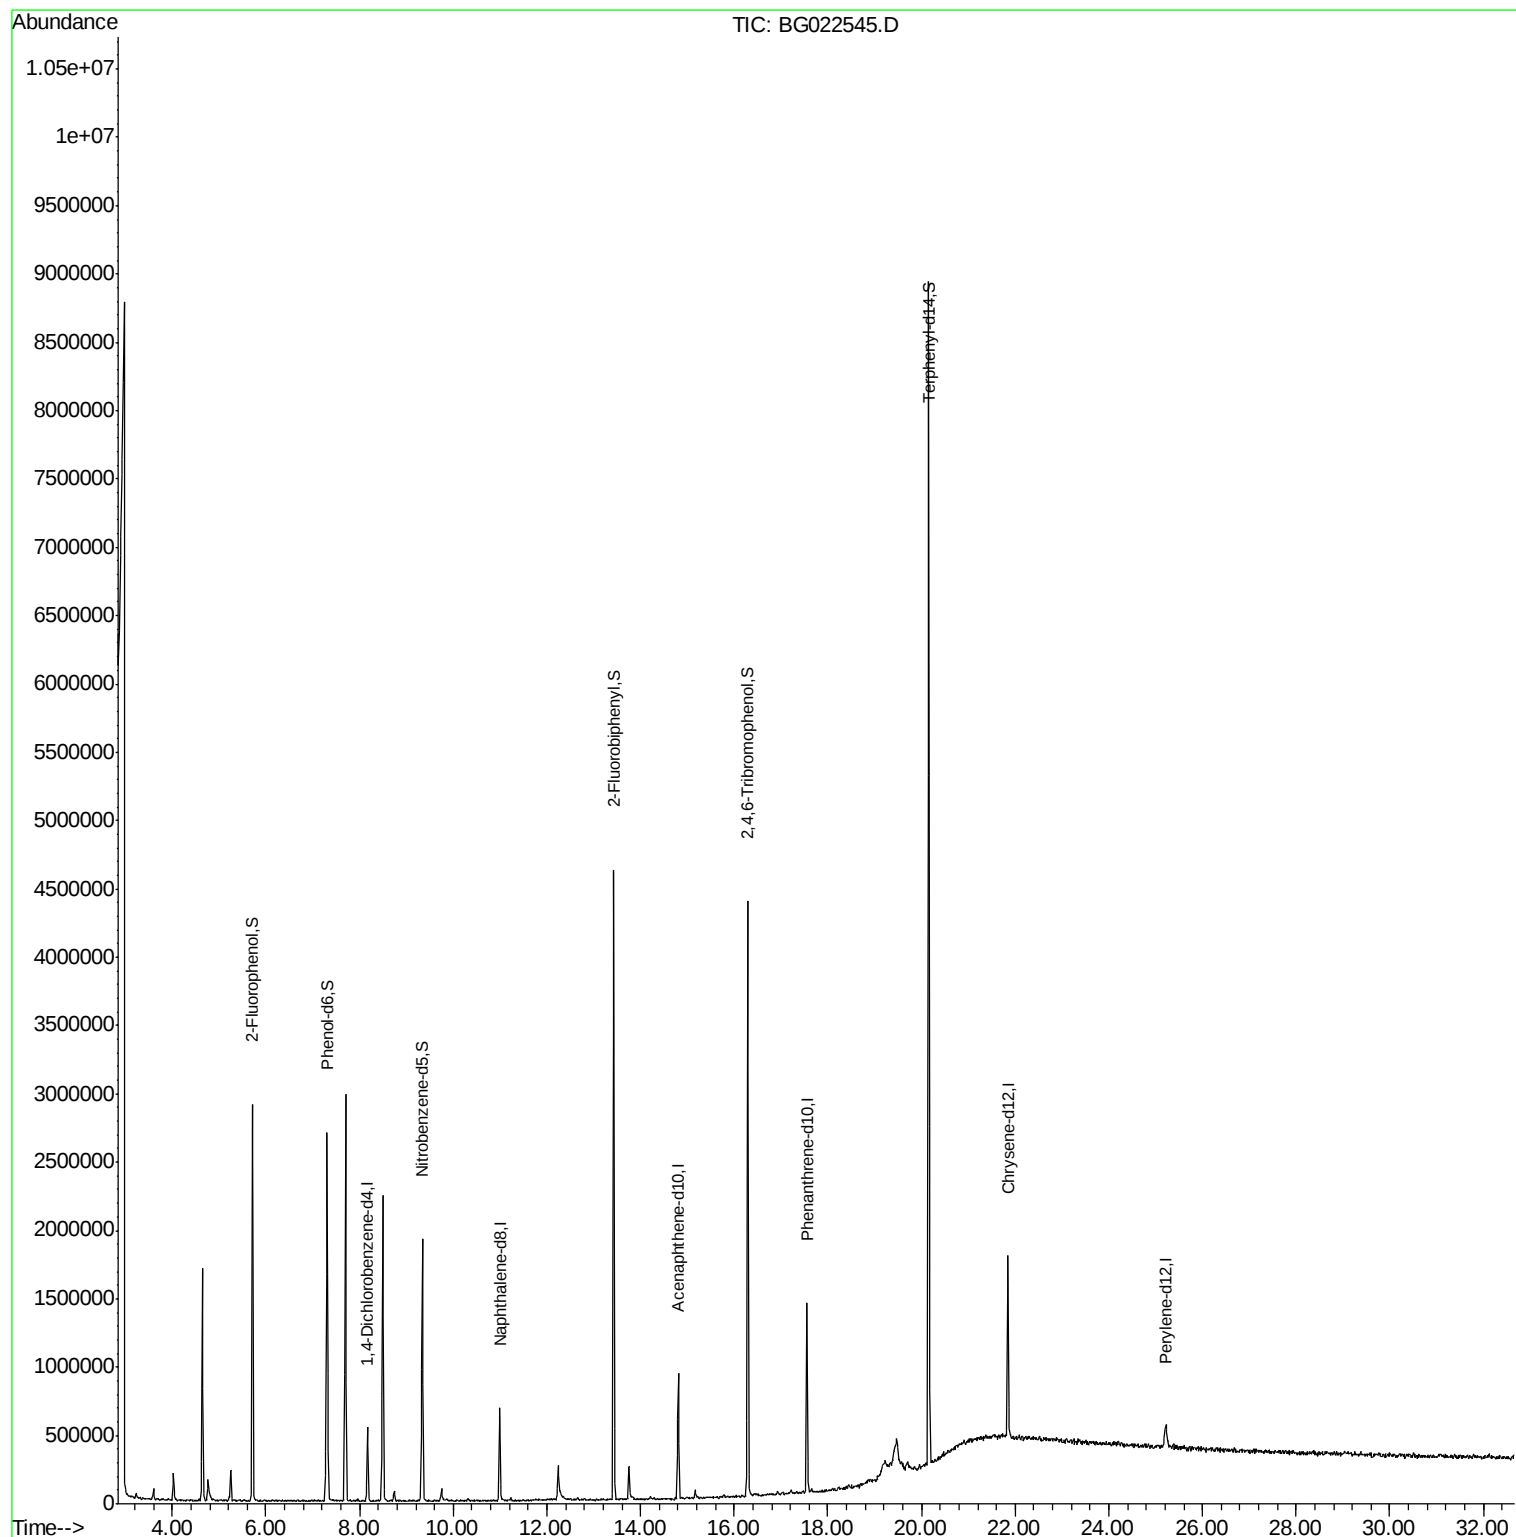

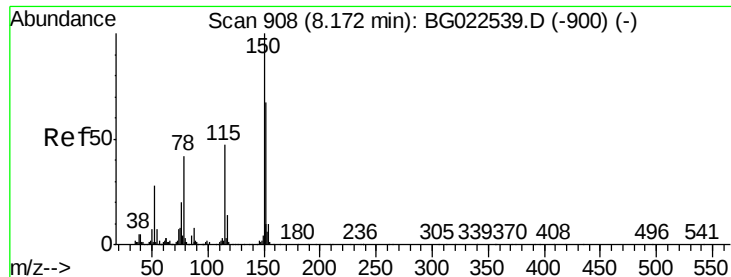

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.17 min Scan# 908

Delta R.T. -0.00 min

Lab File: BG022545.D

Acq: 24 Jun 2016 19:27

Instrument :

BNA_G

ClientSampleId :

SC-STA-1501(0-4)


Tgt Ion:152 Resp: 132928

Ion Ratio Lower Upper

152 100

150 161.0 144.7 217.1




115 69.8 64.0 96.0

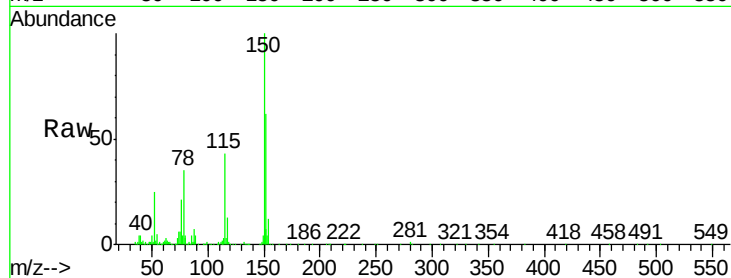

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

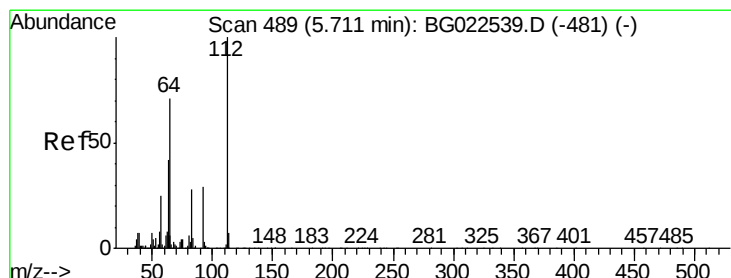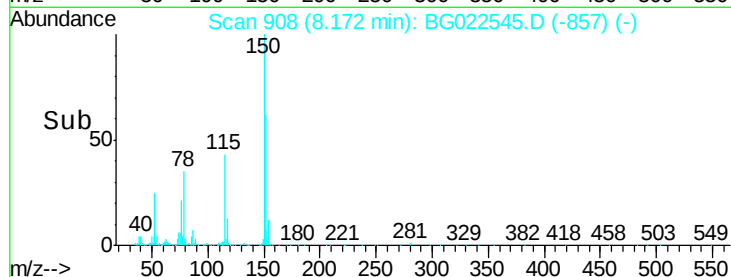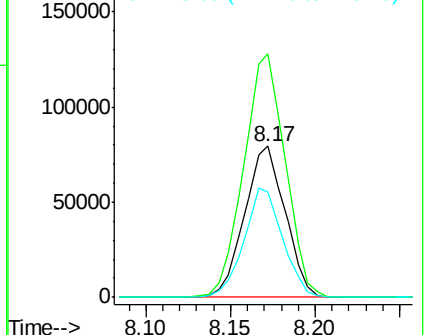

#5

2-Fluorophenol

Concen: 131.10 ng

RT: 5.71 min Scan# 489

Delta R.T. 0.01 min

Lab File: BG022545.D

Acq: 24 Jun 2016 19:27


Tgt Ion:112 Resp: 1086513

Ion Ratio Lower Upper

112 100

64 72.7 59.0 88.4



63 43.6 37.8 56.8

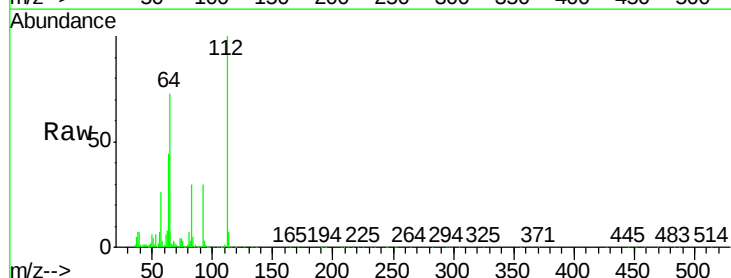

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

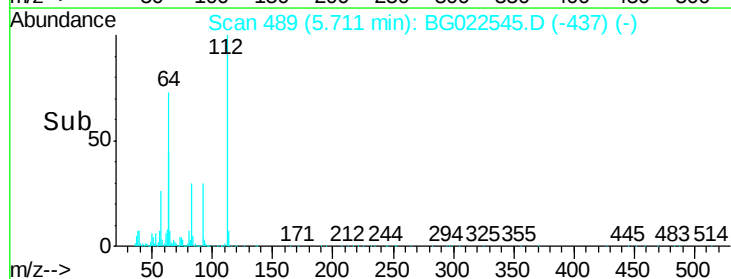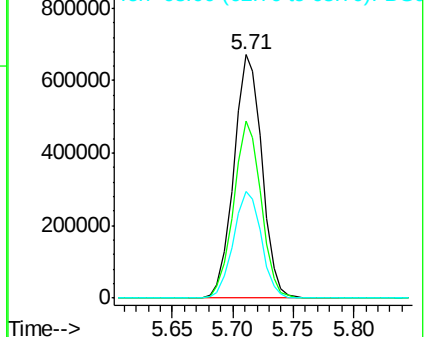



#7

Phenol-d6

Concen: 116.49 ng

RT: 7.31 min Scan# 761

Delta R.T. 0.01 min

Lab File: BG022545.D

Acq: 24 Jun 2016 19:27

Instrument :

BNA_G

ClientSampleId :

SC-STA-1501(0-4)


Tgt Ion: 99 Resp: 1360835

Ion Ratio Lower Upper



99 100

42 21.6 17.8 26.6

71 52.5 41.5 62.3

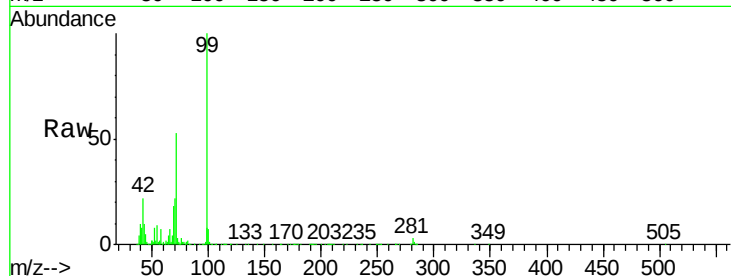

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

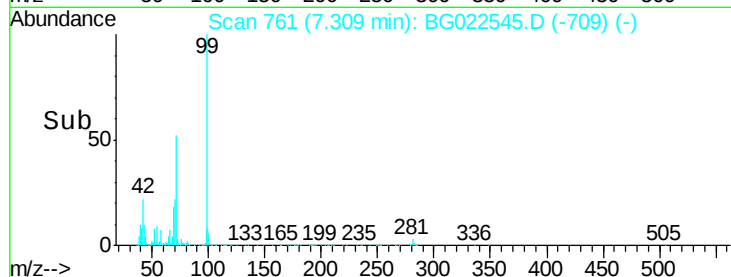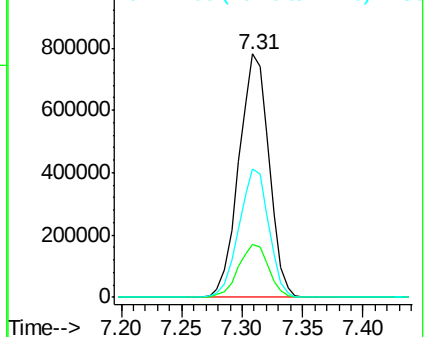

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.99 min Scan# 1388

Delta R.T. -0.00 min

Lab File: BG022545.D

Acq: 24 Jun 2016 19:27

Tgt Ion: 136 Resp: 530209


Ion Ratio Lower Upper

136 100



137 13.3 9.6 14.4


54 9.6 7.3 10.9

68 7.4 5.3 7.9

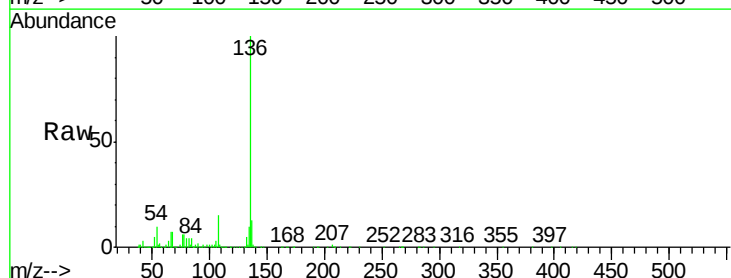

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



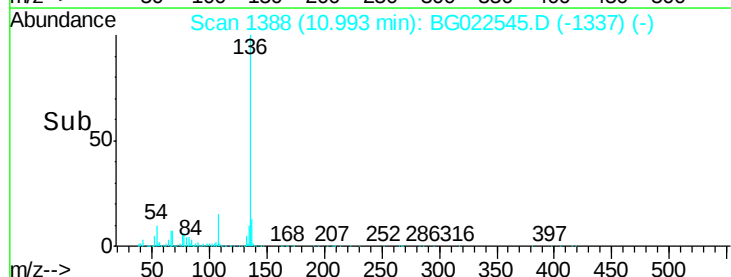
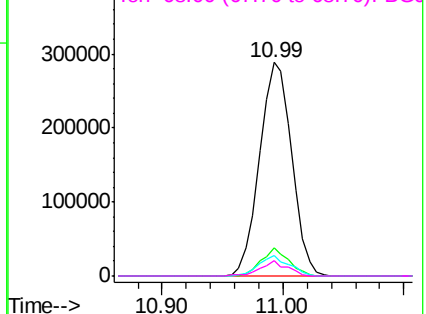


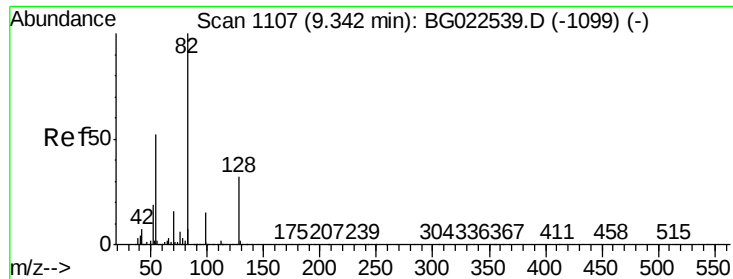

#23
Nitrobenzene-d5
Concen: 96.54 ng
RT: 9.34 min Scan# 1106
Delta R.T. -0.00 min
Lab File: BG022545.D
Acq: 24 Jun 2016 19:27




Instrument :
BNA_G
ClientSampleId :
SC-STA-1501(0-4)


Tgt Ion: 82 Resp: 1209424
Ion Ratio Lower Upper
82 100
128 31.8 24.4 36.6
54 49.7 41.4 62.0

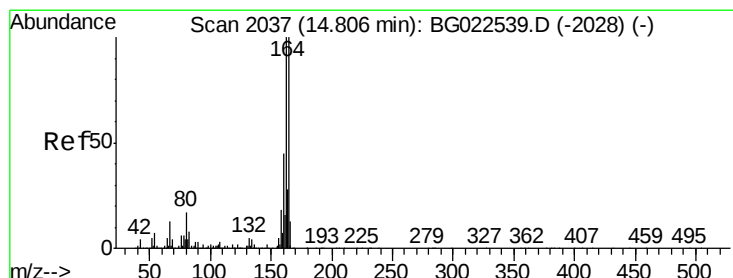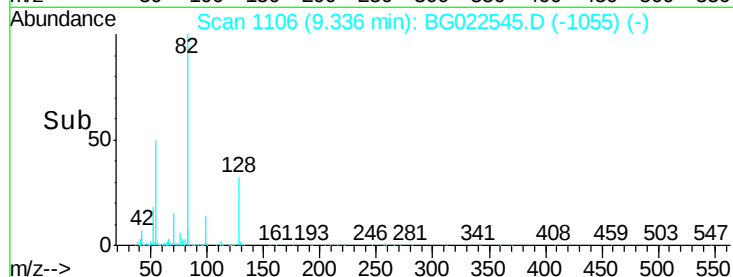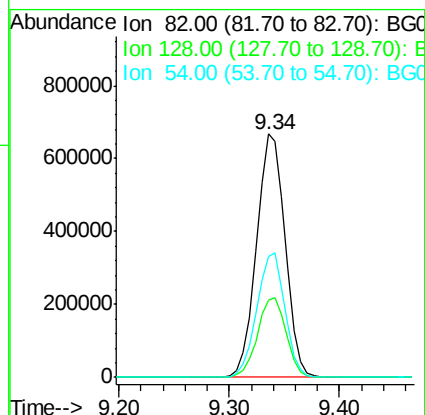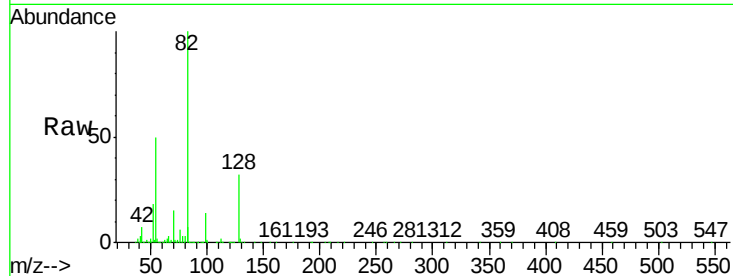

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.81 min Scan# 2037
Delta R.T. 0.01 min
Lab File: BG022545.D
Acq: 24 Jun 2016 19:27

Tgt Ion: 164 Resp: 287871
Ion Ratio Lower Upper
164 100
162 102.6 87.7 131.5
160 44.8 37.2 55.8

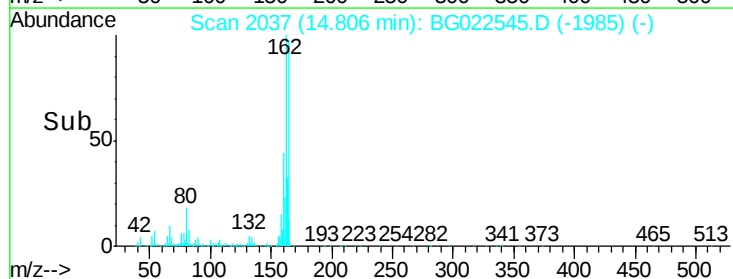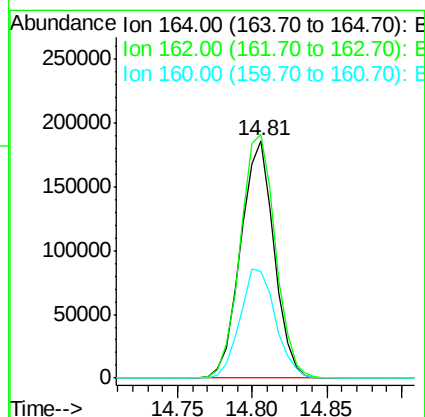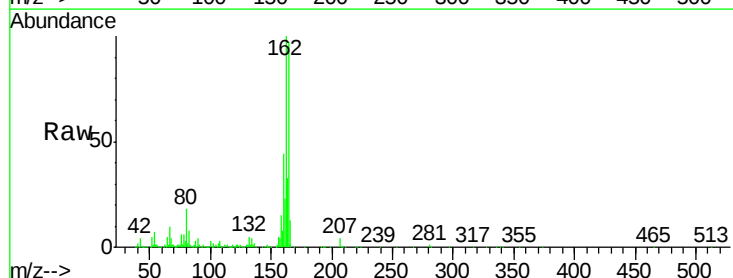


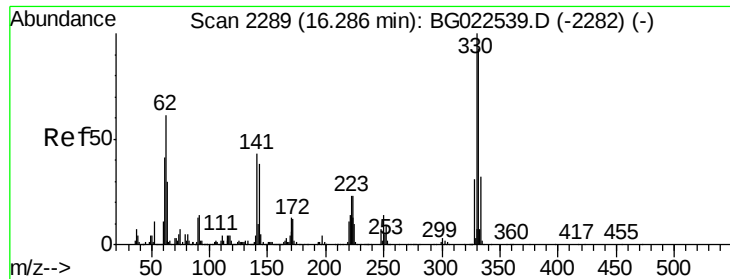




#41
 2,4,6-Tribromophenol
 Concen: 173.79 ng
 RT: 16.29 min Scan# 2290
 Delta R.T. 0.01 min
 Lab File: BG022545.D
 Acq: 24 Jun 2016 19:27

Instrument :
 BNA_G
 ClientSampleId :
 SC-STA-1501(0-4)

Tgt Ion:330 Resp: 786876
 Ion Ratio Lower Upper
 330 100
 332 97.0 77.4 116.2
 141 39.3 31.7 47.5

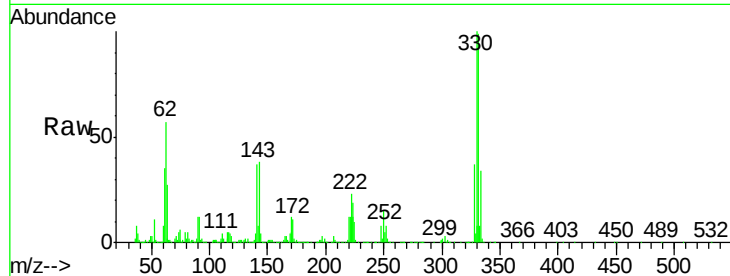


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

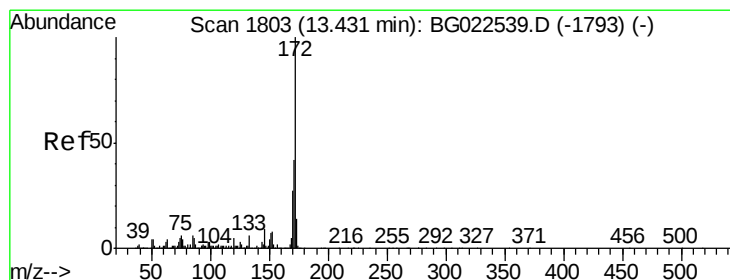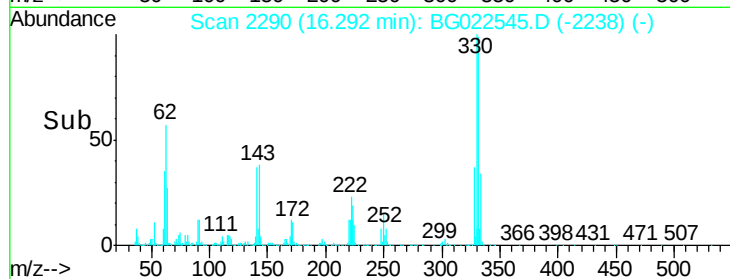
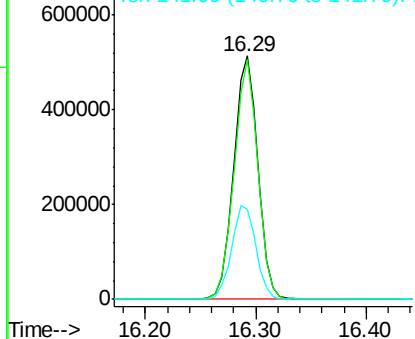



#44
 2-Fluorobiphenyl
 Concen: 118.97 ng
 RT: 13.43 min Scan# 1802
 Delta R.T. -0.00 min
 Lab File: BG022545.D
 Acq: 24 Jun 2016 19:27

Tgt Ion:172 Resp: 2159612
 Ion Ratio Lower Upper
 172 100
 171 43.1 31.6 47.4
 170 28.6 21.3 31.9

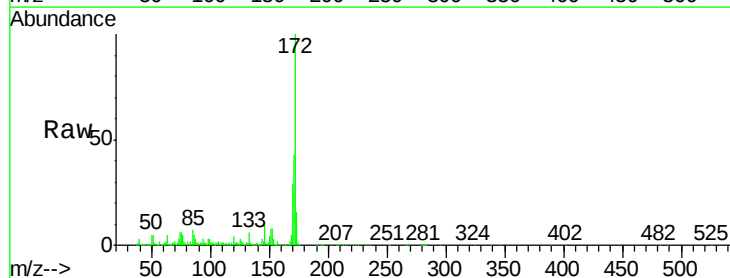

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

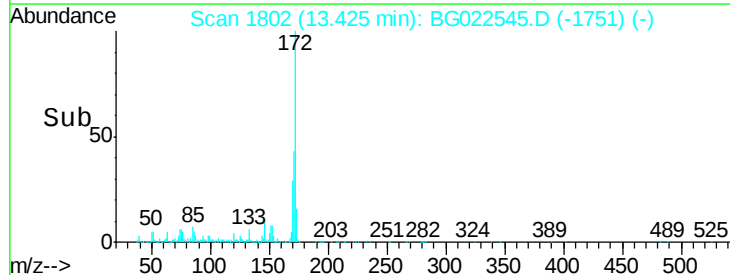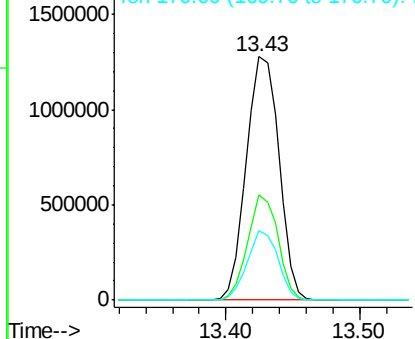

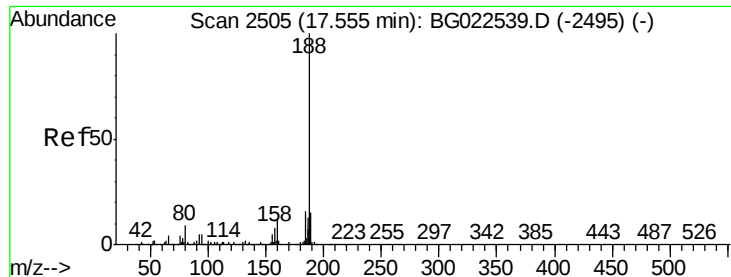

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.56 min Scan# 2505

Delta R.T. 0.01 min

Lab File: BG022545.D

Acq: 24 Jun 2016 19:27

Instrument :

BNA_G

ClientSampleId :

SC-STA-1501(0-4)


Tgt Ion:188 Resp: 840324

Ion Ratio Lower Upper

188 100

94 7.0 5.2 7.8




80 8.5 7.2 10.8

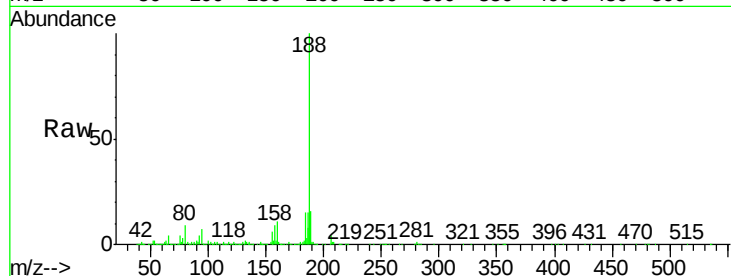

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

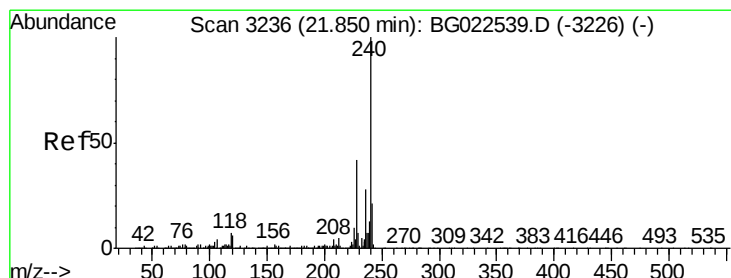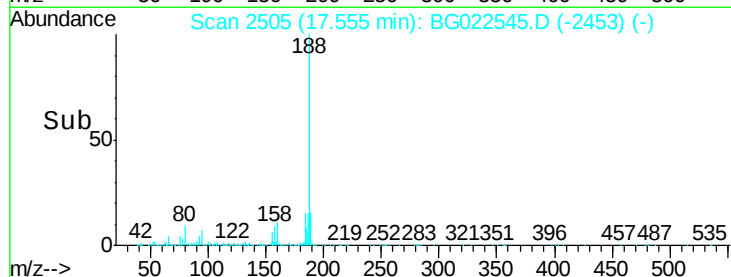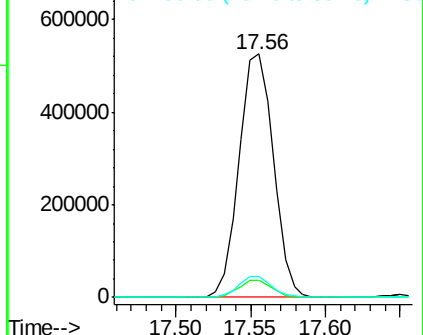

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.84 min Scan# 3235

Delta R.T. -0.00 min

Lab File: BG022545.D

Acq: 24 Jun 2016 19:27


Tgt Ion:240 Resp: 803263

Ion Ratio Lower Upper

240 100

120 5.8 4.1 6.1



236 28.8 21.1 31.7

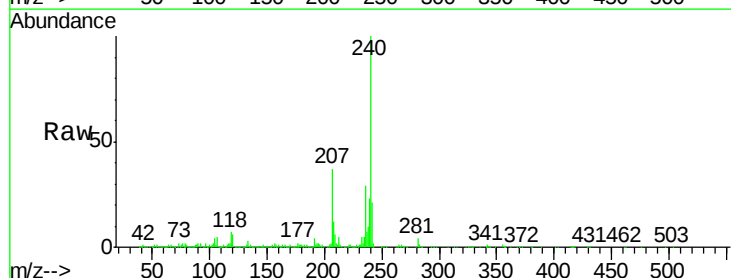


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

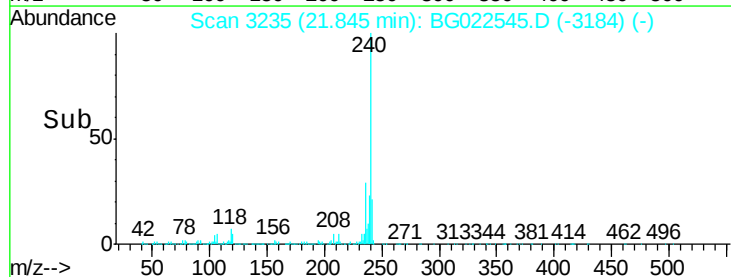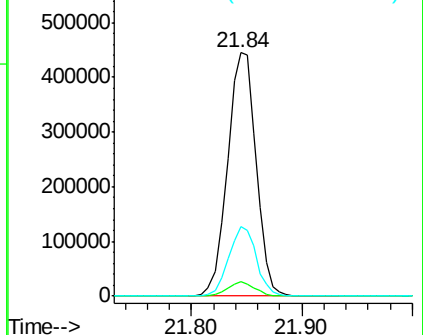

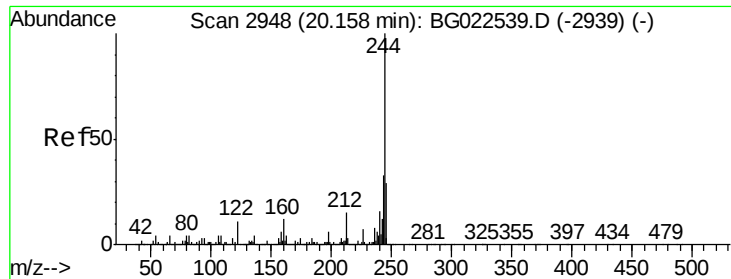

#78

Terphenyl-d14

Concen: 100.74 ng

RT: 20.16 min Scan# 2948

Delta R.T. 0.01 min

Lab File: BG022545.D

Acq: 24 Jun 2016 19:27

Instrument :

BNA_G

ClientSampleId :

SC-STA-1501(0-4)


Tgt Ion:244 Resp: 3054166

Ion Ratio Lower Upper

244 100

212 15.3 10.8 16.2




122 10.5 8.0 12.0

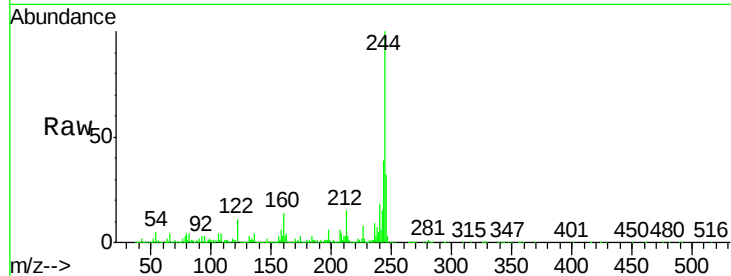

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

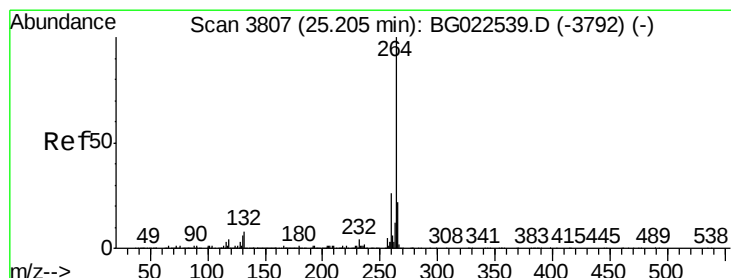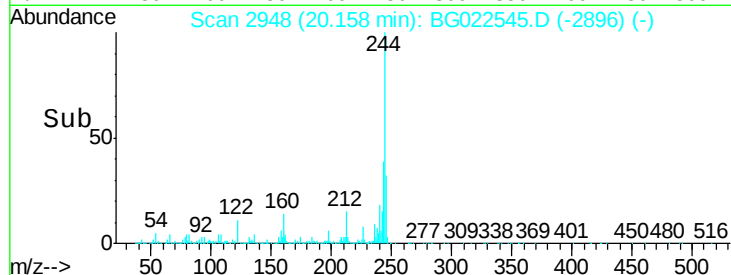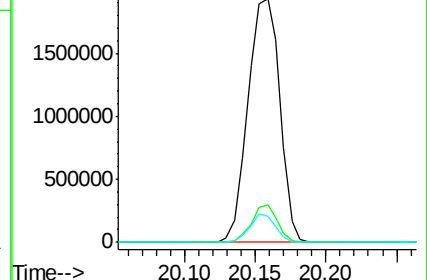

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.20 min Scan# 3806

Delta R.T. -0.01 min

Lab File: BG022545.D

Acq: 24 Jun 2016 19:27


Tgt Ion:264 Resp: 93778

Ion Ratio Lower Upper

264 100

260 33.0 18.4 27.6#

265 23.1 18.9 28.3

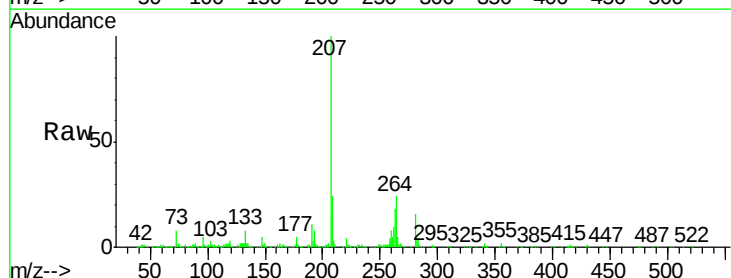

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

