


Data Path : Z:\HPCHEM1\BNA_G\Data\BG062516\
 Data File : BG022535.D
 Acq On : 24 Jun 2016 11:49
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 24 20:14:59 2016

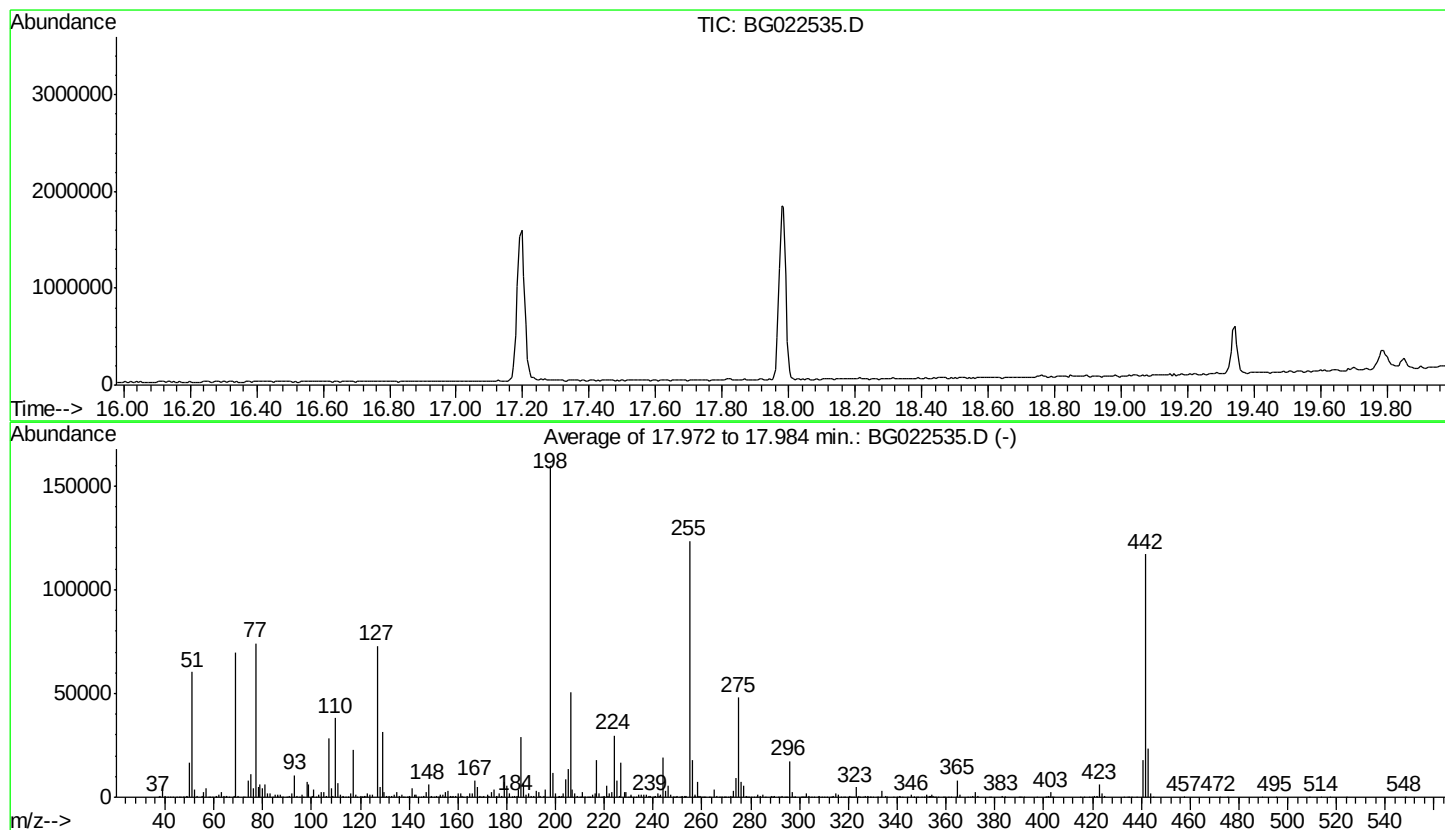

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2570

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	60298	PASS
68	69	0.00	2	0.6	401	PASS
69	198	0.00	100	43.5	69456	PASS
70	69	0.00	2	0.6	427	PASS
127	198	10	80	45.6	72901	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	159794	PASS
199	198	5	9	7.2	11498	PASS
275	198	10	60	30.1	48112	PASS
365	198	1	100	5.2	8323	PASS
441	442	0.01	24	15.3	17895	PASS
442	198	50	100	73.3	117205	PASS
443	442	15	24	20.1	23514	PASS