


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062516\
 Data File : BG022562.D
 Acq On : 25 Jun 2016 6:47
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 24 20:14:59 2016

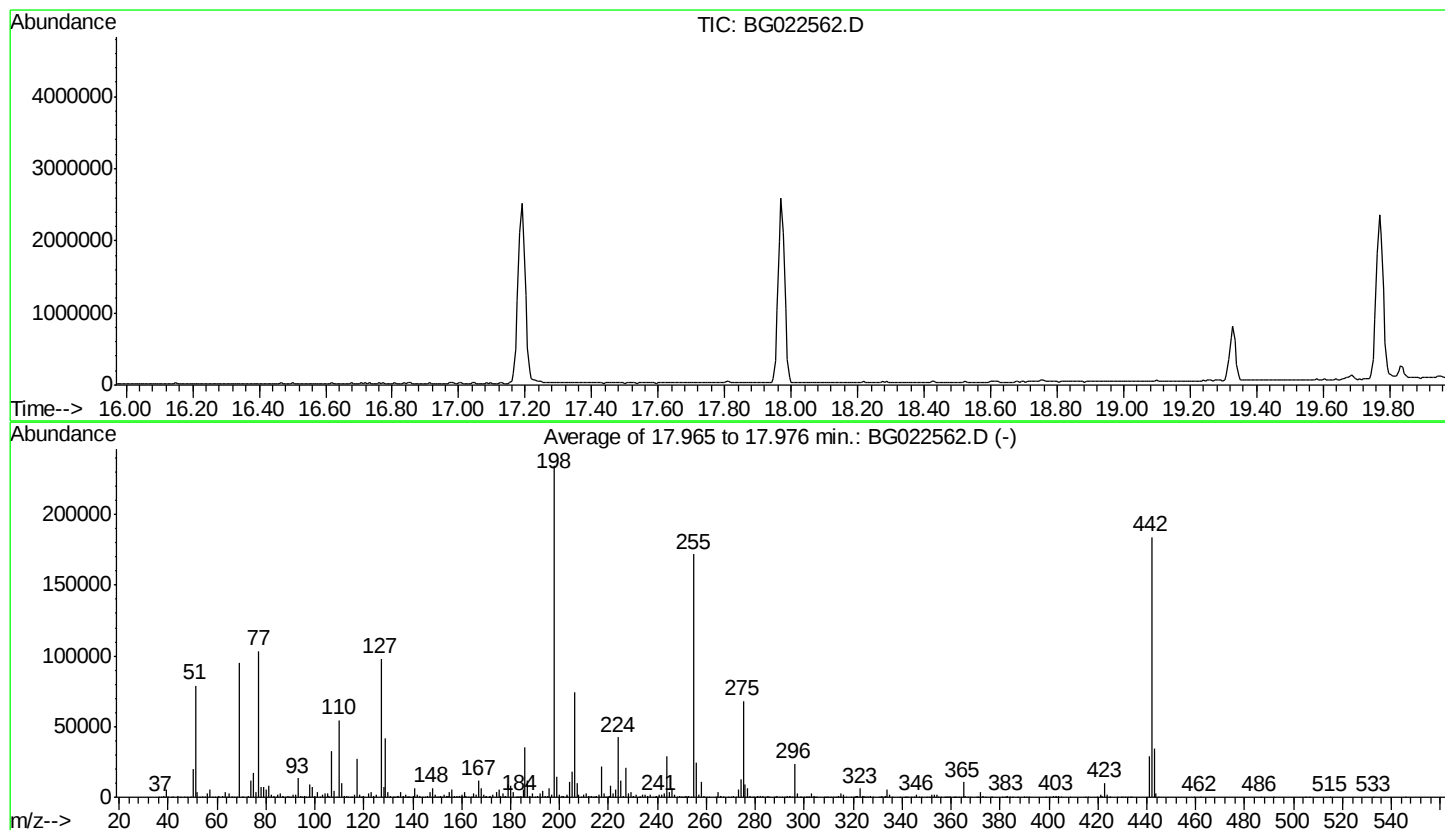

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2565

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	78933	PASS
68	69	0.00	2	0.4	362	PASS
69	198	0.00	100	40.4	94862	PASS
70	69	0.00	2	0.5	433	PASS
127	198	10	80	41.9	98274	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	234624	PASS
199	198	5	9	6.4	14901	PASS
275	198	10	60	29.0	68058	PASS
365	198	1	100	4.5	10521	PASS
441	442	0.01	24	16.0	29454	PASS
442	198	50	100	78.5	184085	PASS
443	442	15	24	18.8	34674	PASS