
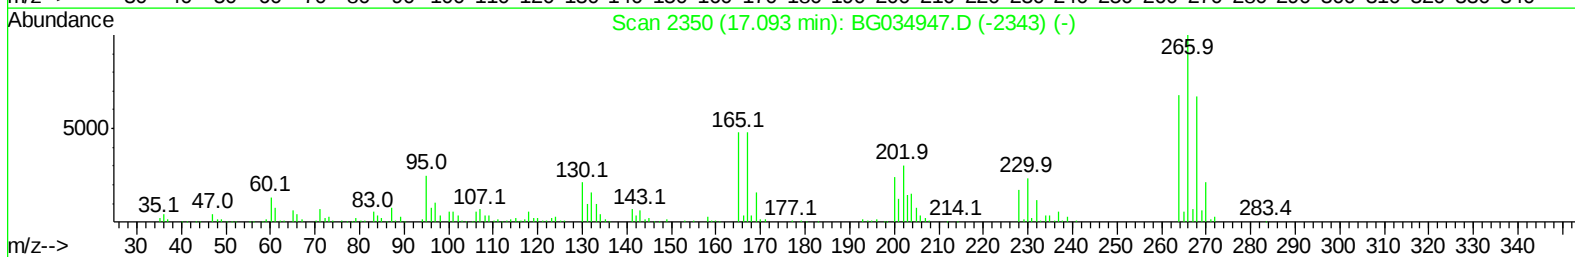
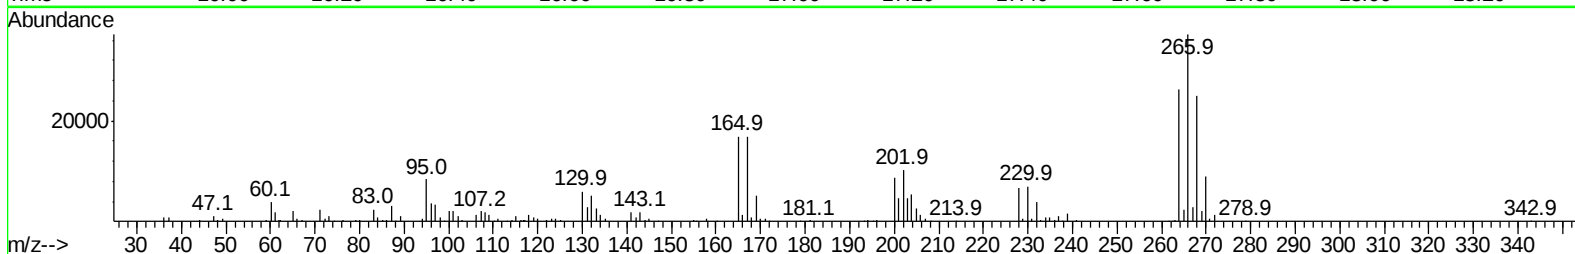


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062518\
Data File : BG035389.D
Acq On : 25 Jun 2018 23:22
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 08:29:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

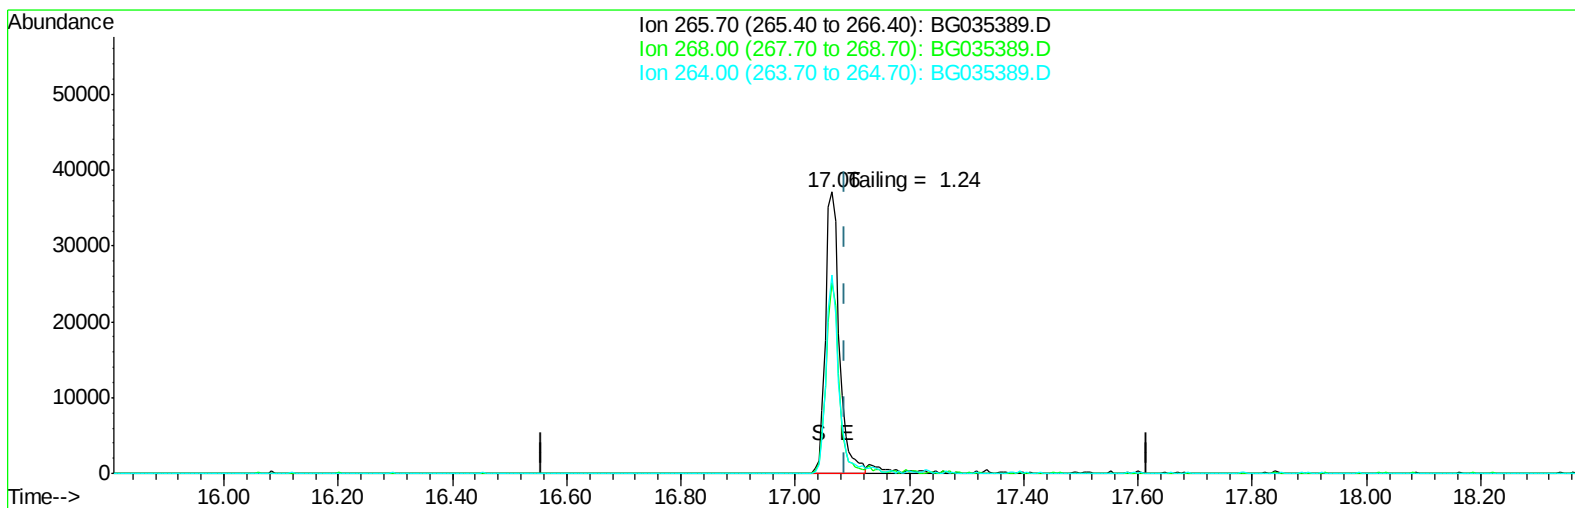

TIC: BG035389.D

(69) Pentachlorophenol (C)




17.064min (-0.023) 120463.80ng

response 62551

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.61
264.00	62.00	70.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062518\
 Data File : BG035389.D
 Acq On : 25 Jun 2018 23:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 08:29:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration

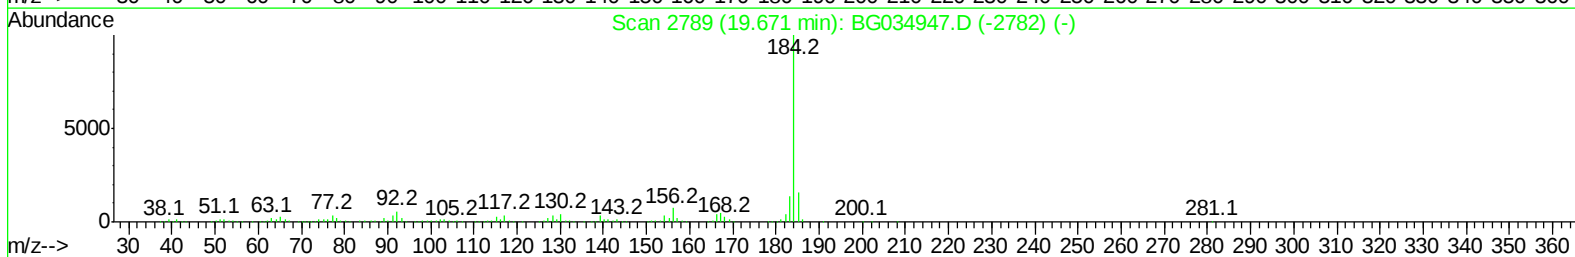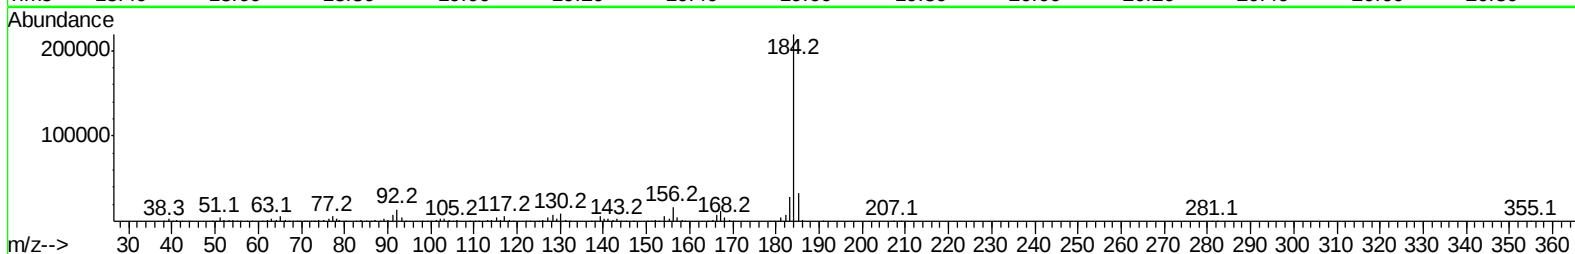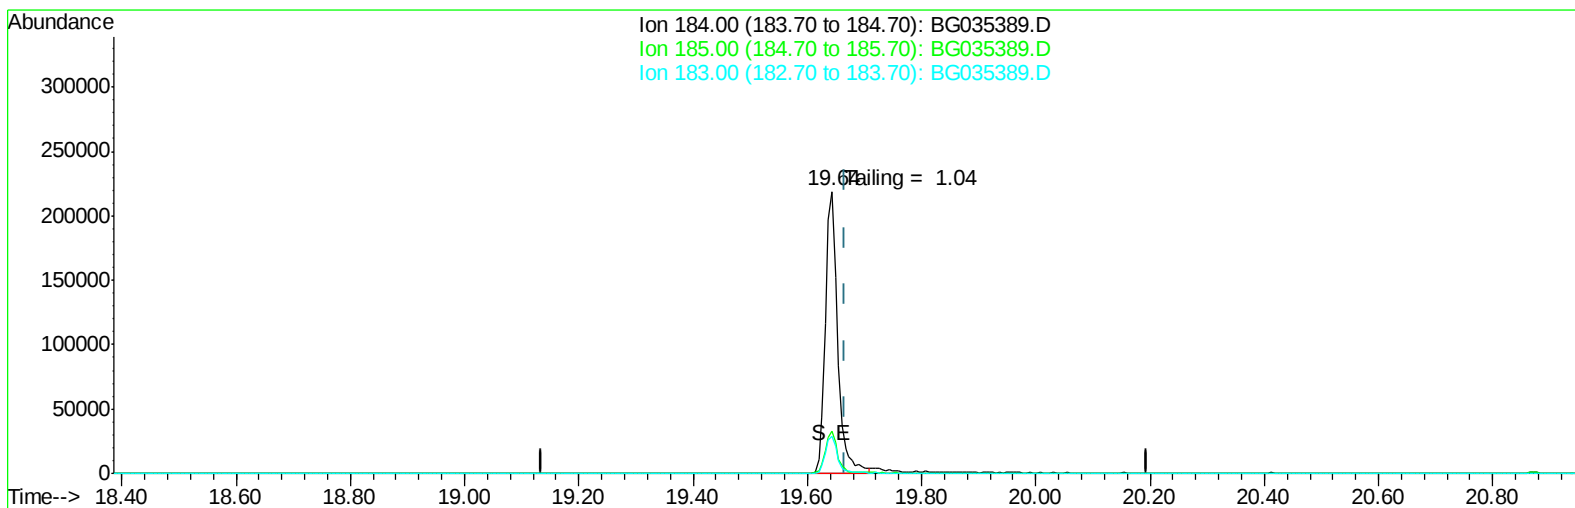

TIC: BG035389.D

(76) Benzidine

19.643min (-0.023) 0.00ng

response 338037

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.88
183.00	13.30	13.24
0.00	0.00	0.00