
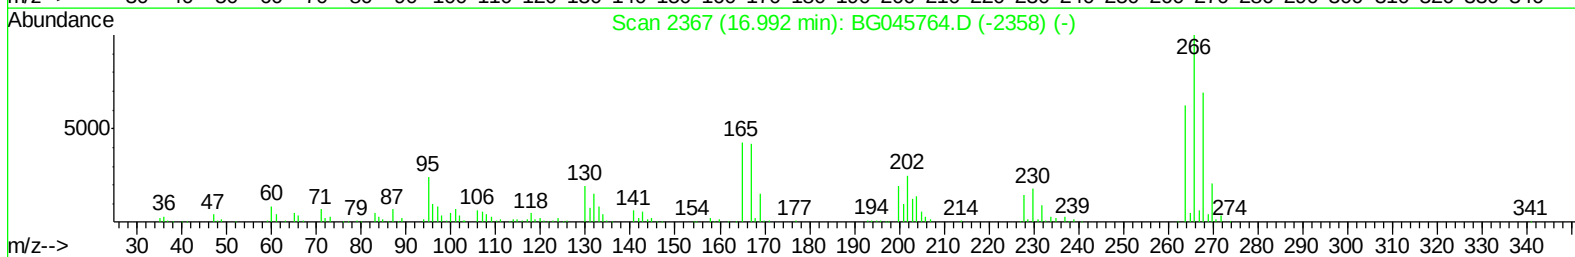
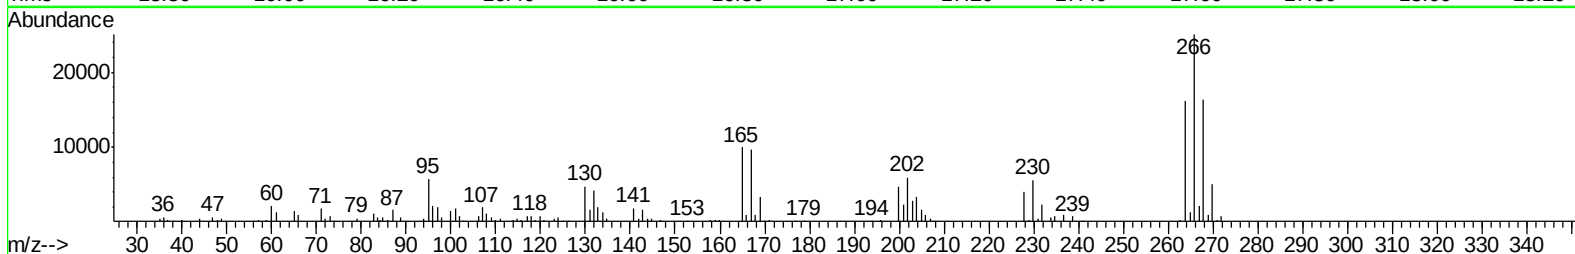


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062520\
Data File : BG045854.D
Acq On : 25 Jun 2020 12:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 00:41:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 25 15:44:32 2020
Response via : Initial Calibration

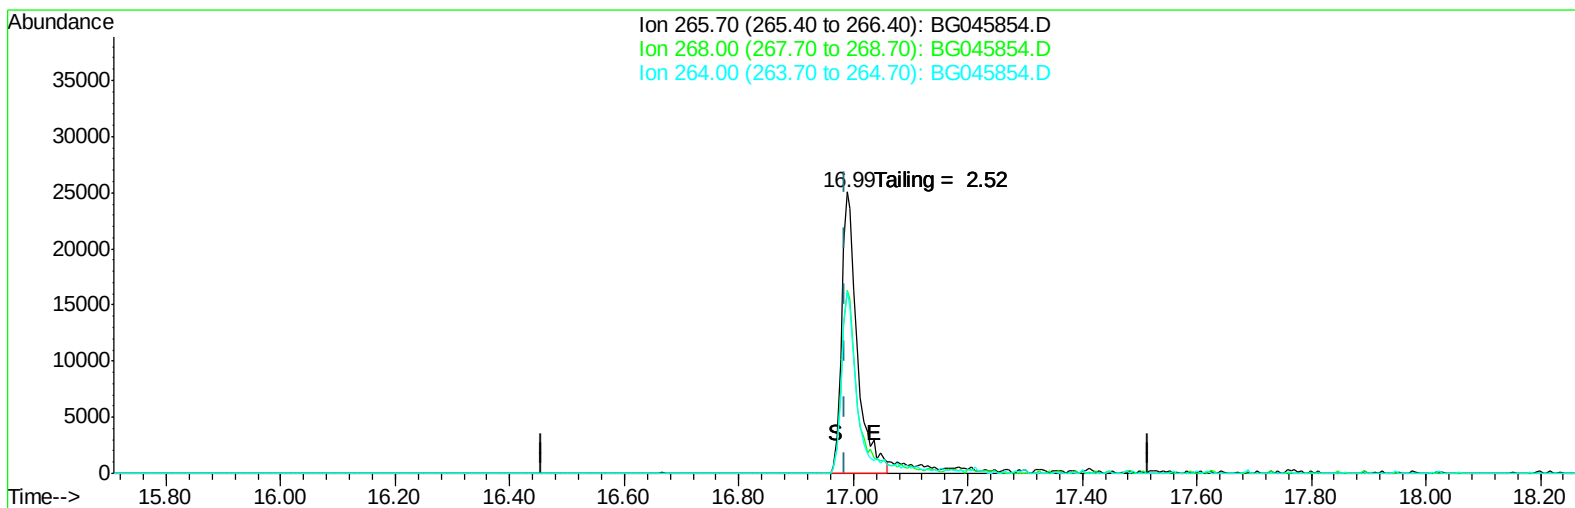

TIC: BG045854.D

(70) Pentachlorophenol (C)




16.989min (+0.003) 121622.88ng

response 47348

Ion	Exp%	Act%
265.70	100	100
268.00	69.20	65.14
264.00	62.20	64.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062520\
 Data File : BG045854.D
 Acq On : 25 Jun 2020 12:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 00:41:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 25 15:44:32 2020
 Response via : Initial Calibration

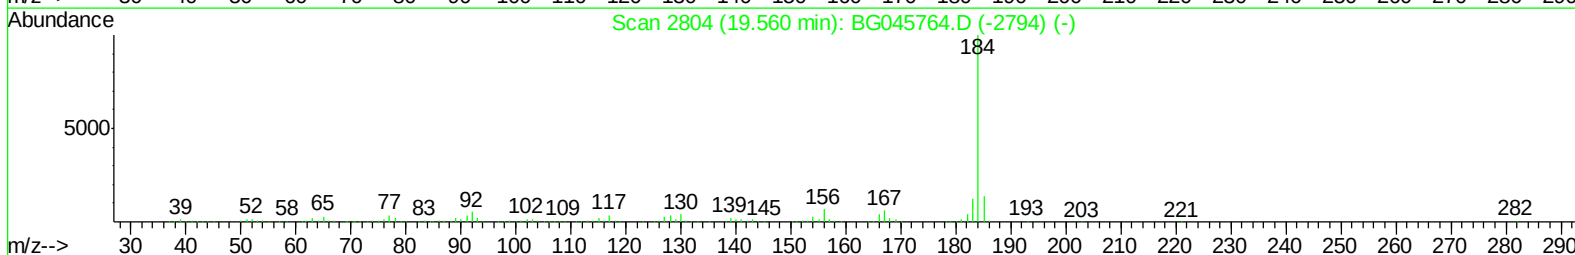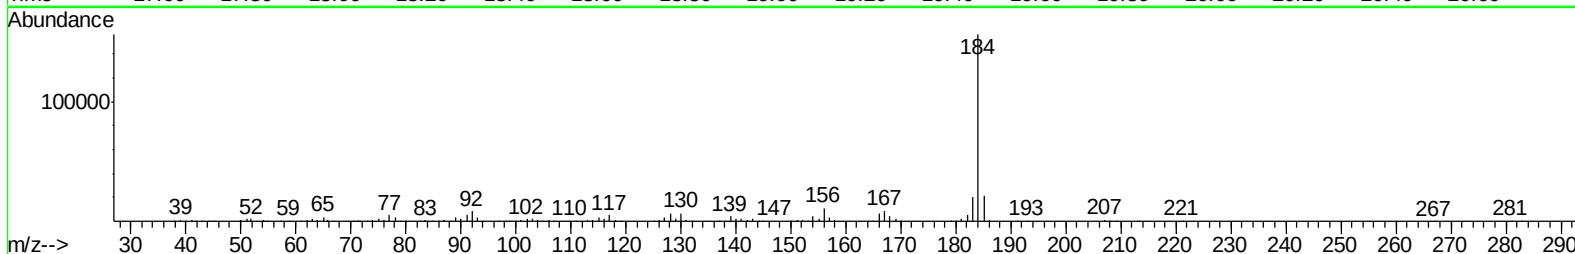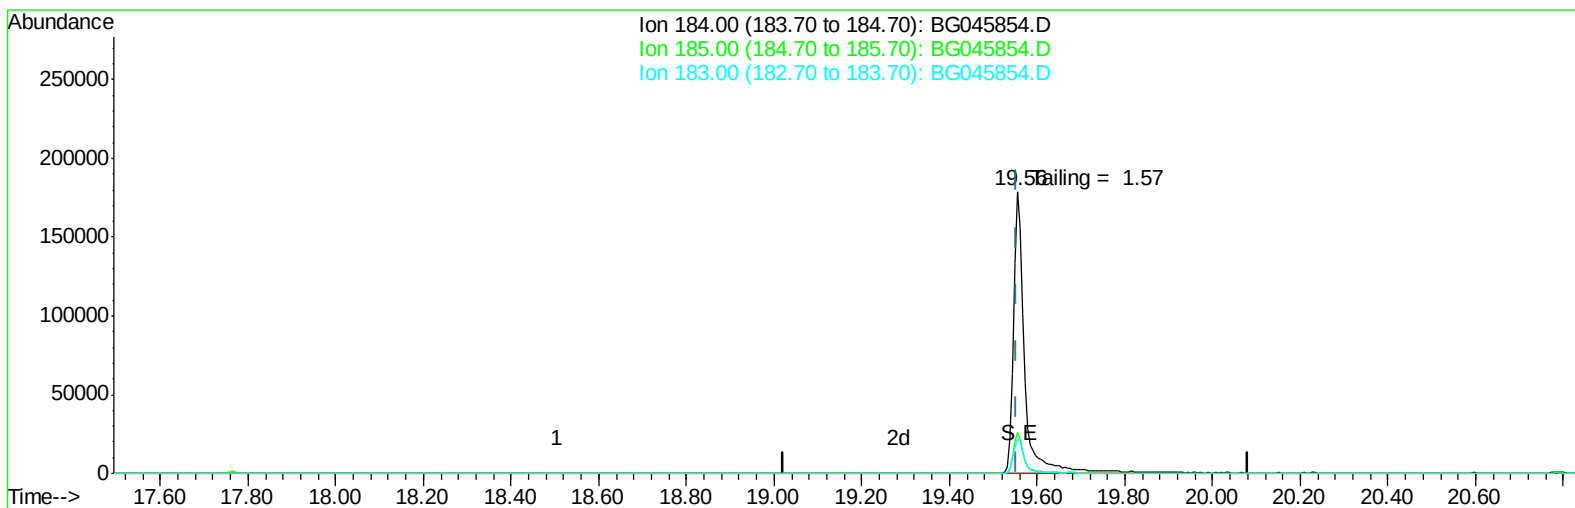

TIC: BG045854.D

(77) Benzidine

18.505min (-1.048) 0.98ng

response 72

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	0.00#
183.00	12.10	0.00#
0.00	0.00	0.00