


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062520\
 Data File : BG045854.D
 Acq On : 25 Jun 2020 12:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 25 15:44:32 2020

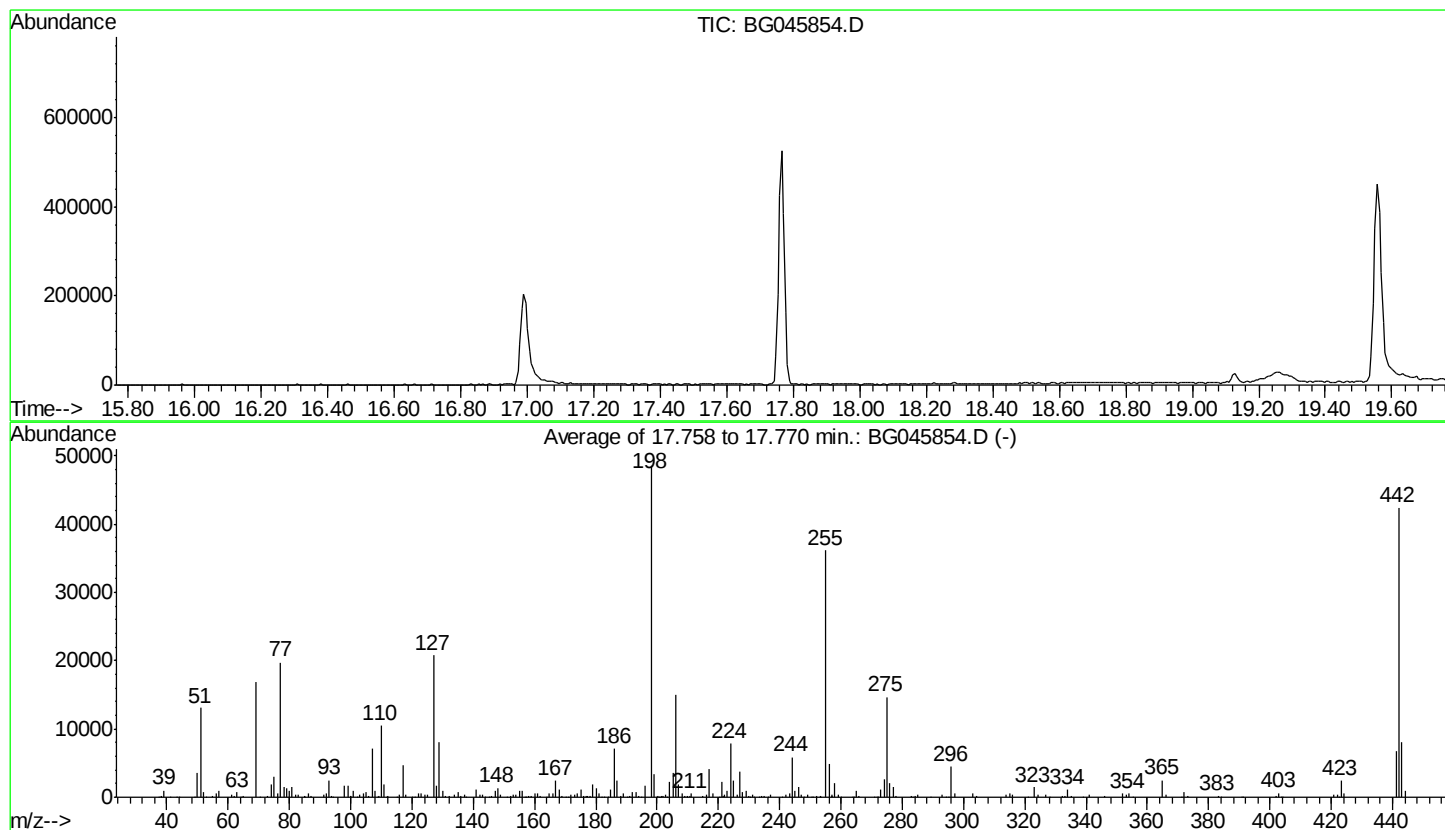

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	13047	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.9	16962	PASS
70	69	0.00	2	0.3	54	PASS
127	198	10	80	42.8	20776	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48552	PASS
199	198	5	9	6.9	3351	PASS
275	198	10	60	30.2	14685	PASS
365	198	1	100	5.1	2488	PASS
441	198	0.01	100	13.8	6707	PASS
442	198	50	100	87.4	42432	PASS
443	442	15	24	19.0	8079	PASS