

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054056.D
 Acq On : 25 Jun 2022 11:28
 Operator : CG/JU
 Sample : PB145713BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK713

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.490	14	17	24	rVB2	5628	9330	0.93%	0.107%
2	3.908	84	88	102	rBV	70115	131834	13.09%	1.516%
3	4.248	142	146	153	rVB7	1467	2953	0.29%	0.034%
4	7.227	647	653	661	rBV	97704	175572	17.43%	2.019%
5	7.392	674	681	689	rBV	70766	122438	12.16%	1.408%
6	7.603	710	717	727	rVB	93422	167257	16.61%	1.923%
7	8.073	791	797	804	rBV	67030	116680	11.59%	1.342%
8	8.772	909	916	925	rBV	127846	233963	23.23%	2.691%
9	9.231	986	994	1004	rVB	92735	174726	17.35%	2.009%
10	9.953	1109	1117	1127	rBB	76870	143761	14.27%	1.653%
11	10.500	1202	1210	1224	rBV	134118	251466	24.97%	2.892%
12	10.882	1266	1275	1283	rBB	106283	195909	19.45%	2.253%
13	11.011	1289	1297	1307	rBV	130597	251457	24.97%	2.892%
14	12.456	1538	1543	1544	rBV2	1565	1785	0.18%	0.021%
15	12.468	1544	1545	1550	rVB2	1585	1337	0.13%	0.015%
16	14.096	1814	1822	1830	rBV	289581	436106	43.30%	5.015%
17	14.389	1865	1872	1881	rBV	304398	500966	49.74%	5.761%
18	14.695	1917	1924	1933	rVB	209630	336762	33.44%	3.873%
19	14.883	1950	1956	1972	rBV	100704	177532	17.63%	2.042%
20	15.688	2086	2093	2100	rBV	439245	683182	67.84%	7.857%
21	15.800	2106	2112	2121	rBV	105734	169500	16.83%	1.949%
22	15.929	2130	2134	2138	rVB	3999	5216	0.52%	0.060%
23	16.469	2223	2226	2231	rBB	1914	2150	0.21%	0.025%
24	16.528	2231	2236	2239	rBV2	682	1280	0.13%	0.015%
25	17.439	2384	2391	2399	rBV	293056	451894	44.87%	5.197%
26	17.539	2401	2408	2417	rVB	511278	790487	78.49%	9.091%
27	19.184	2684	2688	2691	rBV2	674	1080	0.11%	0.012%
28	19.389	2719	2723	2729	rBV4	7211	9863	0.98%	0.113%
29	19.460	2731	2735	2740	rVB2	5618	8554	0.85%	0.098%
30	19.824	2790	2797	2808	rBV	668355	1007104	100.00%	11.582%
31	20.847	2969	2971	2974	rVB3	1440	1324	0.13%	0.015%
32	21.181	3025	3028	3032	rBV3	1185	1902	0.19%	0.022%
33	21.317	3049	3051	3053	rBV3	1356	1453	0.14%	0.017%
34	21.440	3068	3072	3074	rBV4	1679	2110	0.21%	0.024%
35	21.569	3092	3094	3096	rBV2	1526	1466	0.15%	0.017%
36	21.716	3112	3119	3127	rBV	312963	540953	53.71%	6.221%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054056.D
 Acq On : 25 Jun 2022 11:28
 Operator : CG/JU
 Sample : PB145713BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK713

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	22.098	3182	3184	3188	rBV5	1424	1496	0.15%	0.017%
38	22.221	3203	3205	3207	rBV3	1495	1434	0.14%	0.016%
39	22.627	3273	3274	3277	rBV2	1577	1521	0.15%	0.017%
40	24.055	3511	3517	3524	rVB9	5507	11501	1.14%	0.132%
41	24.248	3548	3550	3551	rBV2	1624	1205	0.12%	0.014%
42	24.748	3623	3635	3653	rBV3	327347	998758	99.17%	11.486%
43	24.965	3662	3672	3693	rVB2	172864	543465	53.96%	6.250%
44	26.158	3871	3875	3877	rBV4	3689	4733	0.47%	0.054%
45	27.533	4105	4109	4110	rBV4	3529	4345	0.43%	0.050%
46	27.927	4174	4176	4177	rBV2	1405	1223	0.12%	0.014%
47	28.373	4250	4252	4253	rBV	1653	1204	0.12%	0.014%
48	28.502	4272	4274	4278	rVB4	1742	2016	0.20%	0.023%
49	28.602	4289	4291	4294	rBV3	1376	1436	0.14%	0.017%
50	29.149	4382	4384	4385	rBV2	1423	1136	0.11%	0.013%
51	29.548	4449	4452	4453	rBV3	1863	2160	0.21%	0.025%
52	30.764	4657	4659	4661	rBV3	1423	1262	0.13%	0.015%
53	31.217	4734	4736	4739	rBV3	1849	2633	0.26%	0.030%
54	31.804	4834	4836	4838	rVB3	1836	1098	0.11%	0.013%
55	32.621	4972	4975	4976	rBV4	1865	1737	0.17%	0.020%




Sum of corrected areas: 8695715

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054056.D
Acq On : 25 Jun 2022 11:28
Operator : CG/JU
Sample : PB145713BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK713

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

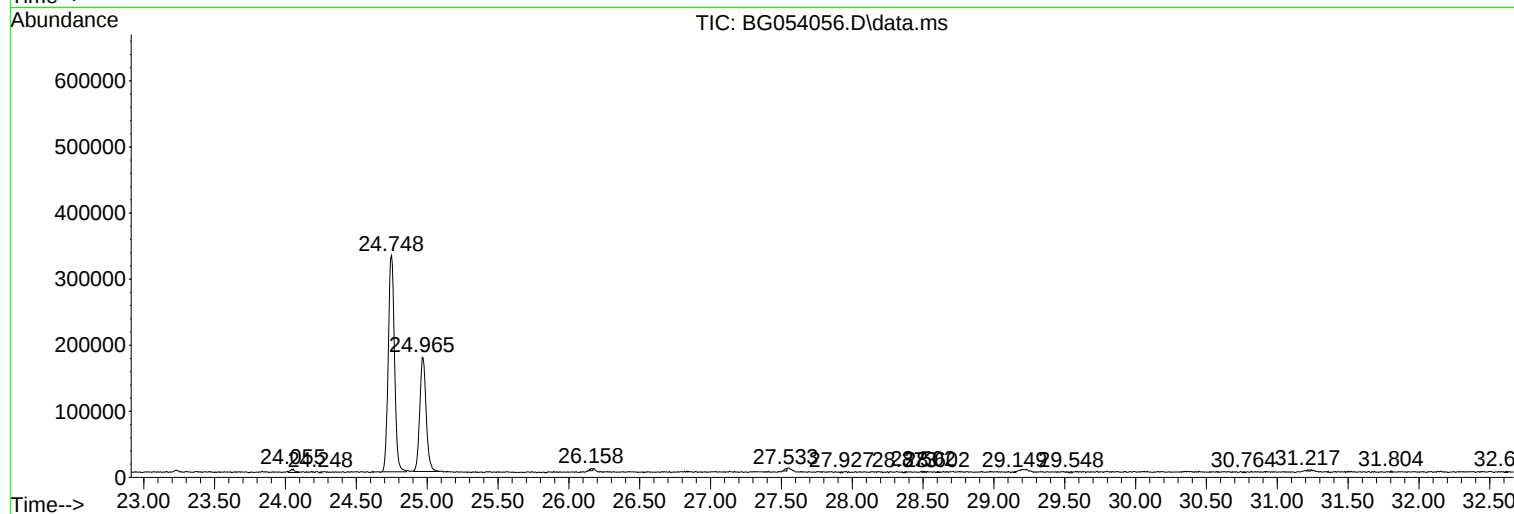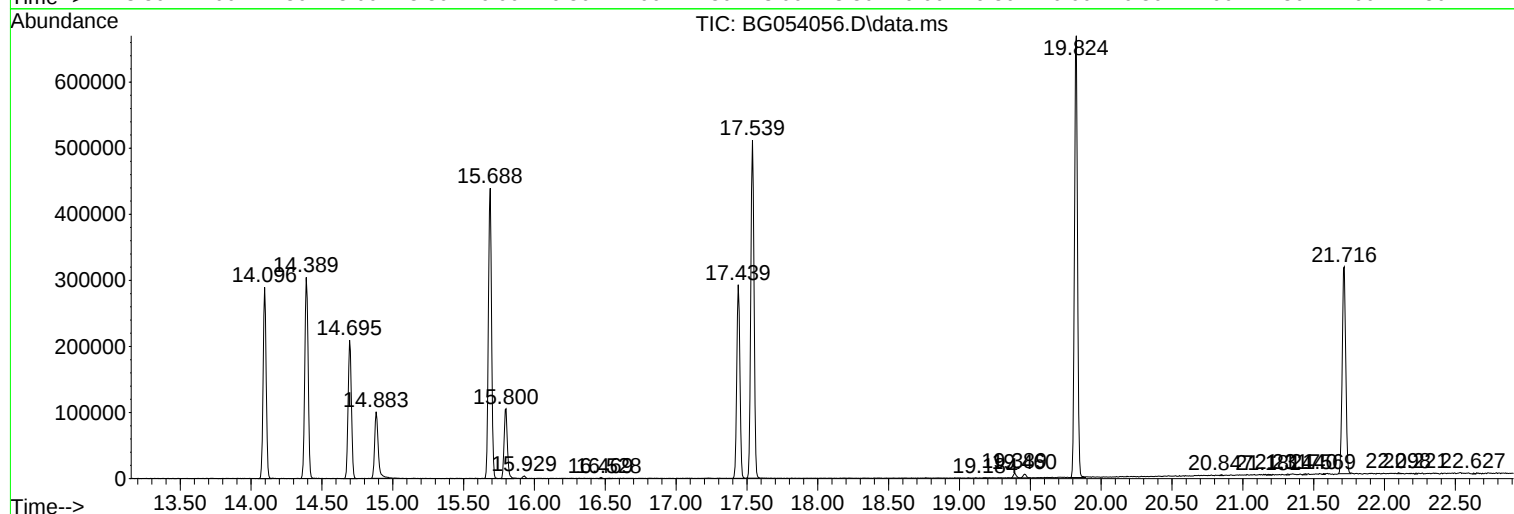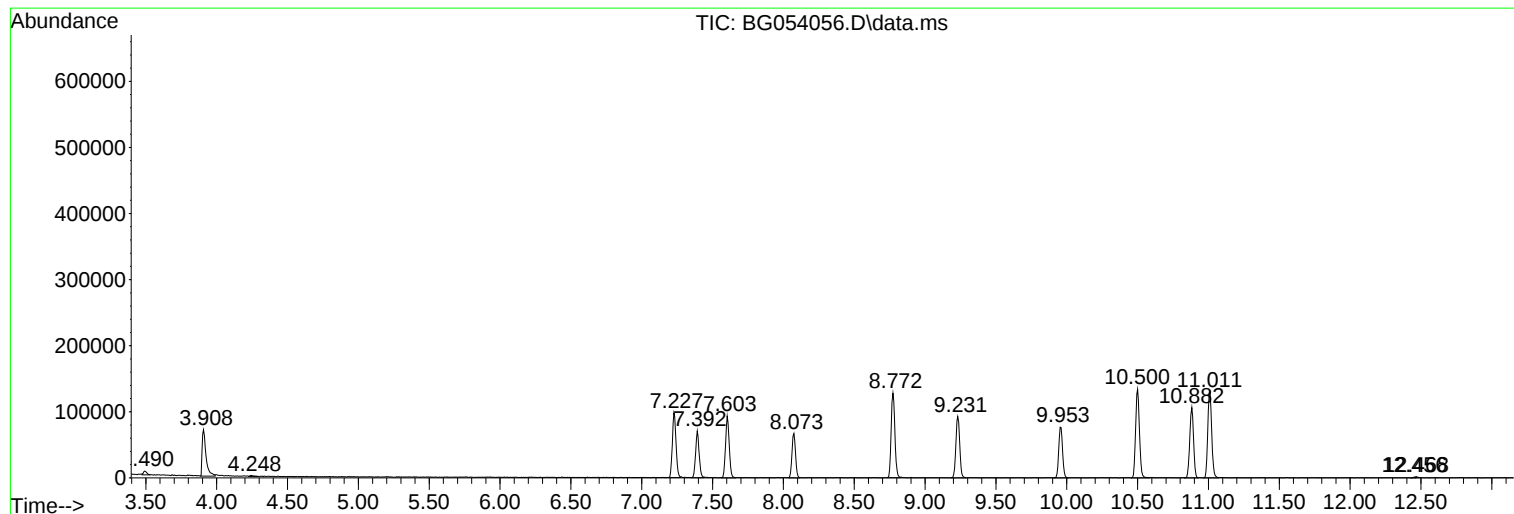

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054056.D
Acq On : 25 Jun 2022 11:28
Operator : CG/JU
Sample : PB145713BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK713

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054056.D
Acq On : 25 Jun 2022 11:28
Operator : CG/JU
Sample : PB145713BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK713

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc