

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054058.D
 Acq On : 25 Jun 2022 12:46
 Operator : CG/JU
 Sample : N3401-09
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.496	13	18	23	rBV3	4328	7564	0.60%	0.068%
2	3.913	86	89	103	rBV2	30434	66282	5.25%	0.596%
3	4.148	127	129	137	rVB5	1901	3691	0.29%	0.033%
4	4.254	142	147	152	rVB5	1425	2678	0.21%	0.024%
5	5.171	300	303	307	rVB5	1254	1702	0.13%	0.015%
6	7.227	645	653	666	rBV4	31442	74074	5.87%	0.666%
7	7.392	675	681	688	rBV	80984	138445	10.96%	1.245%
8	7.480	691	696	702	rVB2	5578	10837	0.86%	0.097%
9	7.603	710	717	729	rBV	83438	160949	12.75%	1.447%
10	8.073	790	797	805	rBV	67466	117717	9.32%	1.058%
11	8.132	805	807	813	rVB2	1114	1576	0.12%	0.014%
12	8.508	865	871	877	rBV4	7907	13361	1.06%	0.120%
13	8.602	881	887	895	rVB2	5029	11017	0.87%	0.099%
14	8.772	910	916	923	rBV	79167	142044	11.25%	1.277%
15	8.837	923	927	930	rVV3	7513	14540	1.15%	0.131%
16	8.890	931	936	945	rVB3	10545	25099	1.99%	0.226%
17	9.160	975	982	987	rBB2	6148	10060	0.80%	0.090%
18	9.231	987	994	1001	rBV	109995	209620	16.60%	1.885%
19	9.660	1063	1067	1072	rVB3	1943	3367	0.27%	0.030%
20	9.795	1085	1090	1097	rVB2	8673	13962	1.11%	0.126%
21	9.953	1110	1117	1128	rVB	87455	170473	13.50%	1.533%
22	10.047	1128	1133	1139	rBB3	9182	16075	1.27%	0.145%
23	10.276	1166	1172	1178	rBV	7227	12112	0.96%	0.109%
24	10.500	1203	1210	1222	rBV	141667	281462	22.29%	2.531%
25	10.882	1267	1275	1281	rBV	106379	199609	15.81%	1.795%
26	10.929	1281	1283	1290	rVV2	11995	17536	1.39%	0.158%
27	11.005	1290	1296	1312	rVB	135433	272176	21.55%	2.447%
28	11.222	1327	1333	1338	rBV3	9393	15061	1.19%	0.135%
29	11.792	1426	1430	1435	rBV3	3523	7203	0.57%	0.065%
30	12.157	1486	1492	1500	rVB3	8314	13900	1.10%	0.125%
31	12.386	1528	1531	1540	rBV2	1626	3539	0.28%	0.032%
32	12.462	1540	1544	1547	rVV	2689	3767	0.30%	0.034%
33	12.533	1550	1556	1562	rBV2	14785	24687	1.96%	0.222%
34	12.750	1587	1593	1600	rVB	15843	25524	2.02%	0.230%
35	12.897	1612	1618	1624	rBB4	15017	26727	2.12%	0.240%
36	13.138	1650	1659	1666	rBV3	7504	13499	1.07%	0.121%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054058.D
 Acq On : 25 Jun 2022 12:46
 Operator : CG/JU
 Sample : N3401-09
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	13.214	1666	1672	1679	rBV3	7594	13729	1.09%	0.123%
38	13.502	1715	1721	1723	rBV	17766	28028	2.22%	0.252%
39	13.531	1723	1726	1730	rVV	23302	36274	2.87%	0.326%
40	13.573	1730	1733	1740	rVB	16722	26863	2.13%	0.242%
41	13.772	1761	1767	1774	rVB2	7376	11758	0.93%	0.106%
42	14.096	1815	1822	1827	rBV	332234	497359	39.39%	4.472%
43	14.137	1827	1829	1835	rVB	18016	25088	1.99%	0.226%
44	14.260	1844	1850	1855	rBV2	10025	14328	1.13%	0.129%
45	14.389	1864	1872	1883	rBV	358202	615593	48.75%	5.535%
46	14.595	1901	1907	1914	rBV2	6706	11106	0.88%	0.100%
47	14.695	1917	1924	1930	rBV	208658	333611	26.42%	3.000%
48	14.759	1930	1935	1941	rVB	24288	36790	2.91%	0.331%
49	14.883	1950	1956	1965	rBV3	29514	55948	4.43%	0.503%
50	15.018	1974	1979	1982	rBV2	19251	30813	2.44%	0.277%
51	15.047	1982	1984	1987	rVV2	9211	10878	0.86%	0.098%
52	15.088	1987	1991	1997	rVB	21416	33701	2.67%	0.303%
53	15.318	2026	2030	2038	rVB	7436	12447	0.99%	0.112%
54	15.429	2042	2049	2054	rVV2	3257	4737	0.38%	0.043%
55	15.500	2056	2061	2068	rVB2	21039	30582	2.42%	0.275%
56	15.688	2085	2093	2098	rBV	509363	803402	63.62%	7.224%
57	15.741	2098	2102	2106	rVV3	47506	82831	6.56%	0.745%
58	15.799	2106	2112	2124	rVB	128144	213705	16.92%	1.922%
59	15.940	2129	2136	2142	rVB2	28946	44758	3.54%	0.402%
60	16.463	2222	2225	2229	rBV	1602	1782	0.14%	0.016%
61	16.622	2248	2252	2257	rBV2	20517	28403	2.25%	0.255%
62	16.751	2269	2274	2279	rVB	23000	32660	2.59%	0.294%
63	16.880	2292	2296	2304	rBV	20828	28089	2.22%	0.253%
64	17.098	2329	2333	2338	rBV5	2501	3889	0.31%	0.035%
65	17.439	2385	2391	2396	rBV	292461	464762	36.81%	4.179%
66	17.480	2396	2398	2402	rVV2	33609	43728	3.46%	0.393%
67	17.539	2402	2408	2419	rVV	599078	977319	77.40%	8.788%
68	17.621	2419	2422	2425	rVB2	2733	3533	0.28%	0.032%
69	17.838	2448	2459	2467	rBV	27163	40536	3.21%	0.364%
70	18.332	2540	2543	2548	rBV4	2271	3371	0.27%	0.030%
71	18.396	2548	2554	2559	rVB	29897	40151	3.18%	0.361%
72	19.389	2718	2723	2729	rVB4	8324	12437	0.98%	0.112%
73	19.489	2730	2740	2748	rBV2	44314	74466	5.90%	0.670%
74	19.736	2780	2782	2787	rVB	1624	1795	0.14%	0.016%
75	19.824	2790	2797	2807	rBV	789125	1246820	98.74%	11.211%
76	20.188	2855	2859	2862	rVV6	1853	3346	0.26%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054058.D
 Acq On : 25 Jun 2022 12:46
 Operator : CG/JU
 Sample : N3401-09
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

77	20.218	2862	2864	2869	rVB5	1378	2562	0.20%	0.023%
78	20.729	2947	2951	2957	rBV	31031	36688	2.91%	0.330%
79	20.846	2967	2971	2975	rVB5	1924	2872	0.23%	0.026%
80	21.358	3052	3058	3062	rVV6	9136	16920	1.34%	0.152%
81	21.598	3094	3099	3107	rVV2	47535	74058	5.86%	0.666%
82	21.710	3109	3118	3124	rVV2	335951	636539	50.41%	5.724%
83	21.757	3124	3126	3136	rVB	45618	65676	5.20%	0.591%
84	22.527	3253	3257	3263	rVB7	3646	7241	0.57%	0.065%
85	22.821	3301	3307	3315	rVB	26473	47590	3.77%	0.428%
86	23.226	3372	3376	3383	rVB7	7523	14117	1.12%	0.127%
87	23.326	3390	3393	3394	rBV2	2848	2299	0.18%	0.021%
88	23.931	3488	3496	3502	rBV2	25489	69946	5.54%	0.629%
89	23.996	3502	3507	3514	rVV	22797	48874	3.87%	0.439%
90	24.748	3623	3635	3658	rBV2	410387	1262743	100.00%	11.354%
91	24.965	3661	3672	3688	rVB2	173033	565911	44.82%	5.089%
92	25.882	3824	3828	3830	rBV5	1437	1977	0.16%	0.018%
93	26.164	3868	3876	3885	rVB4	11545	32812	2.60%	0.295%
94	26.610	3950	3952	3955	rBV4	1674	1645	0.13%	0.015%
95	27.544	4103	4111	4123	rVB7	10327	35886	2.84%	0.323%
96	28.702	4292	4308	4309	rBV4	13489	48599	3.85%	0.437%
97	29.213	4387	4395	4403	rVB9	4963	18394	1.46%	0.165%
98	29.425	4429	4431	4435	rBV4	1340	1540	0.12%	0.014%
99	29.842	4495	4502	4503	rBV4	5646	10899	0.86%	0.098%
100	30.529	4617	4619	4621	rBV3	1951	2130	0.17%	0.019%




Sum of corrected areas: 11121269

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054058.D
Acq On : 25 Jun 2022 12:46
Operator : CG/JU
Sample : N3401-09
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

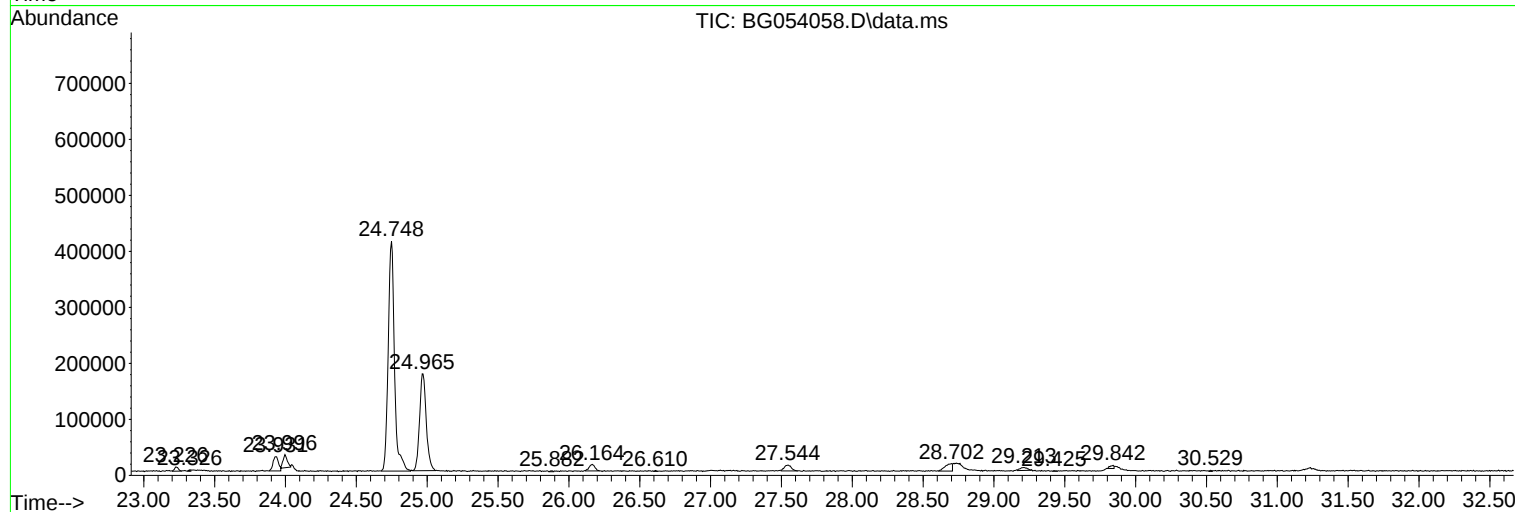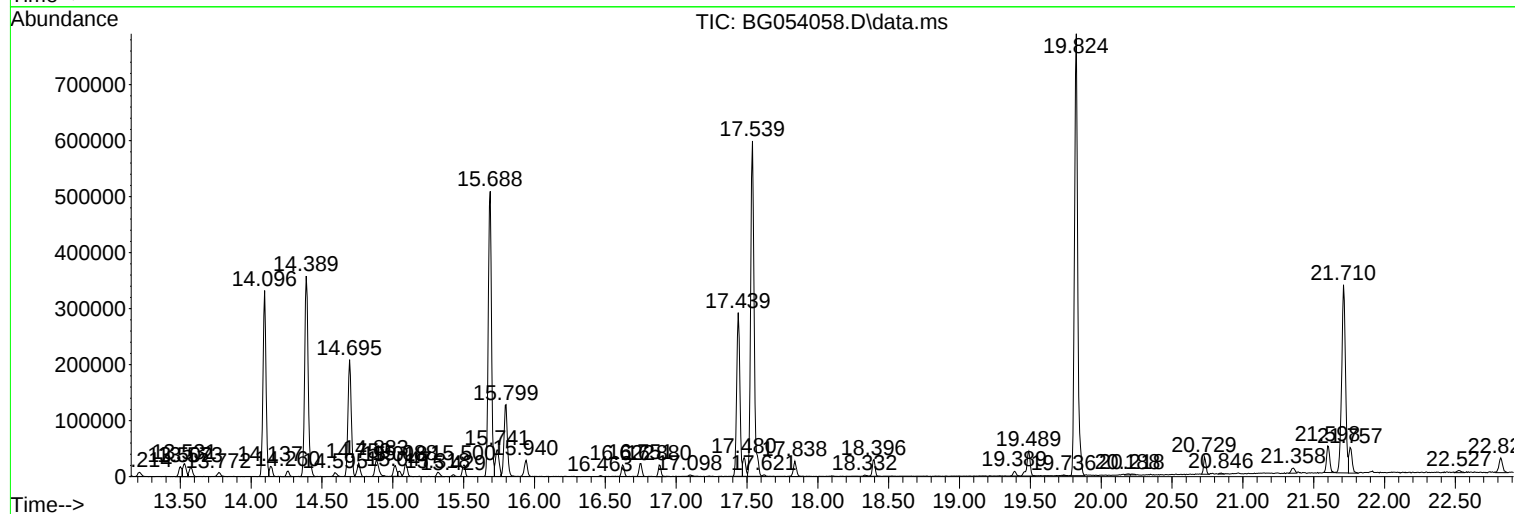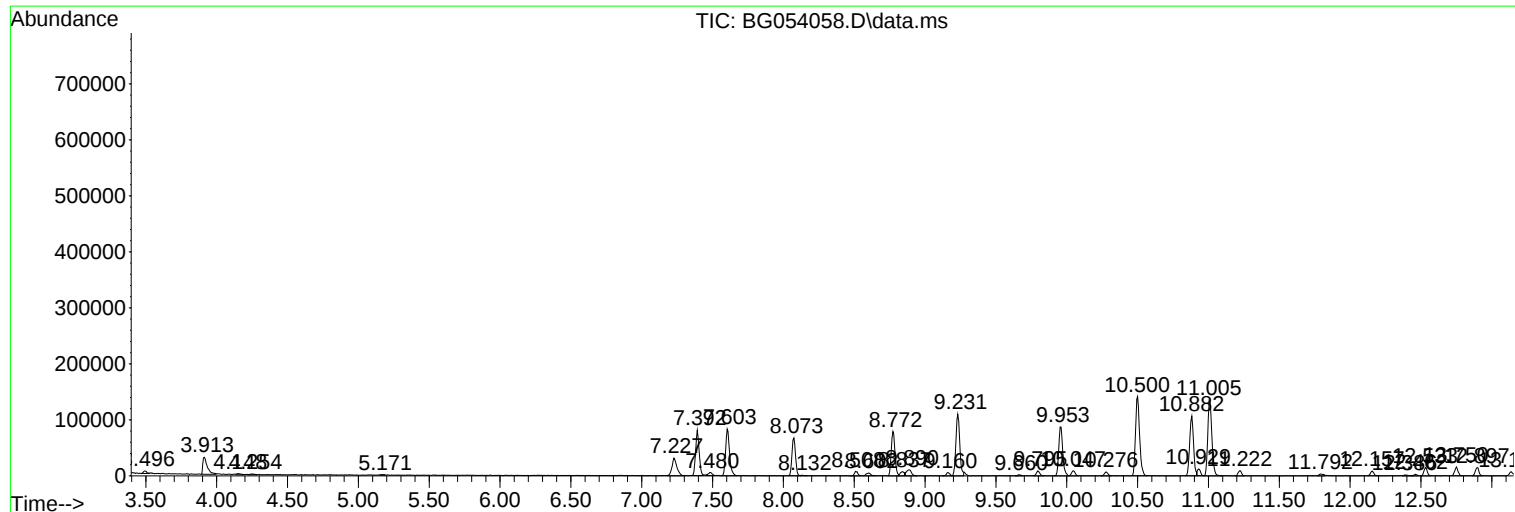

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054058.D
Acq On : 25 Jun 2022 12:46
Operator : CG/JU
Sample : N3401-09
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054058.D
Acq On : 25 Jun 2022 12:46
Operator : CG/JU
Sample : N3401-09
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc