

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054063.D
 Acq On : 25 Jun 2022 16:02
 Operator : CG/JU
 Sample : N3401-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.493	13	18	25	rVB3	5075	9257	0.86%	0.106%
2	3.916	87	90	98	rBV	16516	31746	2.96%	0.364%
3	4.146	125	129	134	rVB4	1793	2897	0.27%	0.033%
4	5.168	299	303	309	rVB5	1309	1589	0.15%	0.018%
5	7.230	647	654	663	rVB	19713	34856	3.25%	0.400%
6	7.389	675	681	689	rBV	66949	120132	11.21%	1.379%
7	7.459	689	693	697	rVV	1077	1561	0.15%	0.018%
8	7.606	710	718	729	rBV	68949	123162	11.49%	1.413%
9	7.894	766	767	774	rBV2	790	1398	0.13%	0.016%
10	8.070	790	797	805	rBV	76637	133457	12.45%	1.531%
11	8.135	805	808	812	rVV2	976	1204	0.11%	0.014%
12	8.775	911	917	924	rBV	61808	113102	10.55%	1.298%
13	9.228	986	994	1005	rBV	93156	171587	16.01%	1.969%
14	9.669	1062	1069	1073	rBV2	2107	3870	0.36%	0.044%
15	9.956	1111	1118	1128	rBV	73915	133562	12.46%	1.533%
16	10.497	1202	1210	1220	rBV	119122	221494	20.67%	2.542%
17	10.879	1267	1275	1285	rVB	122292	224382	20.94%	2.575%
18	11.008	1287	1297	1308	rBV	118126	223640	20.87%	2.566%
19	12.454	1539	1543	1544	rBV	1501	1565	0.15%	0.018%
20	13.523	1720	1725	1727	rBV	2489	2793	0.26%	0.032%
21	14.093	1815	1822	1829	rBV	284609	437916	40.86%	5.025%
22	14.392	1865	1873	1880	rBV	296580	495609	46.25%	5.687%
23	14.698	1918	1925	1933	rBB	233192	376839	35.16%	4.324%
24	14.886	1952	1957	1969	rBV2	15085	28171	2.63%	0.323%
25	15.426	2044	2049	2054	rBV	7591	10310	0.96%	0.118%
26	15.685	2086	2093	2102	rVB	447073	703652	65.66%	8.075%
27	15.797	2106	2112	2126	rBV	108040	164967	15.39%	1.893%
28	15.926	2130	2134	2138	rBV2	4371	5623	0.52%	0.065%
29	16.466	2223	2226	2229	rVB2	1524	1632	0.15%	0.019%
30	17.436	2385	2391	2401	rBV	322727	512969	47.87%	5.887%
31	17.536	2401	2408	2416	rVV2	533984	836550	78.06%	9.600%
32	17.618	2420	2422	2426	rVB3	3030	3267	0.30%	0.037%
33	18.335	2539	2544	2547	rBV5	2748	4540	0.42%	0.052%
34	19.387	2717	2723	2729	rVB3	7953	11381	1.06%	0.131%
35	19.457	2730	2735	2740	rBV	6603	10423	0.97%	0.120%
36	19.592	2756	2758	2762	rBV3	1990	1617	0.15%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054063.D
 Acq On : 25 Jun 2022 16:02
 Operator : CG/JU
 Sample : N3401-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.745	2781	2784	2785	rBV3	1810	1939	0.18%	0.022%
38	19.821	2790	2797	2805	rBV	725816	1071647	100.00%	12.298%
39	20.180	2856	2858	2859	rBV2	1437	1083	0.10%	0.012%
40	20.250	2868	2870	2873	rVB2	1298	1120	0.10%	0.013%

41	20.297	2873	2878	2879	rBV2	1189	1626	0.15%	0.019%
42	20.356	2885	2888	2891	rVB4	1204	1383	0.13%	0.016%
43	20.427	2897	2900	2901	rBV3	958	1082	0.10%	0.012%
44	21.043	3004	3005	3008	rBV2	1384	1296	0.12%	0.015%
45	21.137	3018	3021	3023	rVV3	1360	1395	0.13%	0.016%

46	21.355	3051	3058	3063	rBV5	12715	24127	2.25%	0.277%
47	21.713	3112	3119	3127	rVB	380342	623062	58.14%	7.150%
48	21.825	3136	3138	3140	rBV3	1287	1365	0.13%	0.016%
49	21.913	3150	3153	3157	rVB4	3041	3954	0.37%	0.045%
50	22.324	3220	3223	3224	rBV2	1337	1157	0.11%	0.013%

51	22.530	3253	3258	3261	rBV6	4613	7811	0.73%	0.090%
52	23.059	3346	3348	3351	rVB3	1987	1830	0.17%	0.021%
53	23.088	3351	3353	3354	rBV2	1871	1440	0.13%	0.017%
54	23.229	3373	3377	3382	rVB4	5490	8012	0.75%	0.092%
55	23.623	3442	3444	3446	rBV3	1637	1560	0.15%	0.018%

56	24.046	3510	3516	3524	rVB4	8537	19954	1.86%	0.229%
57	24.351	3567	3568	3570	rBV2	1916	1694	0.16%	0.019%
58	24.504	3591	3594	3596	rBV2	1205	1416	0.13%	0.016%
59	24.745	3623	3635	3650	rBV2	367788	1064884	99.37%	12.220%
60	24.968	3662	3673	3693	rVB2	194341	641904	59.90%	7.366%

61	25.356	3738	3739	3741	rBV2	1807	1484	0.14%	0.017%
62	26.155	3868	3875	3885	rVB4	8841	25302	2.36%	0.290%
63	26.331	3903	3905	3908	rVB2	1253	1146	0.11%	0.013%
64	26.414	3917	3919	3922	rBV4	1401	1850	0.17%	0.021%
65	26.995	4016	4018	4019	rBV	1776	1105	0.10%	0.013%

66	27.501	4102	4104	4105	rBV2	2391	1960	0.18%	0.022%
67	27.548	4106	4112	4118	rVB7	6716	18439	1.72%	0.212%
68	27.877	4166	4168	4174	rBV4	1270	1626	0.15%	0.019%
69	28.094	4203	4205	4206	rBV2	1285	1086	0.10%	0.012%
70	28.347	4246	4248	4250	rBV3	1430	1808	0.17%	0.021%

71	28.488	4270	4272	4273	rVB2	1583	1089	0.10%	0.012%
72	28.682	4304	4305	4307	rBV2	1609	1153	0.11%	0.013%
73	29.481	4439	4441	4443	rBV2	1197	1142	0.11%	0.013%
74	30.321	4582	4584	4585	rBV2	1567	1346	0.13%	0.015%
75	31.226	4735	4738	4739	rBV3	1952	2369	0.22%	0.027%

76	31.937	4857	4859	4864	rVB5	1471	1809	0.17%	0.021%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054063.D
Acq On : 25 Jun 2022 16:02
Operator : CG/JU
Sample : N3401-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Title : SVOA CALIBRATION




Sum of corrected areas: 8714175

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054063.D
Acq On : 25 Jun 2022 16:02
Operator : CG/JU
Sample : N3401-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

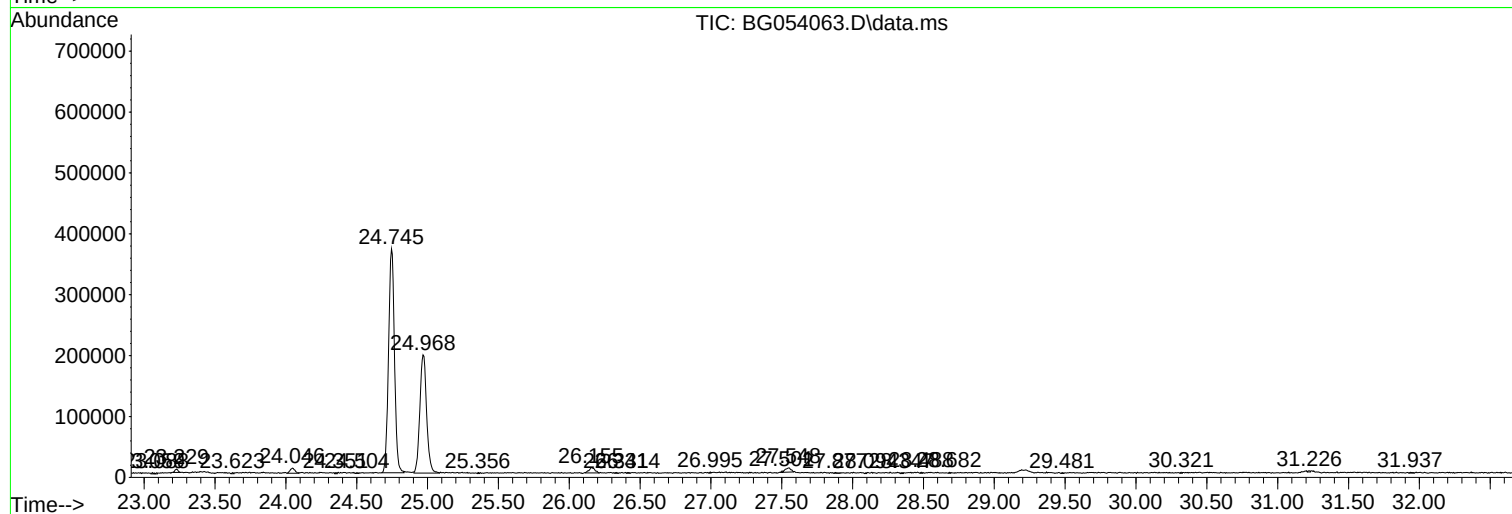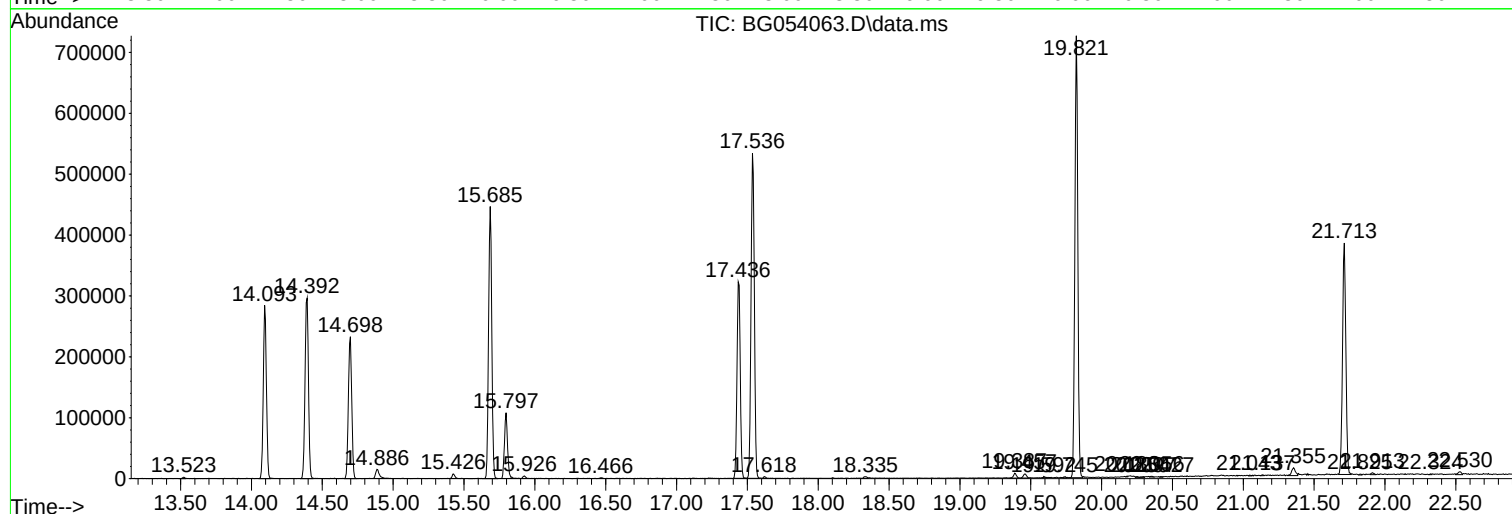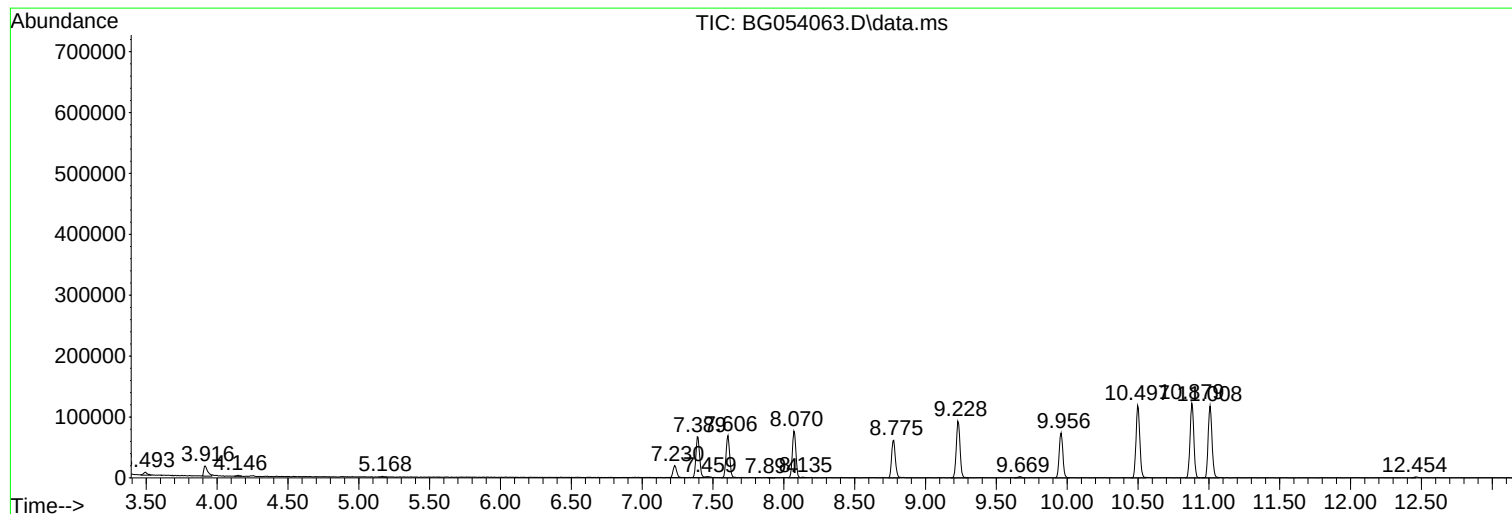

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054063.D
Acq On : 25 Jun 2022 16:02
Operator : CG/JU
Sample : N3401-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054063.D
Acq On : 25 Jun 2022 16:02
Operator : CG/JU
Sample : N3401-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc