

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054064.D
 Acq On : 25 Jun 2022 16:41
 Operator : CG/JU
 Sample : N3400-20
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054064.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.459	9	12	14	rBV4	1473	1792	0.16%	0.020%
2	3.495	14	18	24	rVB3	5179	7870	0.70%	0.089%
3	3.912	87	89	104	rBV	14070	31062	2.77%	0.353%
4	4.253	142	147	150	rBV3	1483	2298	0.20%	0.026%
5	4.493	184	188	195	rBV5	832	1946	0.17%	0.022%
6	5.163	299	302	306	rVB3	906	1192	0.11%	0.014%
7	6.103	455	462	464	rBV4	797	1355	0.12%	0.015%
8	7.231	648	654	662	rBV2	18674	33922	3.02%	0.385%
9	7.390	675	681	690	rBV	70549	125818	11.21%	1.428%
10	7.602	710	717	727	rBV	69938	128323	11.44%	1.457%
11	8.072	790	797	807	rVB2	71469	125820	11.21%	1.428%
12	8.777	908	917	925	rBV	61978	114349	10.19%	1.298%
13	8.894	934	937	939	rBV3	1272	1242	0.11%	0.014%
14	9.229	985	994	1002	rBV	98361	184361	16.43%	2.093%
15	9.958	1111	1118	1126	rBV	76226	142083	12.66%	1.613%
16	10.498	1202	1210	1222	rBV	124589	229863	20.49%	2.609%
17	10.880	1266	1275	1283	rBV	113402	209719	18.69%	2.380%
18	11.009	1290	1297	1308	rBV	111283	212816	18.97%	2.416%
19	11.544	1381	1388	1393	rBB3	1267	2328	0.21%	0.026%
20	12.461	1541	1544	1549	rVB2	1829	2740	0.24%	0.031%
21	14.094	1815	1822	1830	rBV	302259	446975	39.84%	5.073%
22	14.388	1865	1872	1881	rBV	319709	523389	46.65%	5.941%
23	14.693	1918	1924	1931	rVB	218728	360146	32.10%	4.088%
24	14.887	1952	1957	1965	rBV3	14520	26849	2.39%	0.305%
25	15.686	2086	2093	2102	rVB	456197	723257	64.46%	8.209%
26	15.798	2106	2112	2124	rVV	115777	184218	16.42%	2.091%
27	15.927	2130	2134	2140	rVB3	4374	6895	0.61%	0.078%
28	16.368	2206	2209	2212	rVB2	1025	1435	0.13%	0.016%
29	16.468	2223	2226	2231	rBB3	1727	2834	0.25%	0.032%
30	17.231	2352	2356	2359	rVB	1003	1498	0.13%	0.017%
31	17.437	2383	2391	2399	rVV	317942	492009	43.85%	5.585%
32	17.537	2401	2408	2420	rVB	581668	878290	78.28%	9.969%
33	19.388	2719	2723	2729	rVB4	6711	10084	0.90%	0.114%
34	19.458	2729	2735	2741	rVB	6467	10420	0.93%	0.118%
35	19.740	2778	2783	2786	rBV3	2017	2590	0.23%	0.029%
36	19.822	2790	2797	2806	rBV	759962	1121999	100.00%	12.735%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054064.D
 Acq On : 25 Jun 2022 16:41
 Operator : CG/JU
 Sample : N3400-20
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	20.298	2875	2878	2880	rBV3	1170	1390	0.12%	0.016%
38	20.504	2911	2913	2916	rVB3	1388	1407	0.13%	0.016%
39	20.592	2924	2928	2931	rBV4	1195	2201	0.20%	0.025%
40	20.851	2967	2972	2979	rBV7	1371	2852	0.25%	0.032%
41	21.068	3007	3009	3010	rBV2	1403	1225	0.11%	0.014%
42	21.297	3045	3048	3049	rBV3	1510	1612	0.14%	0.018%
43	21.344	3052	3056	3057	rBV3	1094	1171	0.10%	0.013%
44	21.391	3062	3064	3066	rBV3	1323	1256	0.11%	0.014%
45	21.579	3095	3096	3098	rBV2	1224	1242	0.11%	0.014%
46	21.714	3111	3119	3129	rBV	350022	590570	52.64%	6.703%
47	21.908	3148	3152	3158	rVB6	1619	3103	0.28%	0.035%
48	22.531	3254	3258	3261	rVB6	2288	3901	0.35%	0.044%
49	23.230	3372	3377	3385	rBV8	5378	11087	0.99%	0.126%
50	23.524	3425	3427	3429	rBV3	1259	1252	0.11%	0.014%
51	23.565	3432	3434	3436	rVB3	1874	1363	0.12%	0.015%
52	23.671	3450	3452	3455	rBV2	1334	1139	0.10%	0.013%
53	24.041	3510	3515	3522	rVB3	8080	16024	1.43%	0.182%
54	24.746	3623	3635	3655	rBV2	383613	1113853	99.27%	12.643%
55	24.969	3661	3673	3691	rBV2	189808	600797	53.55%	6.819%
56	25.398	3744	3746	3749	rBV3	1208	1646	0.15%	0.019%
57	25.886	3828	3829	3833	rBV3	1929	2606	0.23%	0.030%
58	26.109	3865	3867	3868	rBV2	1314	1167	0.10%	0.013%
59	26.156	3870	3875	3888	rVB7	9500	26552	2.37%	0.301%
60	26.432	3920	3922	3923	rBV2	1709	1142	0.10%	0.013%
61	26.515	3934	3936	3938	rVB3	1481	1232	0.11%	0.014%
62	26.532	3938	3939	3941	rBV2	1315	1184	0.11%	0.013%
63	26.973	4012	4014	4016	rBV2	1961	1226	0.11%	0.014%
64	27.108	4034	4037	4041	rBV4	1915	2208	0.20%	0.025%
65	27.466	4095	4098	4099	rBV2	1277	1413	0.13%	0.016%
66	27.549	4101	4112	4122	rVV7	8565	31644	2.82%	0.359%
67	28.324	4242	4244	4246	rBV2	1345	1539	0.14%	0.017%
68	29.206	4385	4394	4400	rBV8	5415	15313	1.36%	0.174%
69	29.306	4409	4411	4414	rVB3	1601	1282	0.11%	0.015%
70	29.846	4501	4503	4507	rVB3	1615	1682	0.15%	0.019%
71	30.915	4683	4685	4687	rBV3	1285	1322	0.12%	0.015%
72	31.844	4841	4843	4844	rBV2	1387	1153	0.10%	0.013%
73	32.079	4881	4883	4885	rBV2	1191	1389	0.12%	0.016%
74	32.531	4958	4960	4963	rBV4	1330	1701	0.15%	0.019%
75	32.590	4968	4970	4972	rBV2	1526	1412	0.13%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054064.D
Acq On : 25 Jun 2022 16:41
Operator : CG/JU
Sample : N3400-20
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Title : SVOA CALIBRATION




Sum of corrected areas: 8810045

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054064.D
Acq On : 25 Jun 2022 16:41
Operator : CG/JU
Sample : N3400-20
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

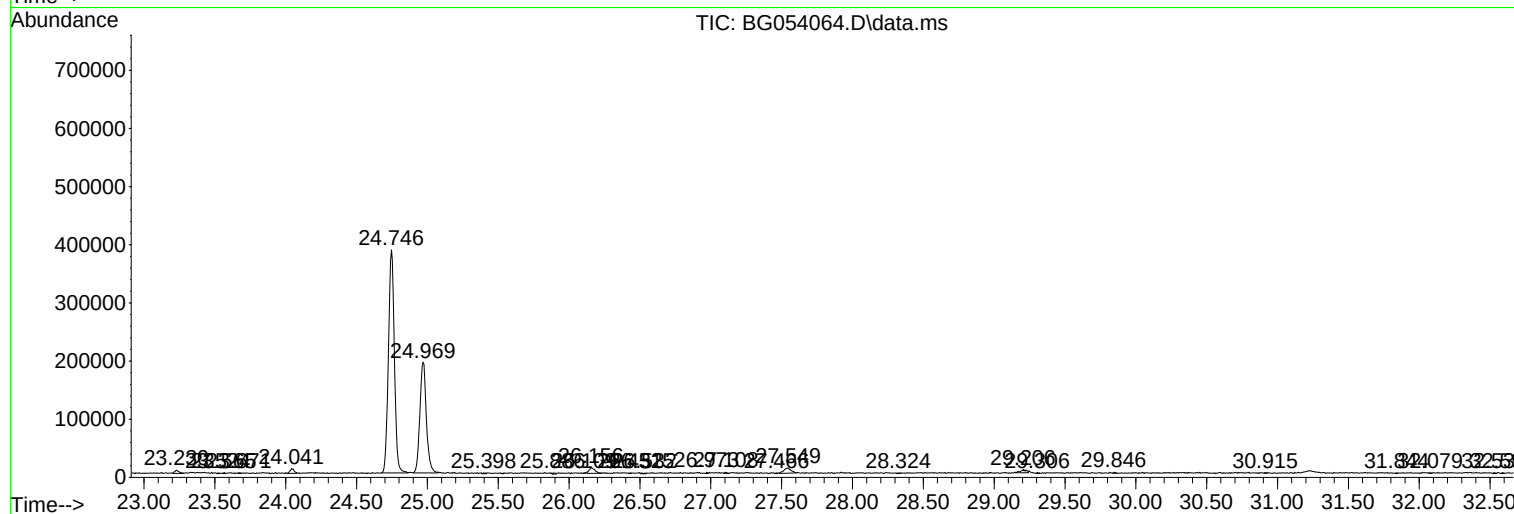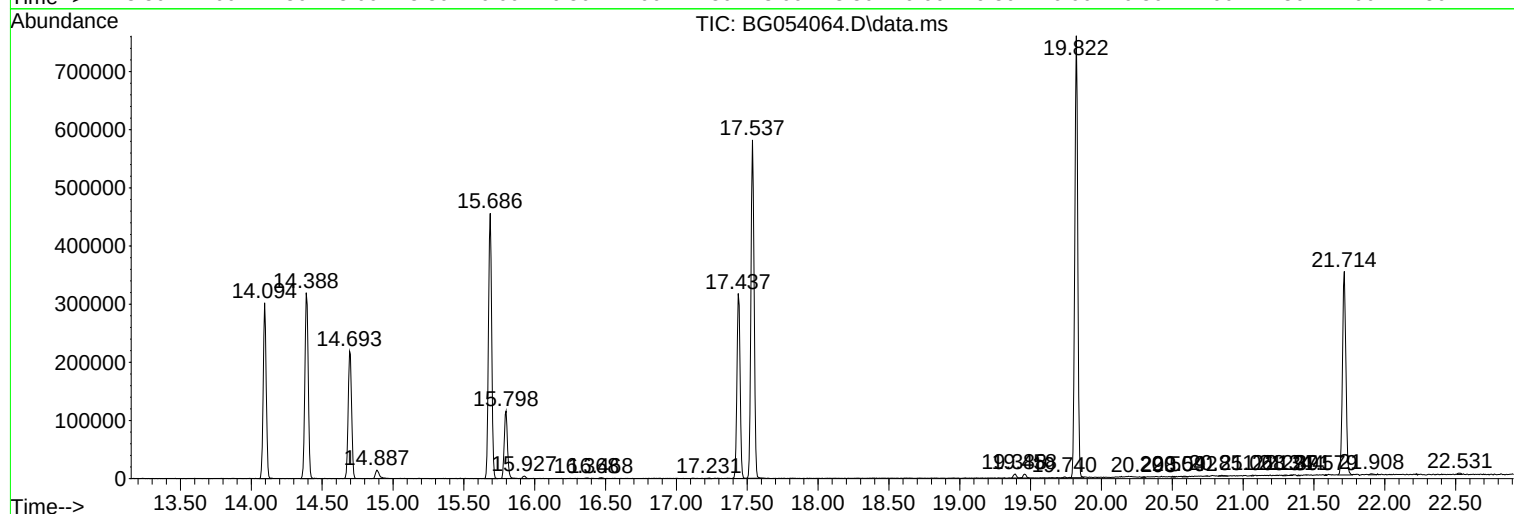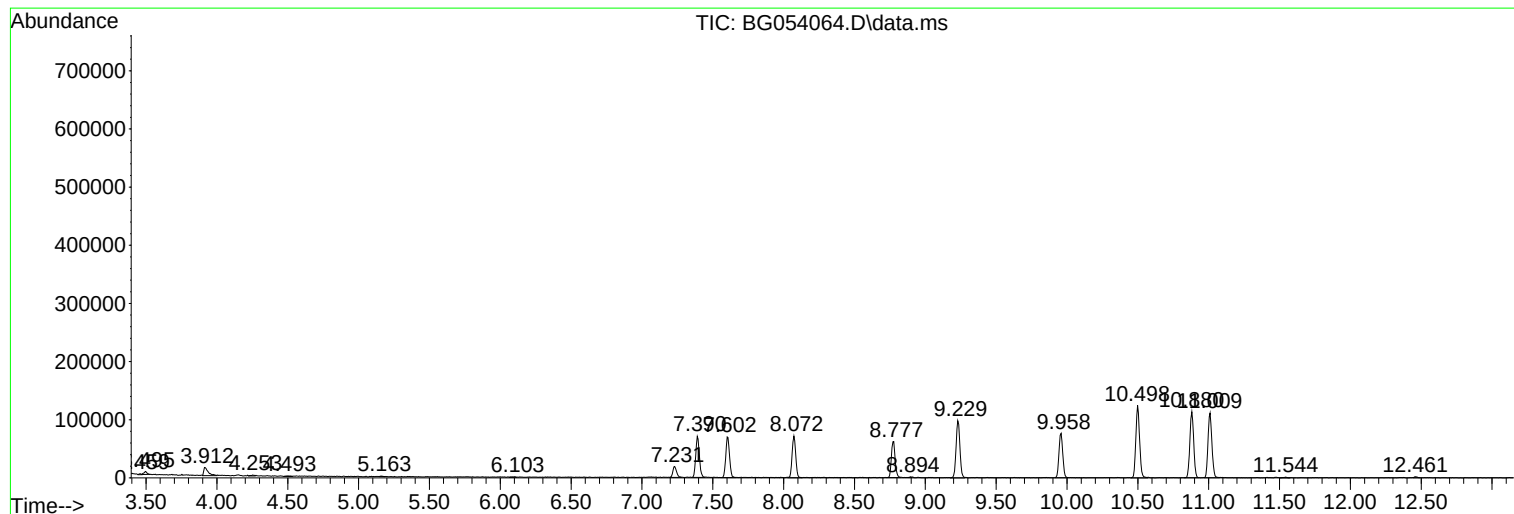

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054064.D
Acq On : 25 Jun 2022 16:41
Operator : CG/JU
Sample : N3400-20
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054064.D
Acq On : 25 Jun 2022 16:41
Operator : CG/JU
Sample : N3400-20
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------