

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054065.D
 Acq On : 25 Jun 2022 17:20
 Operator : CG/JU
 Sample : N3401-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054065.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.494	14	18	27	rVB4	4241	7685	0.68%	0.086%
2	3.911	86	89	100	rBV	15905	31642	2.78%	0.356%
3	4.158	126	131	135	rVB4	1432	2240	0.20%	0.025%
4	4.252	143	147	150	rVB2	1702	2456	0.22%	0.028%
5	5.168	298	303	309	rBV4	1671	2977	0.26%	0.033%
6	7.230	648	654	663	rBV2	21628	38219	3.36%	0.430%
7	7.395	672	682	689	rBV	76713	139049	12.21%	1.564%
8	7.454	689	692	698	rVV3	2219	3488	0.31%	0.039%
9	7.606	711	718	727	rBV	75060	136493	11.99%	1.535%
10	8.071	791	797	805	rBV	64903	116191	10.21%	1.307%
11	8.770	909	916	925	rBV	68034	124772	10.96%	1.403%
12	9.228	987	994	1003	rVV	100403	192718	16.93%	2.168%
13	9.663	1064	1068	1073	rBB2	2860	4277	0.38%	0.048%
14	9.957	1109	1118	1127	rBV	83105	154133	13.54%	1.734%
15	10.497	1203	1210	1221	rBV	130444	247776	21.76%	2.787%
16	10.879	1268	1275	1283	rBV	105919	194414	17.08%	2.187%
17	11.008	1290	1297	1309	rBV	124644	239158	21.01%	2.690%
18	12.465	1539	1545	1550	rBV3	2377	3643	0.32%	0.041%
19	13.523	1721	1725	1730	rVB2	2891	3496	0.31%	0.039%
20	13.588	1732	1736	1740	rVV3	1329	2110	0.19%	0.024%
21	14.093	1815	1822	1834	rBB	313894	478764	42.05%	5.385%
22	14.393	1865	1873	1881	rBV	334089	552490	48.53%	6.214%
23	14.698	1918	1925	1933	rBB	198316	326308	28.66%	3.670%
24	14.886	1952	1957	1965	rBV3	14387	27614	2.43%	0.311%
25	15.427	2044	2049	2055	rVB3	13762	20141	1.77%	0.227%
26	15.685	2086	2093	2101	rBV	483386	763276	67.04%	8.585%
27	15.797	2106	2112	2120	rBV	115866	179477	15.76%	2.019%
28	15.926	2129	2134	2138	rBV2	4019	5945	0.52%	0.067%
29	16.467	2223	2226	2229	rBV	1492	1674	0.15%	0.019%
30	17.442	2385	2392	2401	rBV	283248	451804	39.68%	5.082%
31	17.536	2401	2408	2419	rVB2	557595	880601	77.35%	9.905%
32	17.624	2419	2423	2426	rBV4	2113	2446	0.21%	0.028%
33	18.106	2501	2505	2508	rBV4	1048	1267	0.11%	0.014%
34	18.329	2538	2543	2550	rBV4	3431	5906	0.52%	0.066%
35	18.394	2550	2554	2558	rBV2	997	1224	0.11%	0.014%
36	19.387	2719	2723	2731	rVB3	7827	11638	1.02%	0.131%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054065.D
 Acq On : 25 Jun 2022 17:20
 Operator : CG/JU
 Sample : N3401-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.457	2731	2735	2741	rVB	6841	10716	0.94%	0.121%
38	19.822	2790	2797	2808	rBV	755502	1134090	99.61%	12.756%
39	20.162	2851	2855	2856	rVV2	1001	1398	0.12%	0.016%
40	20.356	2885	2888	2892	rVB3	1853	2278	0.20%	0.026%
41	20.415	2892	2898	2900	rBV3	1168	1759	0.15%	0.020%
42	20.856	2969	2973	2974	rBV4	1412	1490	0.13%	0.017%
43	21.249	3037	3040	3041	rBV3	1069	1317	0.12%	0.015%
44	21.355	3052	3058	3064	rBV2	17594	29941	2.63%	0.337%
45	21.431	3069	3071	3073	rVV2	1585	1251	0.11%	0.014%
46	21.590	3096	3098	3101	rVB4	1427	1176	0.10%	0.013%
47	21.661	3107	3110	3112	rBV4	1531	1685	0.15%	0.019%
48	21.713	3112	3119	3128	rBV	325112	548518	48.18%	6.170%
49	21.907	3149	3152	3158	rBV5	3234	5842	0.51%	0.066%
50	22.095	3182	3184	3186	rBV3	1283	1268	0.11%	0.014%
51	22.407	3235	3237	3239	rVB	2078	1341	0.12%	0.015%
52	22.524	3253	3257	3259	rBV5	3510	5132	0.45%	0.058%
53	22.595	3267	3269	3272	rBV3	1793	1374	0.12%	0.015%
54	23.229	3373	3377	3383	rVB6	5314	8816	0.77%	0.099%
55	23.552	3431	3432	3435	rBV3	1606	1364	0.12%	0.015%
56	23.993	3505	3507	3509	rBV3	1493	1735	0.15%	0.020%
57	24.046	3511	3516	3521	rVV6	6403	13452	1.18%	0.151%
58	24.493	3590	3592	3593	rVB	2020	1247	0.11%	0.014%
59	24.745	3623	3635	3658	rVB	383392	1138485	100.00%	12.805%
60	24.968	3662	3673	3691	rVB2	173461	551105	48.41%	6.199%
61	25.773	3808	3810	3813	rVB2	1572	1560	0.14%	0.018%
62	26.114	3866	3868	3869	rBV	2243	2270	0.20%	0.026%
63	26.161	3871	3876	3884	rVB8	7126	19454	1.71%	0.219%
64	26.390	3914	3915	3917	rBV3	1825	1486	0.13%	0.017%
65	26.502	3931	3934	3936	rBV3	1626	1823	0.16%	0.021%
66	26.725	3970	3972	3974	rBV3	1539	1437	0.13%	0.016%
67	27.542	4105	4111	4124	rVB3	6160	20729	1.82%	0.233%
68	29.146	4382	4384	4387	rBV4	1722	2440	0.21%	0.027%
69	29.210	4390	4395	4397	rVV6	2213	4568	0.40%	0.051%
70	29.733	4482	4484	4486	rBV3	1251	1485	0.13%	0.017%
71	29.786	4490	4493	4497	rBV4	1709	2556	0.22%	0.029%
72	30.292	4577	4579	4583	rBV4	2159	3750	0.33%	0.042%
73	30.591	4627	4630	4631	rBV3	1617	1479	0.13%	0.017%
74	30.879	4678	4679	4681	rBV2	1597	1391	0.12%	0.016%

Sum of corrected areas: 8890720




Instrument :
BNA_G
ClientSampleId :
C0AE2

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054065.D
Acq On : 25 Jun 2022 17:20
Operator : CG/JU
Sample : N3401-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

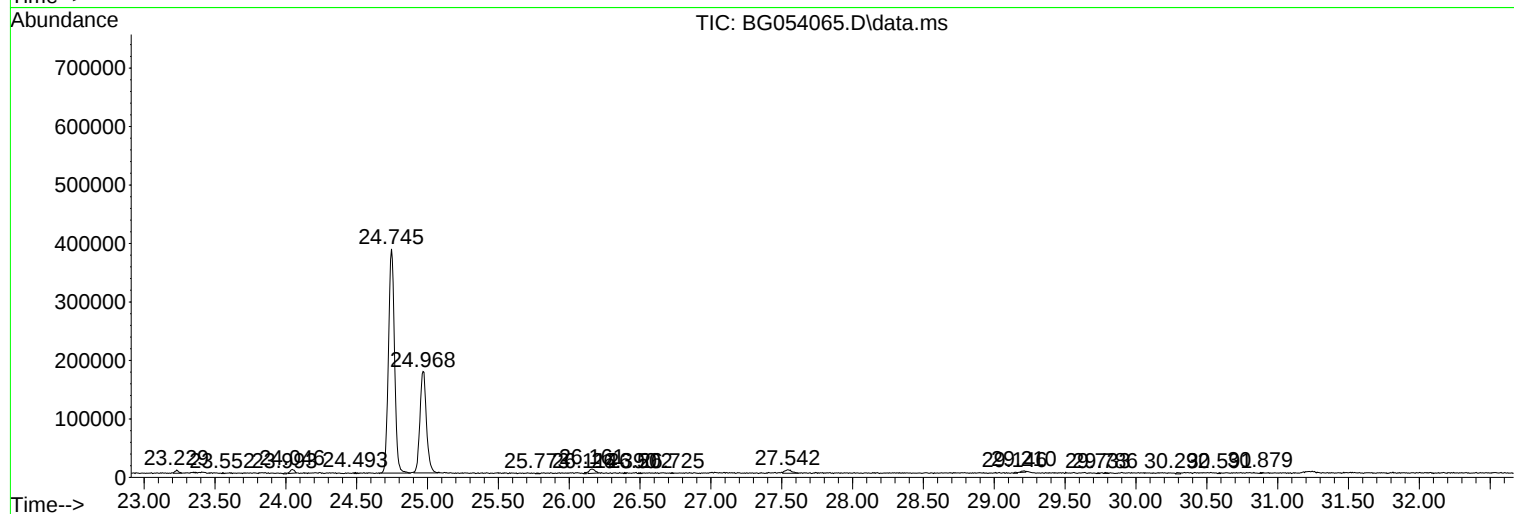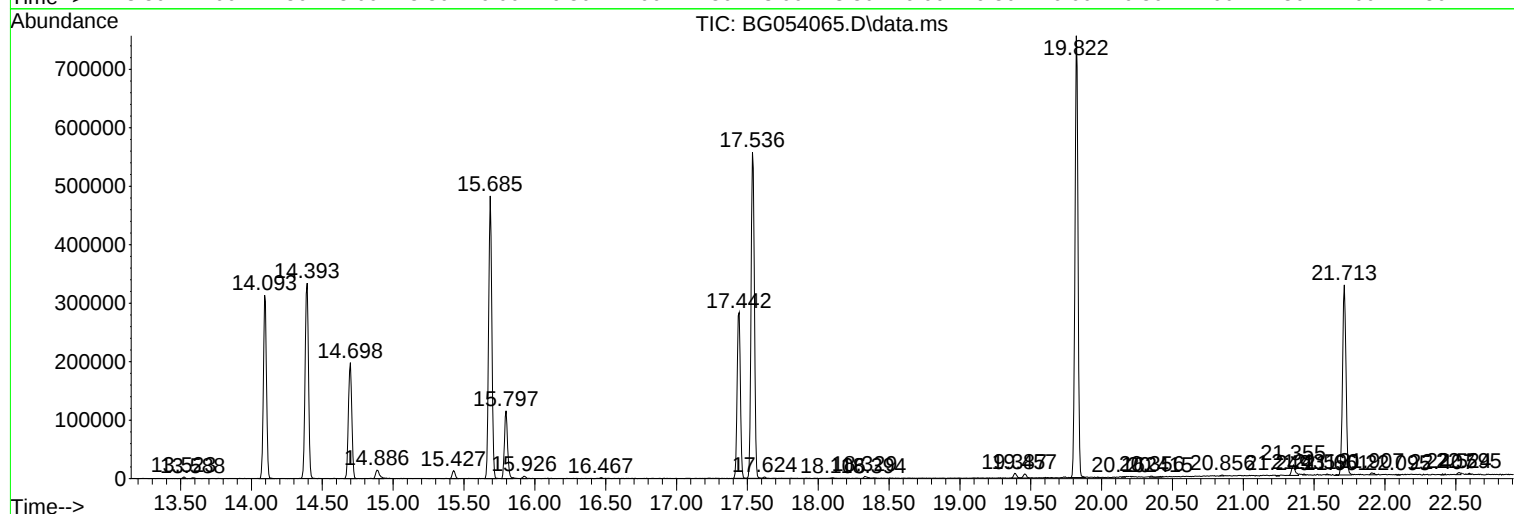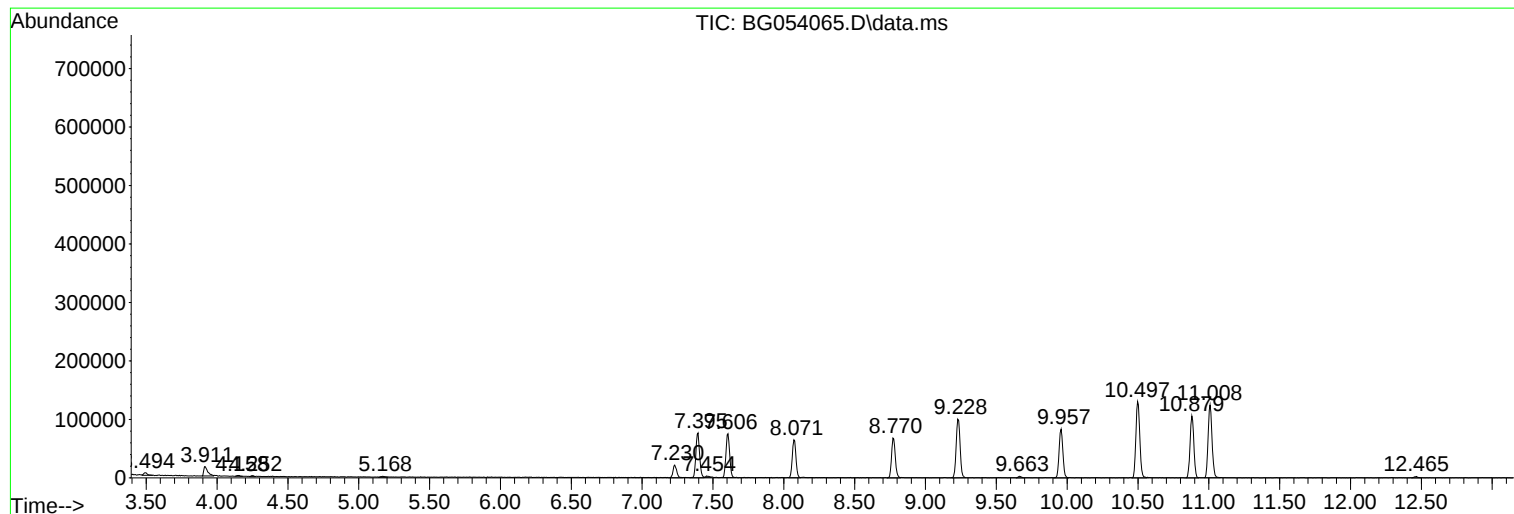

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054065.D
Acq On : 25 Jun 2022 17:20
Operator : CG/JU
Sample : N3401-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054065.D
Acq On : 25 Jun 2022 17:20
Operator : CG/JU
Sample : N3401-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------