

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054067.D
 Acq On : 25 Jun 2022 18:38
 Operator : CG/JU
 Sample : PB145715BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK715

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054067.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.494	14	18	25	rVB4	5511	9931	1.09%	0.122%
2	3.576	30	32	35	rBV3	1584	1363	0.15%	0.017%
3	3.905	84	88	102	rBV	61620	116152	12.74%	1.427%
4	4.246	144	146	149	rBV3	1222	1210	0.13%	0.015%
5	5.045	279	282	286	rBV3	838	1089	0.12%	0.013%
6	5.556	368	369	374	rBV3	805	1244	0.14%	0.015%
7	7.230	647	654	664	rVB	89001	157976	17.32%	1.941%
8	7.389	673	681	692	rBV	62210	111757	12.25%	1.373%
9	7.606	711	718	726	rVV	79403	146624	16.08%	1.802%
10	8.071	790	797	806	rBV2	65022	117417	12.88%	1.443%
11	8.770	910	916	928	rBV	116442	208460	22.86%	2.561%
12	9.228	987	994	1003	rBV	84797	157012	17.22%	1.929%
13	9.957	1112	1118	1127	rVB	69006	126045	13.82%	1.549%
14	10.497	1202	1210	1220	rBV	120432	221790	24.32%	2.725%
15	10.879	1266	1275	1286	rBB	106531	198058	21.72%	2.434%
16	11.008	1290	1297	1310	rVV	118863	224157	24.58%	2.754%
17	12.465	1539	1545	1549	rVB3	1434	2774	0.30%	0.034%
18	14.093	1816	1822	1831	rVB	259109	391226	42.90%	4.807%
19	14.393	1865	1873	1882	rBV	266629	451260	49.48%	5.545%
20	14.698	1918	1925	1934	rBV	202045	334579	36.69%	4.111%
21	14.880	1950	1956	1972	rBV	87497	158759	17.41%	1.951%
22	14.986	1972	1974	1980	rVB3	914	1209	0.13%	0.015%
23	15.685	2085	2093	2101	rBV	405234	619413	67.92%	7.611%
24	15.797	2106	2112	2122	rVV	96937	152317	16.70%	1.871%
25	15.926	2125	2134	2138	rVB2	3545	6245	0.68%	0.077%
26	16.467	2224	2226	2230	rBV3	1100	1219	0.13%	0.015%
27	17.236	2351	2357	2361	rBV4	635	1407	0.15%	0.017%
28	17.442	2385	2392	2399	rVV	289647	459176	50.35%	5.642%
29	17.536	2401	2408	2417	rVV	454405	719030	78.85%	8.835%
30	18.194	2516	2520	2523	rBV3	668	988	0.11%	0.012%
31	19.140	2678	2681	2686	rBV3	611	1240	0.14%	0.015%
32	19.387	2719	2723	2728	rBV	5952	8219	0.90%	0.101%
33	19.463	2730	2736	2739	rBV	5432	7374	0.81%	0.091%
34	19.822	2790	2797	2804	rBV	634220	911952	100.00%	11.205%
35	19.910	2810	2812	2816	rBV3	1061	1331	0.15%	0.016%
36	20.603	2925	2930	2931	rBV4	831	1132	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
 Data File : BG054067.D
 Acq On : 25 Jun 2022 18:38
 Operator : CG/JU
 Sample : PB145715BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK715

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	20.650	2934	2938	2943	rVB3	1162	2196	0.24%	0.027%
38	21.055	3004	3007	3008	rBV3	1099	1101	0.12%	0.014%
39	21.073	3008	3010	3013	rBV4	955	1060	0.12%	0.013%
40	21.120	3017	3018	3020	rBV2	1152	1174	0.13%	0.014%
41	21.261	3040	3042	3045	rVV3	1072	1047	0.11%	0.013%
42	21.343	3054	3056	3058	rBV3	1220	980	0.11%	0.012%
43	21.390	3061	3064	3067	rBV3	1193	1934	0.21%	0.024%
44	21.420	3067	3069	3072	rBV3	974	959	0.11%	0.012%
45	21.584	3095	3097	3098	rBV2	2755	1811	0.20%	0.022%
46	21.713	3111	3119	3128	rBV	330288	551736	60.50%	6.779%
47	22.354	3226	3228	3231	rVB3	1870	1518	0.17%	0.019%
48	22.383	3231	3233	3234	rBV	1739	1286	0.14%	0.016%
49	22.583	3265	3267	3270	rBV3	1097	1186	0.13%	0.015%
50	22.765	3297	3298	3302	rBV3	1225	1552	0.17%	0.019%
51	22.800	3302	3304	3307	rVV4	1173	1081	0.12%	0.013%
52	23.165	3361	3366	3368	rBV5	1955	3389	0.37%	0.042%
53	23.229	3373	3377	3381	rVB5	3111	5361	0.59%	0.066%
54	23.265	3381	3383	3387	rBV4	1035	1124	0.12%	0.014%
55	23.317	3389	3392	3393	rBV2	1796	1607	0.18%	0.020%
56	23.329	3393	3394	3396	rBV2	1694	1318	0.14%	0.016%
57	23.723	3459	3461	3463	rBV2	1271	1274	0.14%	0.016%
58	23.811	3474	3476	3479	rBV2	1495	1774	0.19%	0.022%
59	24.052	3513	3517	3522	rVB6	4903	9191	1.01%	0.113%
60	24.475	3587	3589	3593	rBV4	1188	1178	0.13%	0.014%
61	24.745	3623	3635	3648	rBV2	298334	903055	99.02%	11.096%
62	24.968	3660	3673	3687	rBV2	176767	554276	60.78%	6.810%
63	25.168	3706	3707	3713	rBV4	1336	1503	0.16%	0.018%
64	25.292	3726	3728	3730	rBV3	1620	1461	0.16%	0.018%
65	25.521	3765	3767	3769	rBV3	1245	1677	0.18%	0.021%
66	25.568	3773	3775	3777	rBV3	1212	936	0.10%	0.012%
67	25.691	3794	3796	3797	rBV2	1191	1014	0.11%	0.012%
68	26.161	3872	3876	3879	rVB4	4329	6115	0.67%	0.075%
69	26.255	3890	3892	3895	rBV2	1536	1465	0.16%	0.018%
70	26.379	3910	3913	3915	rBV3	1603	1751	0.19%	0.022%
71	26.913	4002	4004	4007	rBV4	1302	1345	0.15%	0.017%
72	27.042	4024	4026	4028	rVB3	1414	1021	0.11%	0.013%
73	27.513	4102	4106	4107	rBV4	3846	3851	0.42%	0.047%
74	28.094	4203	4205	4206	rBV2	1888	1130	0.12%	0.014%
75	28.570	4283	4286	4287	rBV3	1653	1447	0.16%	0.018%
76	29.046	4365	4367	4369	rBV3	1247	984	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054067.D
Acq On : 25 Jun 2022 18:38
Operator : CG/JU
Sample : PB145715BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK715

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Title : SVOA CALIBRATION

77	29.211	4387	4395	4404	rVB10	4069	15461	1.70%	0.190%
78	29.428	4431	4432	4435	rVB3	1760	1054	0.12%	0.013%
79	29.528	4447	4449	4453	rBV3	1510	1597	0.18%	0.020%
80	29.592	4458	4460	4461	rBV2	1267	931	0.10%	0.011%
81	30.409	4597	4599	4601	rVB3	1232	1029	0.11%	0.013%
82	30.721	4650	4652	4654	rBV3	1292	1206	0.13%	0.015%
83	30.909	4682	4684	4687	rBV3	1330	1459	0.16%	0.018%
84	31.343	4755	4758	4759	rBV2	1403	1331	0.15%	0.016%
85	31.361	4759	4761	4763	rBV2	1199	1127	0.12%	0.014%
86	32.336	4923	4927	4928	rBV4	1463	1576	0.17%	0.019%
87	32.448	4944	4946	4948	rVB3	1598	1024	0.11%	0.013%




Sum of corrected areas: 8138798

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054067.D
Acq On : 25 Jun 2022 18:38
Operator : CG/JU
Sample : PB145715BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK715

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

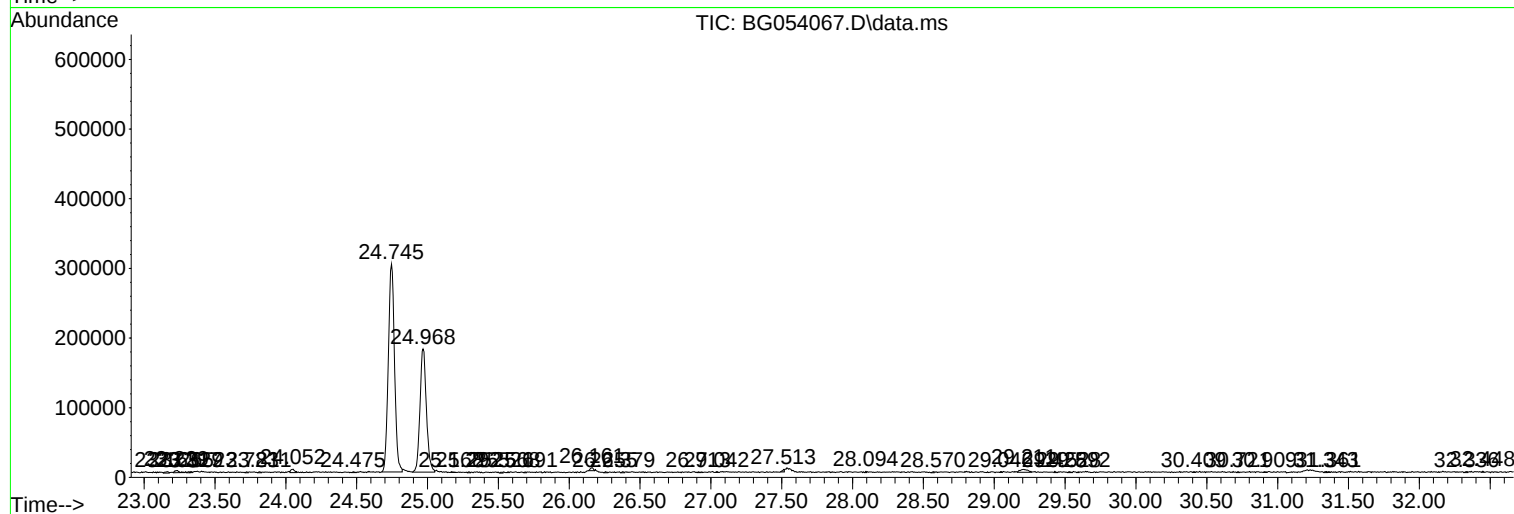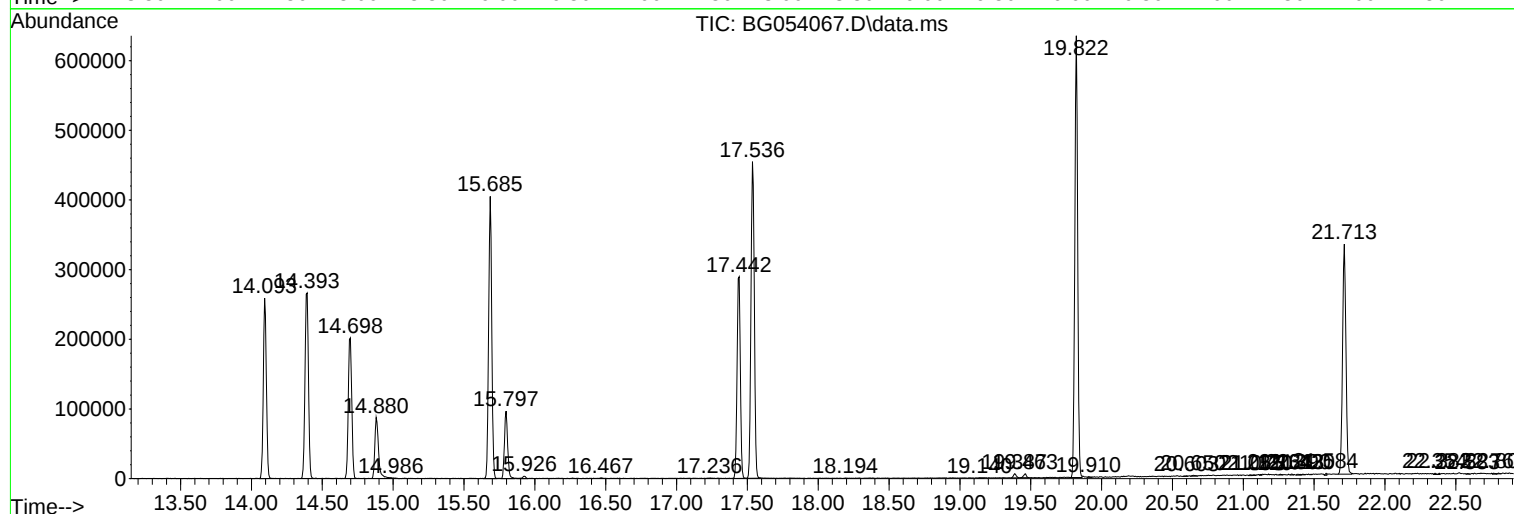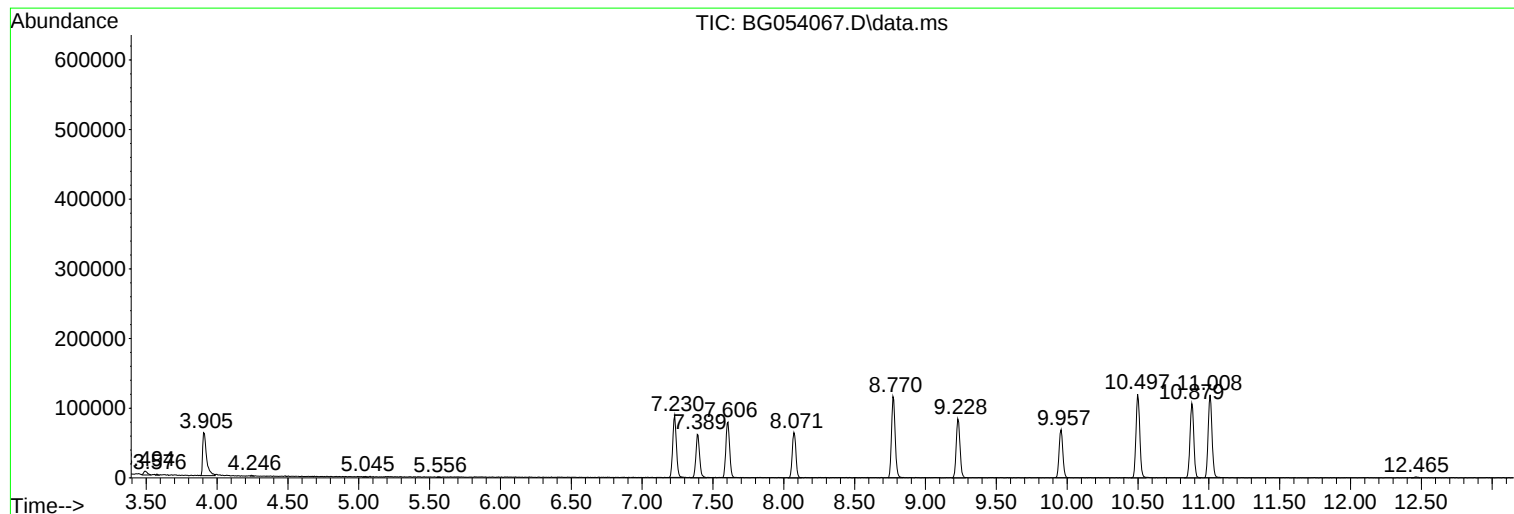

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054067.D
Acq On : 25 Jun 2022 18:38
Operator : CG/JU
Sample : PB145715BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK715

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062522\
Data File : BG054067.D
Acq On : 25 Jun 2022 18:38
Operator : CG/JU
Sample : PB145715BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK715

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------