

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062616\
 Data File : BG022609.D
 Acq On : 26 Jun 2016 14:05
 Operator : UM/SJ
 Sample : H3738-01
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 W-03

Quant Time: Jun 27 01:51:05 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 20:14:59 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	145951	20.00	ng	0.00
21) Naphthalene-d8	10.98	136	595539	20.00	ng	0.00
38) Acenaphthene-d10	14.80	164	409509	20.00	ng	0.00
63) Phenanthrene-d10	17.55	188	1069355	20.00	ng	0.00
75) Chrysene-d12	21.85	240	1247849	20.00	ng	0.00
86) Perylene-d12	25.21	264	1300461	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.70	112	465858	51.20	ng	0.00
7) Phenol-d6	7.31	99	419249	32.69	ng	0.00
23) Nitrobenzene-d5	9.33	82	1148816	81.64	ng	0.00
41) 2,4,6-Tribromophenol	16.29	330	941056	146.10	ng	0.00
44) 2-Fluorobiphenyl	13.42	172	2238266	86.68	ng	0.00
78) Terphenyl-d14	20.16	244	3316321	70.41	ng	0.00


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062616\
Data File : BG022609.D
Acq On : 26 Jun 2016 14:05
Operator : UM/SJ
Sample : H3738-01
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
W-03

Quant Time: Jun 27 01:51:05 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

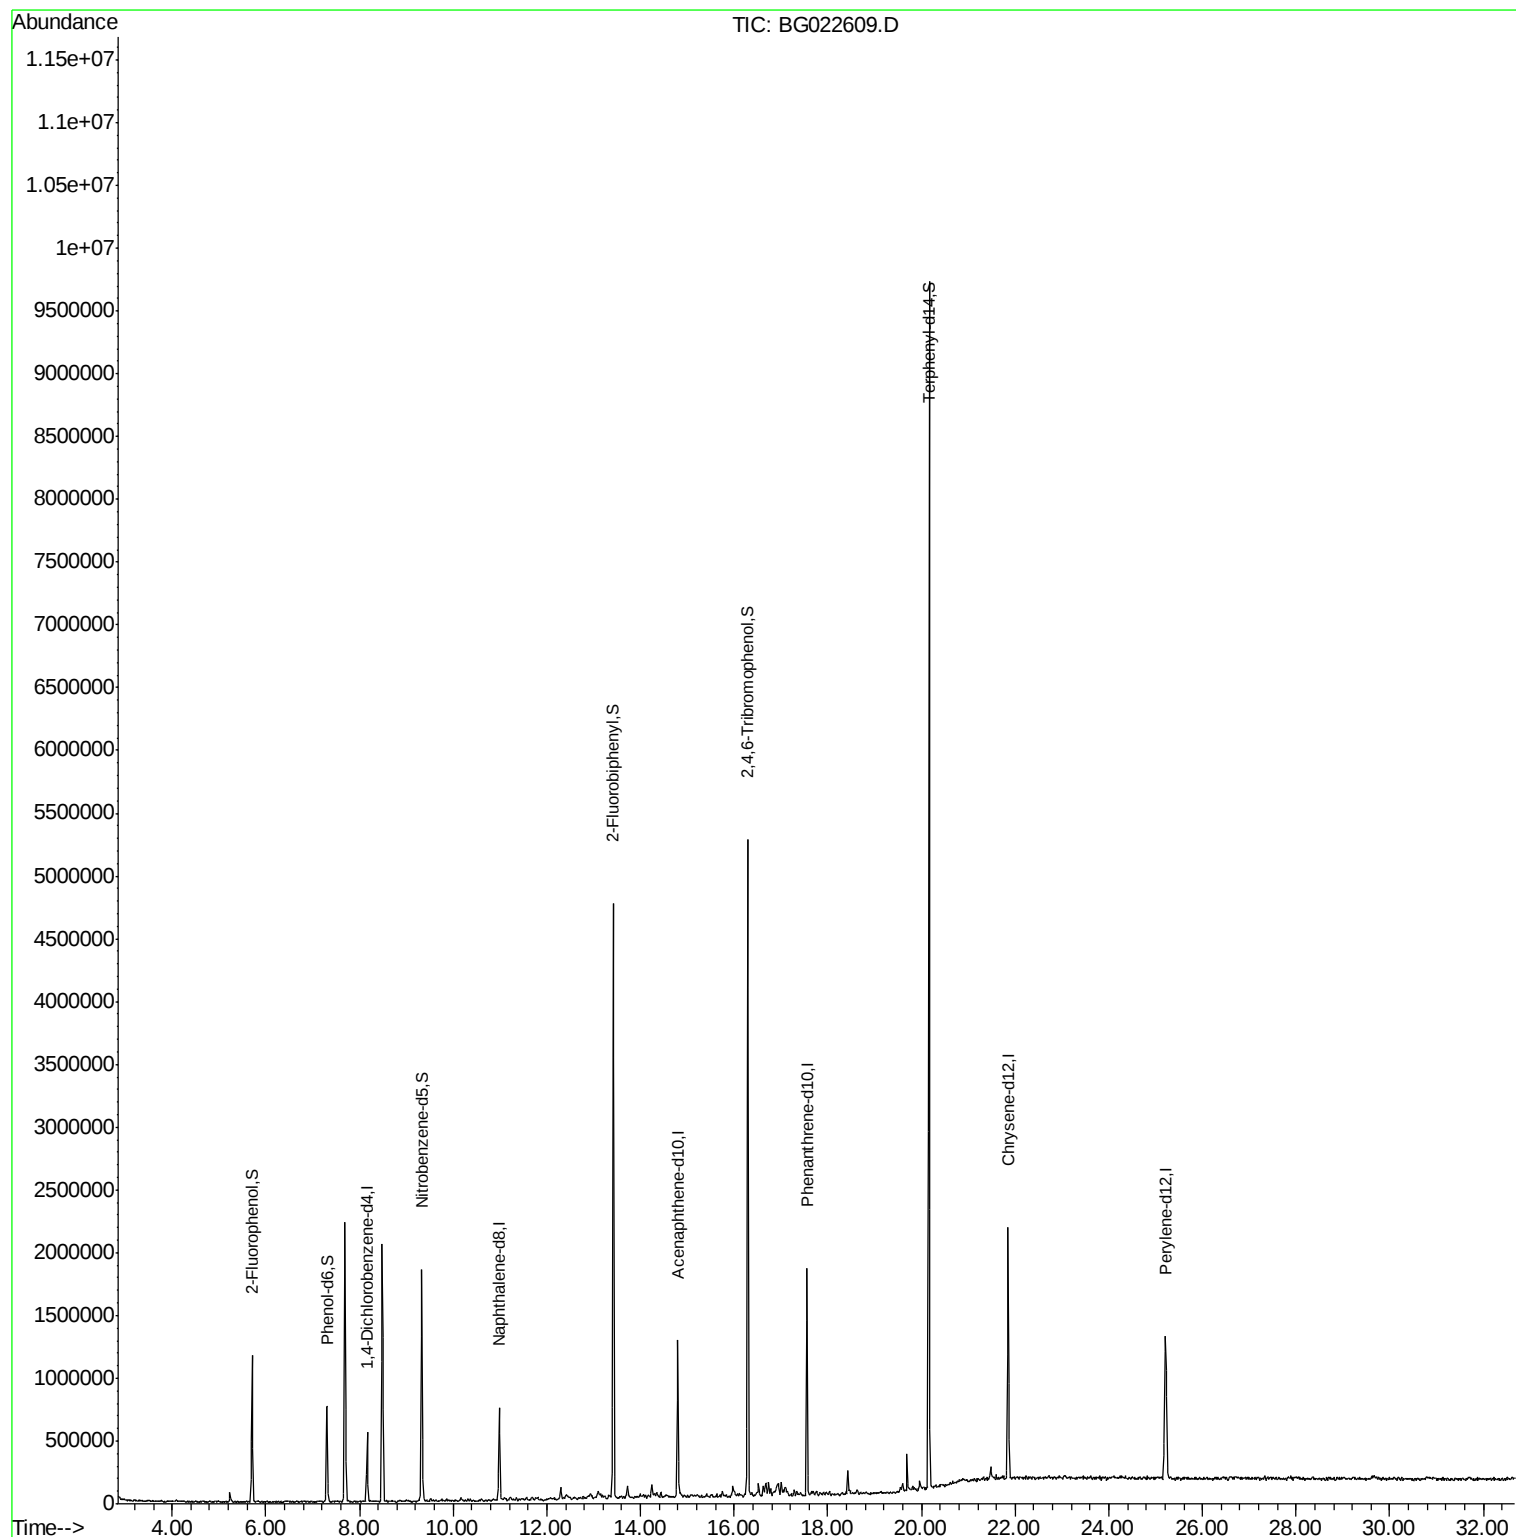



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.16 min Scan# 906

Delta R.T. -0.01 min

Lab File: BG022609.D

Acq: 26 Jun 2016 14:05

Instrument :

BNA_G

ClientSampleId :

W-03


Tgt Ion:152 Resp: 145951

Ion Ratio Lower Upper

152 100

150 159.5 144.7 217.1




115 67.4 64.0 96.0

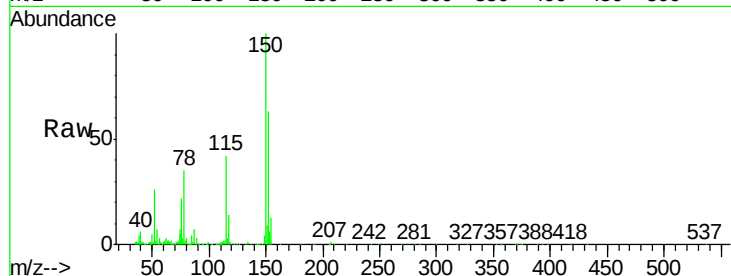

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

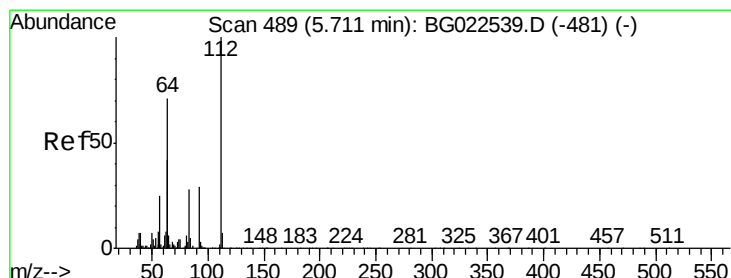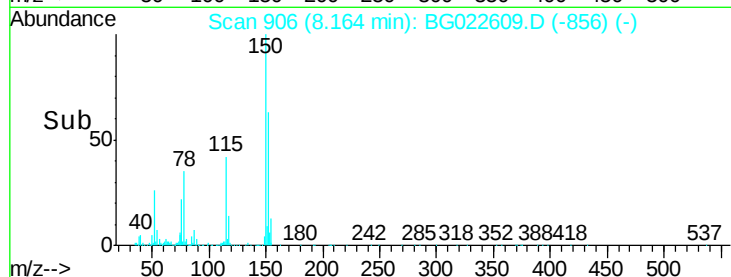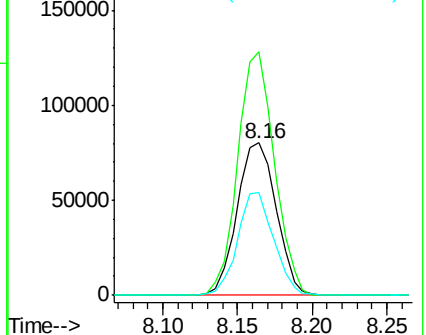

#5

2-Fluorophenol

Concen: 51.20 ng

RT: 5.70 min Scan# 487

Delta R.T. -0.00 min

Lab File: BG022609.D

Acq: 26 Jun 2016 14:05


Tgt Ion:112 Resp: 465858

Ion Ratio Lower Upper

112 100

64 71.8 59.0 88.4



63 38.5 37.8 56.8

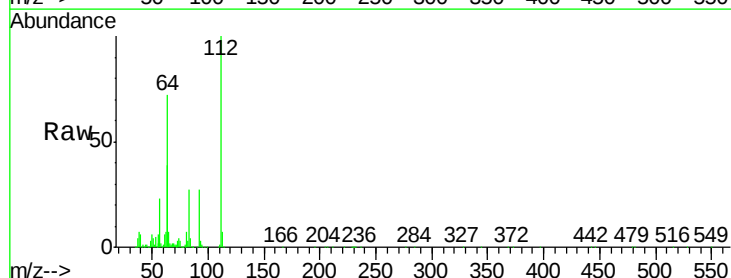

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

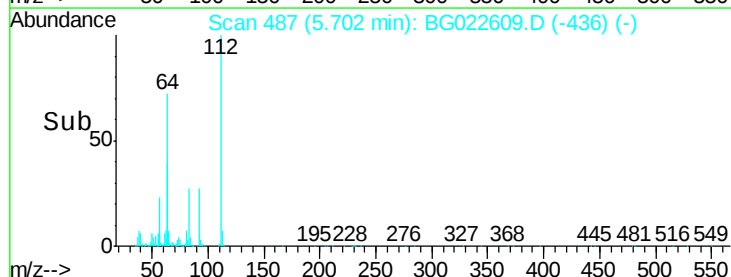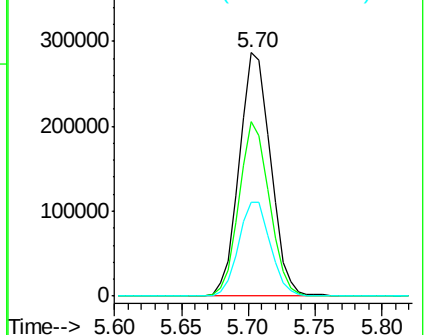



#7

Phenol-d6

Concen: 32.69 ng

RT: 7.31 min Scan# 760

Delta R.T. 0.00 min

Lab File: BG022609.D

Acq: 26 Jun 2016 14:05

Instrument :

BNA_G

ClientSampleId :

W-03


Tgt Ion: 99 Resp: 419249

Ion Ratio Lower Upper



99 100

42 19.7 17.8 26.6

71 47.7 41.5 62.3

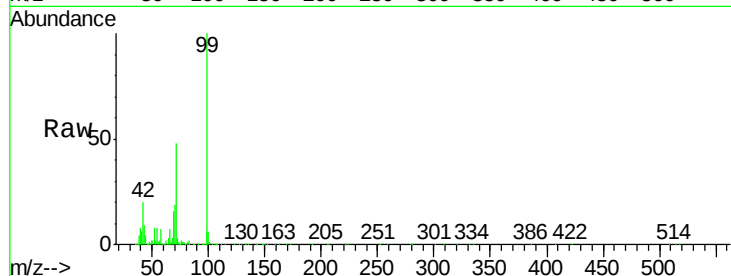

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

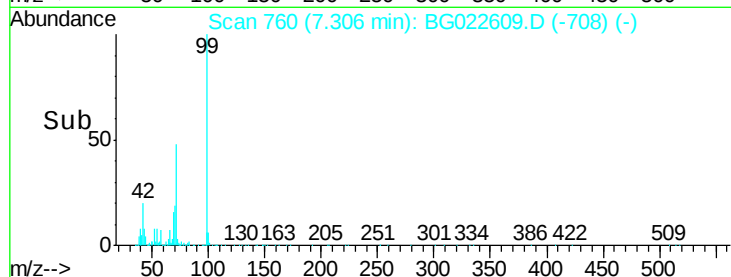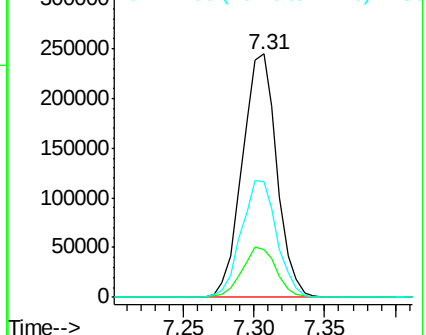

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.98 min Scan# 1386

Delta R.T. -0.01 min

Lab File: BG022609.D

Acq: 26 Jun 2016 14:05

Tgt Ion: 136 Resp: 595539


Ion Ratio Lower Upper

136 100



137 12.0 9.6 14.4


54 7.8 7.3 10.9

68 6.0 5.3 7.9

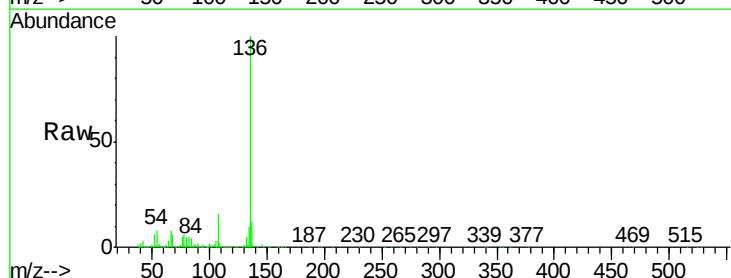

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



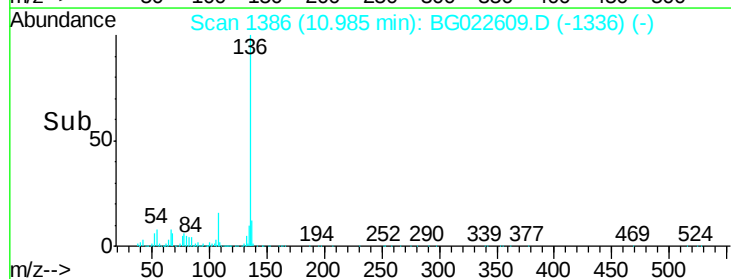
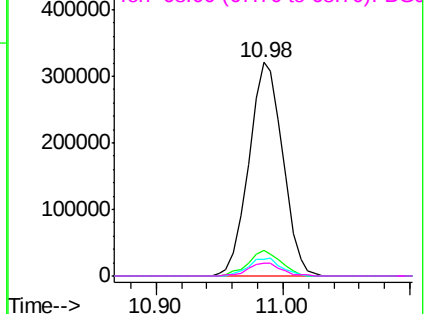


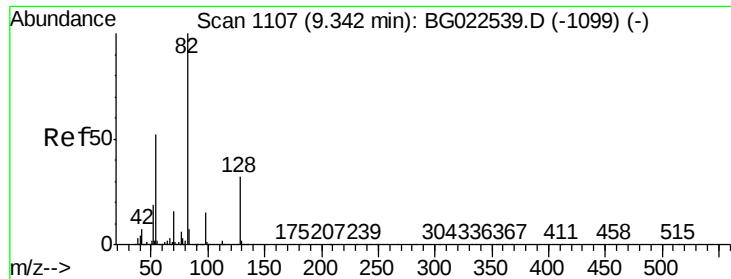

#23
 Nitrobenzene-d5
 Concen: 81.64 ng
 RT: 9.33 min Scan# 1105
 Delta R.T. -0.00 min
 Lab File: BG022609.D
 Acq: 26 Jun 2016 14:05




Instrument :
 BNA_G
 ClientSampleId :
 W-03


Tgt Ion: 82 Resp: 1148816
 Ion Ratio Lower Upper
 82 100
 128 34.0 24.4 36.6
 54 50.4 41.4 62.0

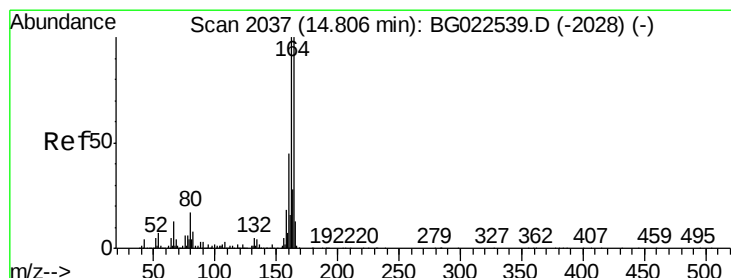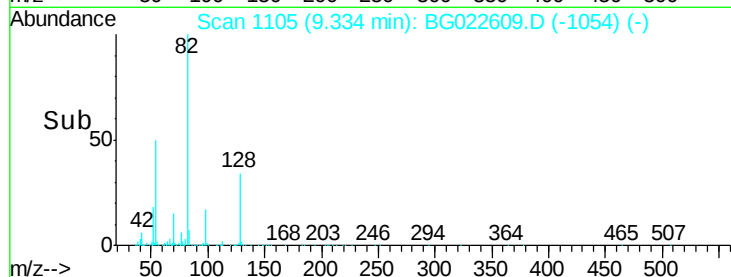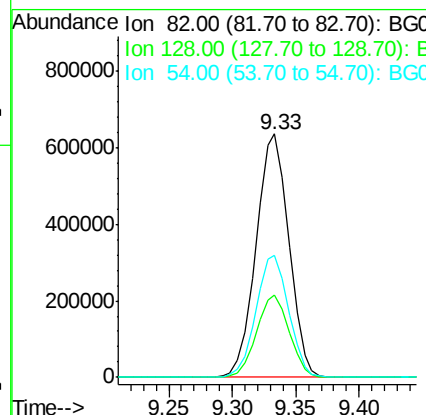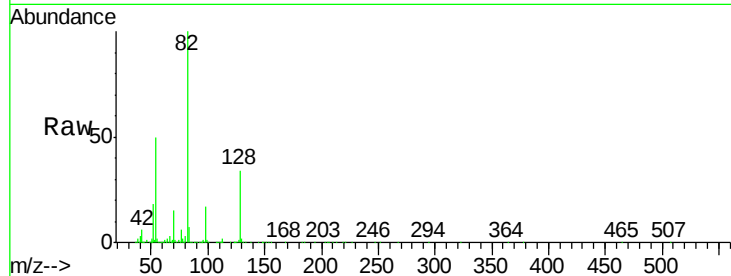

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.80 min Scan# 2035
 Delta R.T. -0.00 min
 Lab File: BG022609.D
 Acq: 26 Jun 2016 14:05

Tgt Ion: 164 Resp: 409509
 Ion Ratio Lower Upper
 164 100
 162 104.1 87.7 131.5
 160 45.5 37.2 55.8

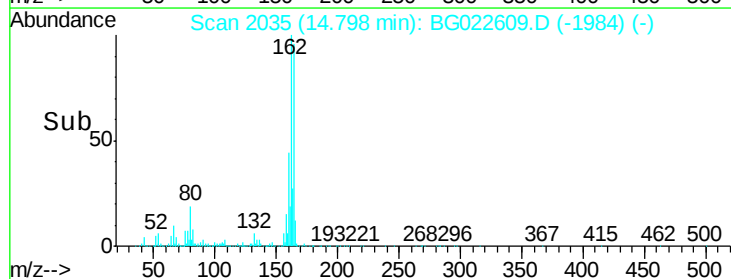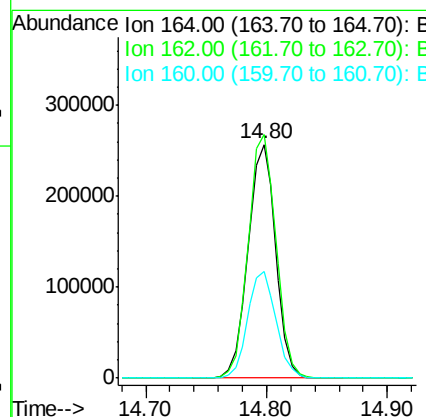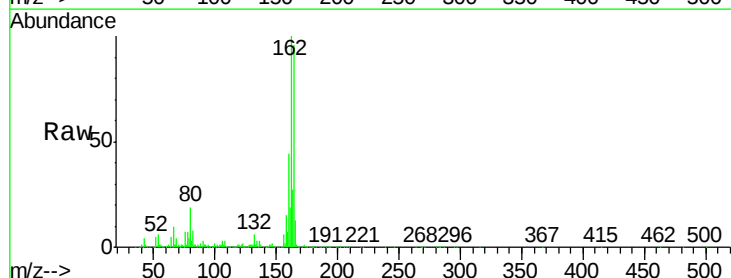


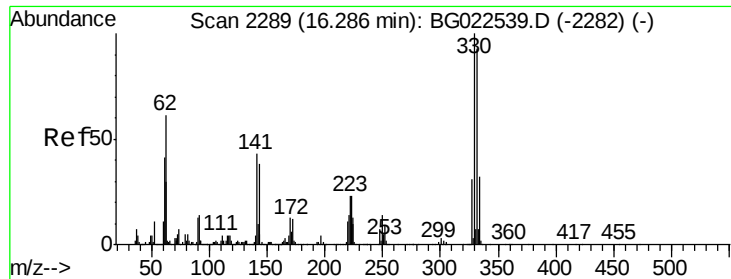




#41
 2,4,6-Tribromophenol
 Concen: 146.10 ng
 RT: 16.29 min Scan# 2289
 Delta R.T. 0.00 min
 Lab File: BG022609.D
 Acq: 26 Jun 2016 14:05

Instrument :
 BNA_G
 ClientSampleId :
 W-03

Tgt Ion:330 Resp: 941056
 Ion Ratio Lower Upper
 330 100
 332 97.1 77.4 116.2
 141 38.6 31.7 47.5

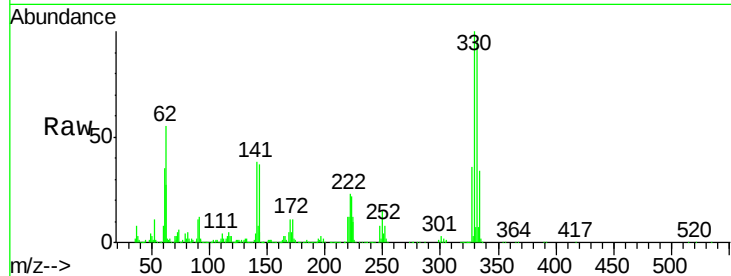


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

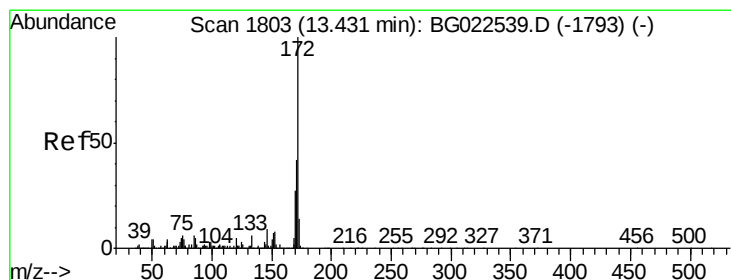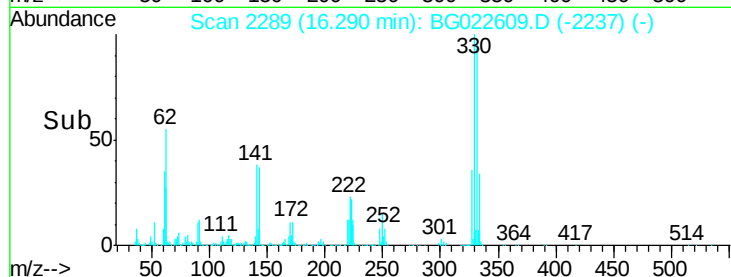
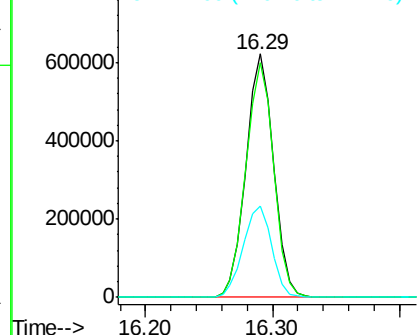



#44
 2-Fluorobiphenyl
 Concen: 86.68 ng
 RT: 13.42 min Scan# 1801
 Delta R.T. -0.00 min
 Lab File: BG022609.D
 Acq: 26 Jun 2016 14:05

Tgt Ion:172 Resp: 2238266
 Ion Ratio Lower Upper
 172 100
 171 42.2 31.6 47.4
 170 29.6 21.3 31.9

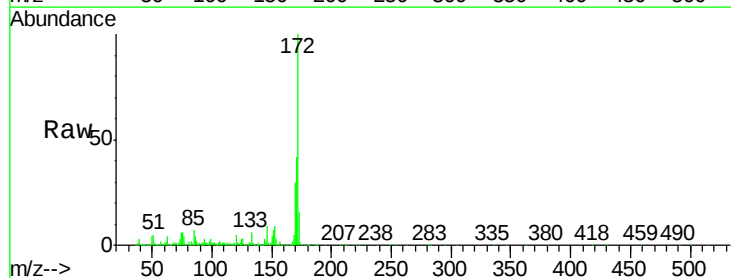

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

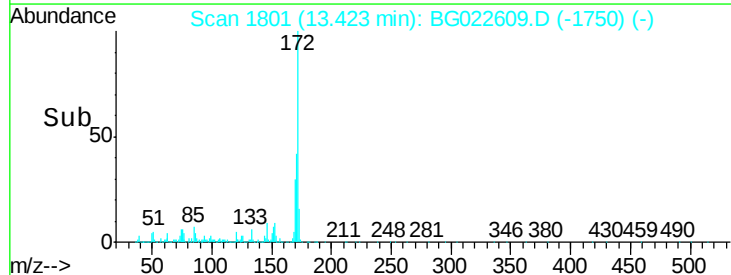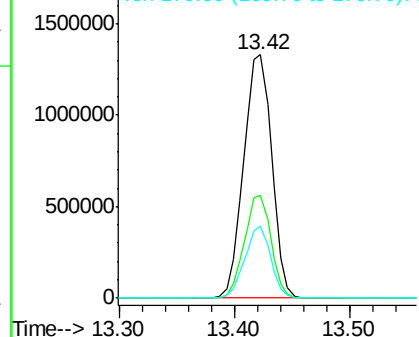

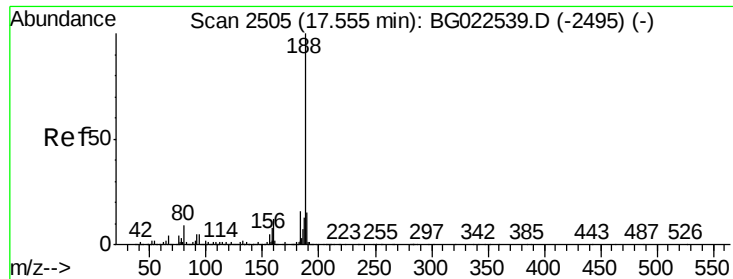

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.55 min Scan# 2504

Delta R.T. 0.00 min

Lab File: BG022609.D

Acq: 26 Jun 2016 14:05

Instrument :

BNA_G

ClientSampleId :

W-03


Tgt Ion:188 Resp: 1069355

Ion Ratio Lower Upper

188 100

94 6.9 5.2 7.8




80 8.2 7.2 10.8

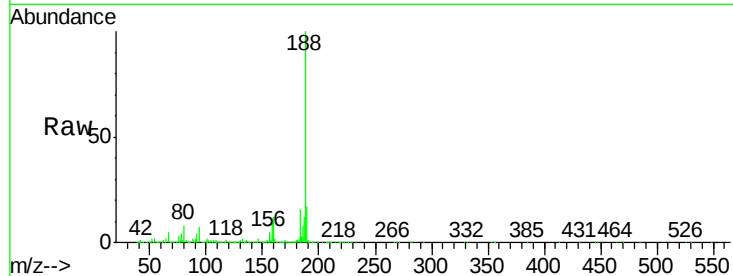

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

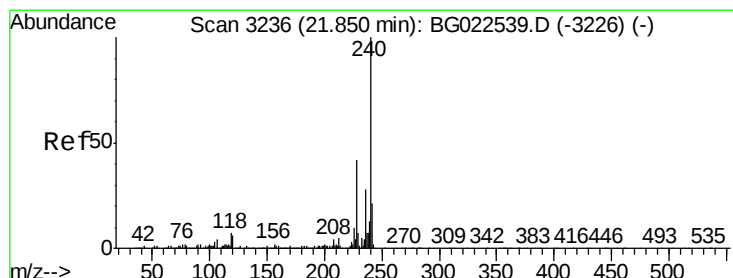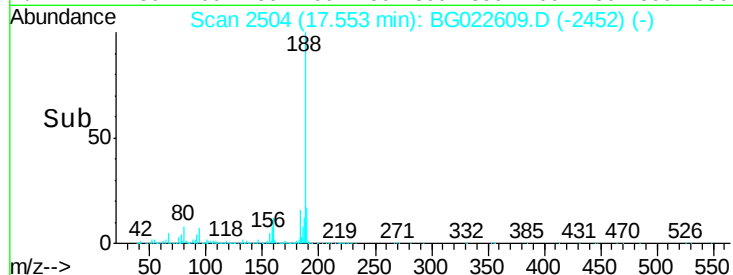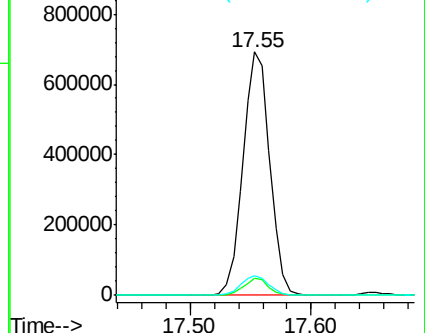

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.85 min Scan# 3235

Delta R.T. 0.00 min

Lab File: BG022609.D

Acq: 26 Jun 2016 14:05


Tgt Ion:240 Resp: 1247849

Ion Ratio Lower Upper

240 100

120 6.1 4.1 6.1



236 29.1 21.1 31.7

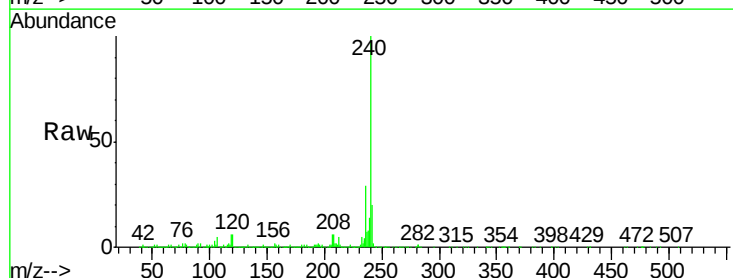


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

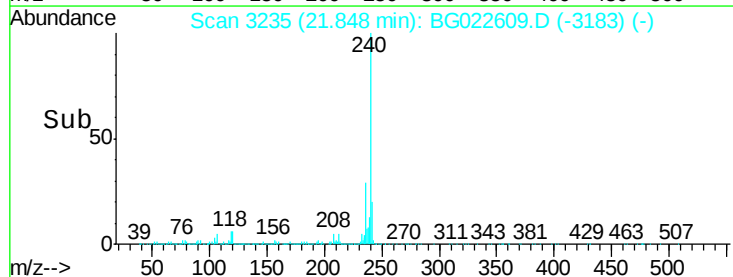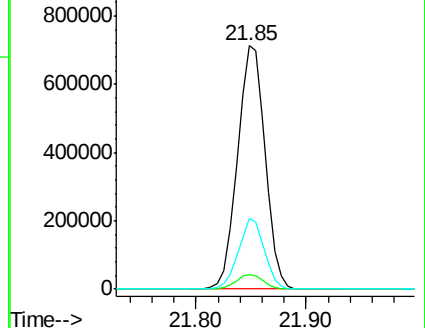

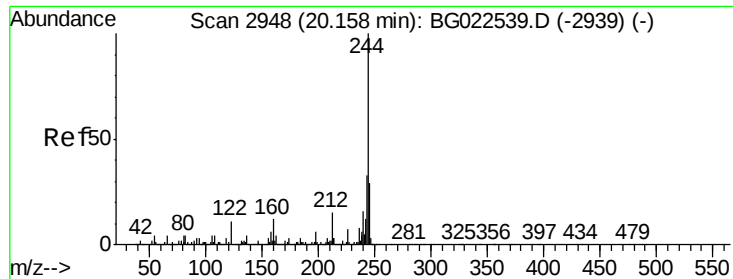

#78

Terphenyl-d14

Concen: 70.41 ng

RT: 20.16 min Scan# 2948

Delta R.T. 0.01 min

Lab File: BG022609.D

Acq: 26 Jun 2016 14:05

Instrument :

BNA_G

ClientSampleId :

W-03


Tgt Ion:244 Resp: 3316321

Ion Ratio Lower Upper

244 100

212 16.4 10.8 16.2#




122 12.3 8.0 12.0#

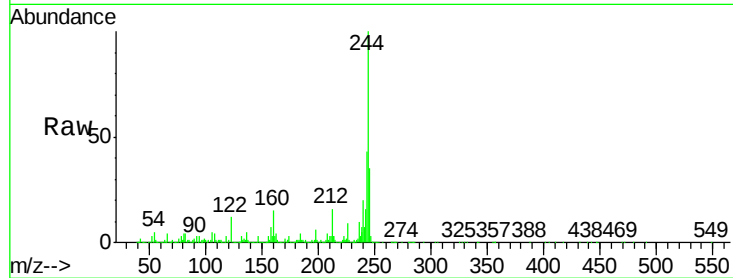

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

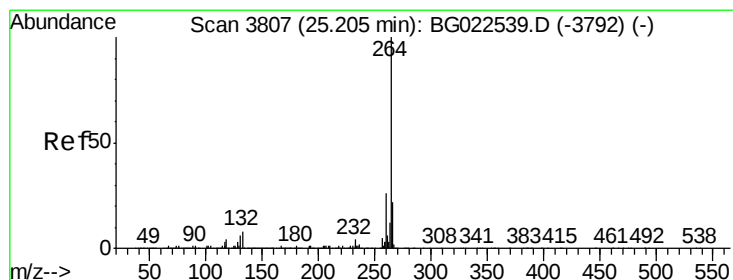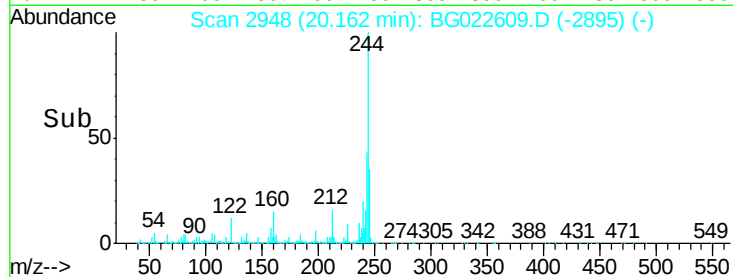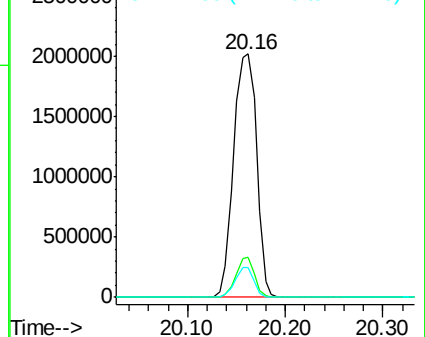

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.21 min Scan# 3808

Delta R.T. 0.01 min

Lab File: BG022609.D

Acq: 26 Jun 2016 14:05


Tgt Ion:264 Resp: 1300461

Ion Ratio Lower Upper

264 100

260 23.4 18.4 27.6

265 21.4 18.9 28.3

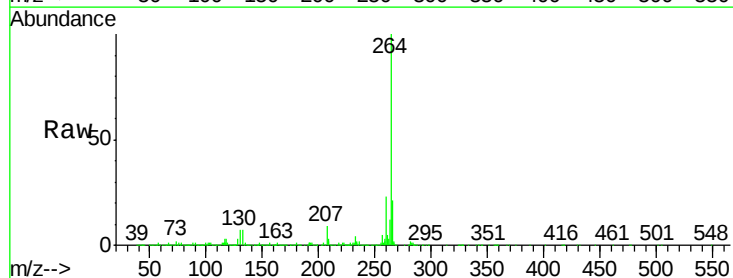

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

