


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062616\
 Data File : BG022579.D
 Acq On : 25 Jun 2016 18:06
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 24 20:14:59 2016

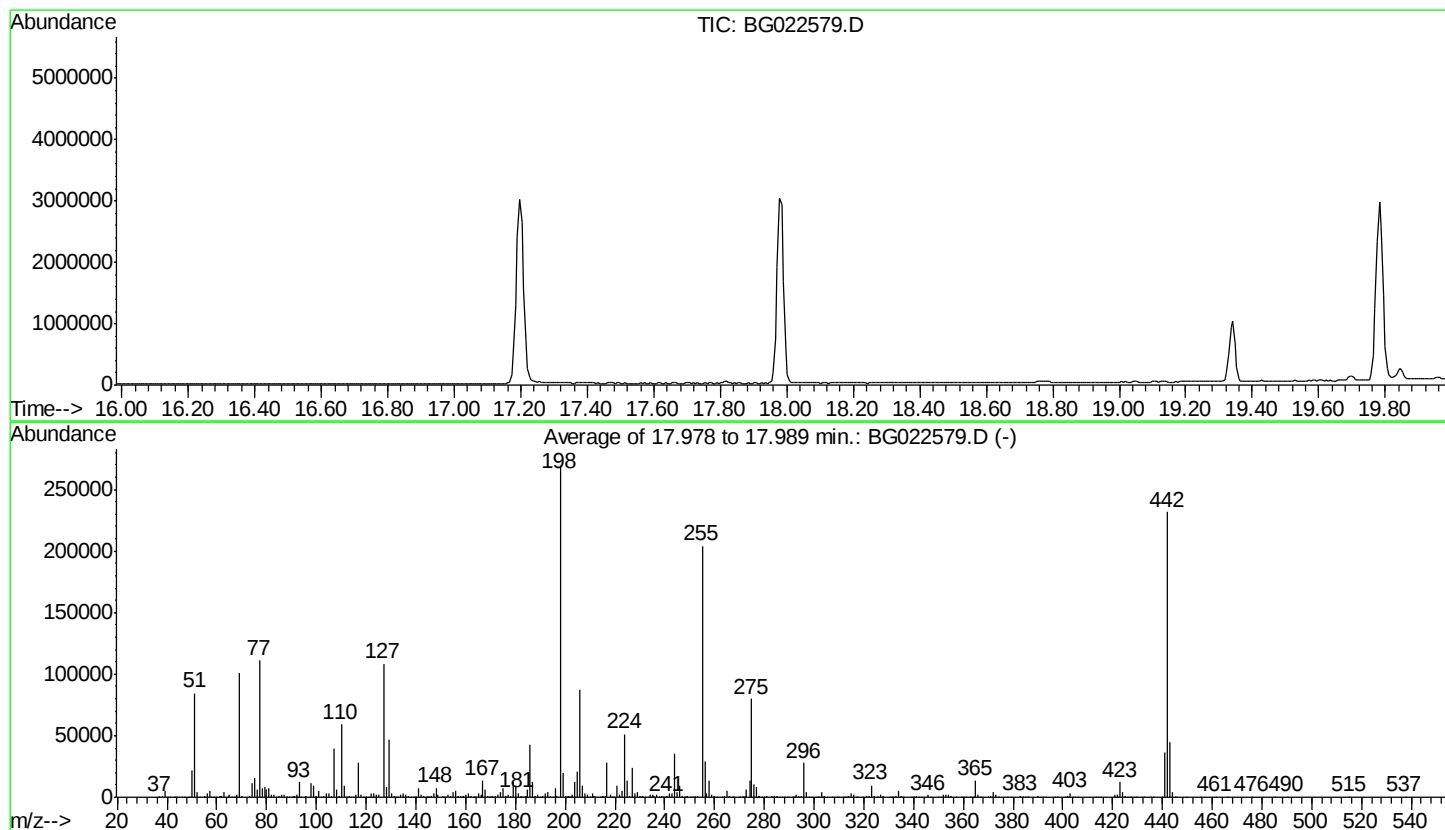

AutoFind: Scans 2577, 2578, 2579; Background Corrected with Scan 2570

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	84712	PASS
68	69	0.00	2	2.5	2494	FAIL*
69	198	0.00	100	37.4	100834	PASS
70	69	0.00	2	0.8	762	PASS
127	198	10	80	40.3	108476	PASS
197	198	0.00	2	0.4	1007	PASS
198	198	100	100	100.0	269397	PASS
199	198	5	9	7.5	20200	PASS
275	198	10	60	29.7	79906	PASS
365	198	1	100	4.9	13158	PASS
441	442	0.01	24	15.6	36045	PASS
442	198	50	100	86.0	231616	PASS
443	442	15	24	19.5	45074	PASS