


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062616\
 Data File : BG022596.D
 Acq On : 26 Jun 2016 5:26
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 24 20:14:59 2016

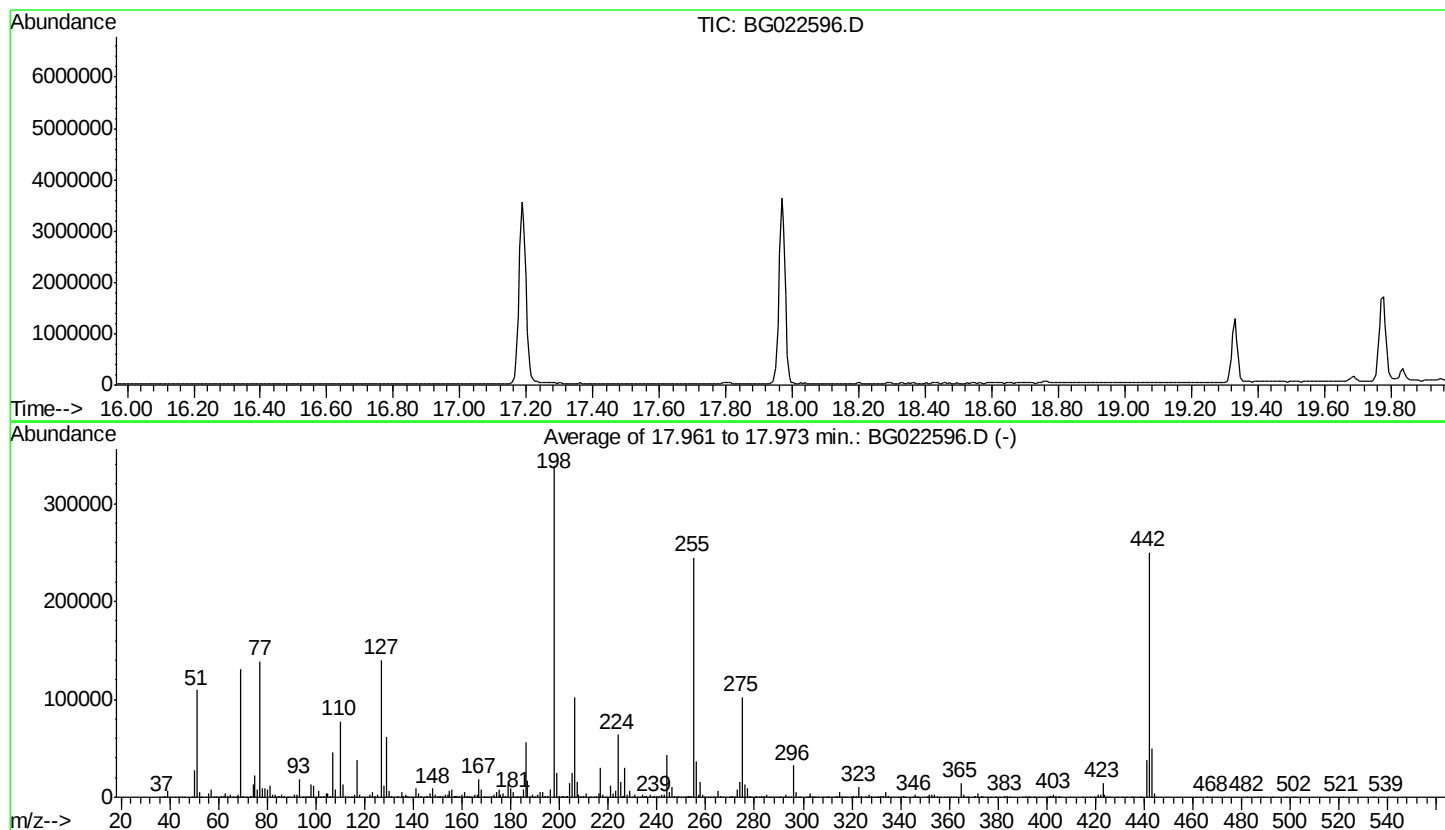

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	109570	PASS
68	69	0.00	2	1.7	2166	PASS
69	198	0.00	100	38.5	130237	PASS
70	69	0.00	2	0.6	823	PASS
127	198	10	80	41.5	140437	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	338688	PASS
199	198	5	9	7.4	25045	PASS
275	198	10	60	30.2	102290	PASS
365	198	1	100	4.3	14547	PASS
441	442	0.01	24	15.2	38008	PASS
442	198	50	100	73.8	249877	PASS
443	442	15	24	19.8	49592	PASS