


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062616\
 Data File : BG022615.D
 Acq On : 26 Jun 2016 18:44
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 24 20:14:59 2016

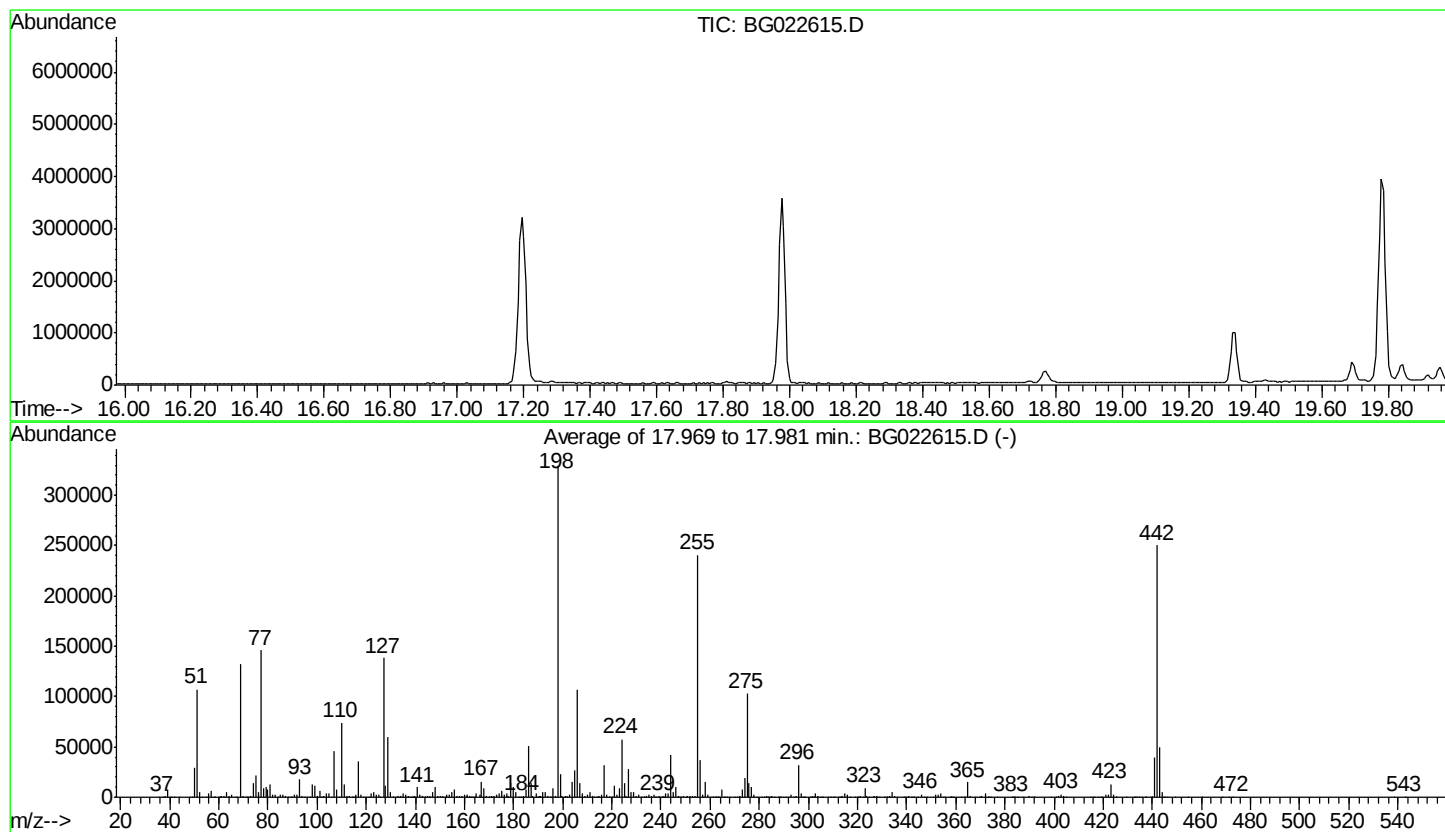

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	107274	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.3	132698	PASS
70	69	0.00	2	0.6	758	PASS
127	198	10	80	41.9	138090	PASS
197	198	0.00	2	0.5	1786	PASS
198	198	100	100	100.0	329408	PASS
199	198	5	9	7.0	23128	PASS
275	198	10	60	31.1	102560	PASS
365	198	1	100	4.5	14744	PASS
441	442	0.01	24	15.9	39850	PASS
442	198	50	100	75.9	250112	PASS
443	442	15	24	20.1	50237	PASS