
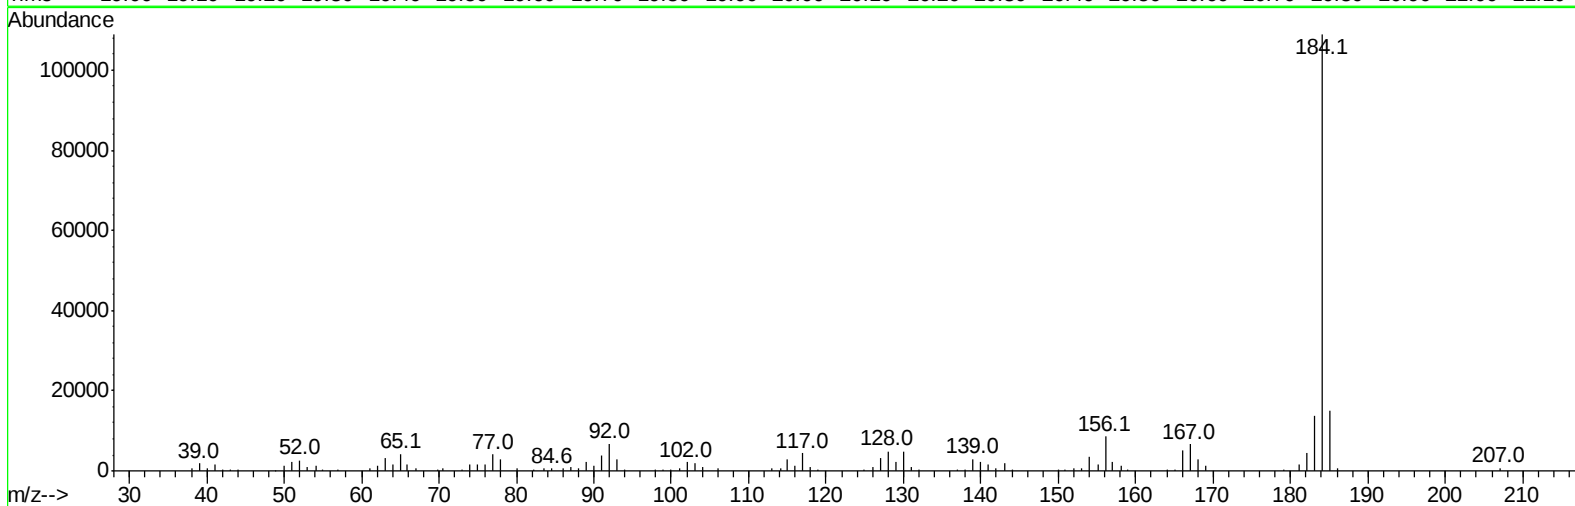


Data Path : Z:\HPCHEM1\BNA G\DATA\BG062617\
Data File : BG027675.D
Acq On : 26 Jun 2017 15:07
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 09:09:05 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 18:52:15 2017
Response via : Initial Calibration

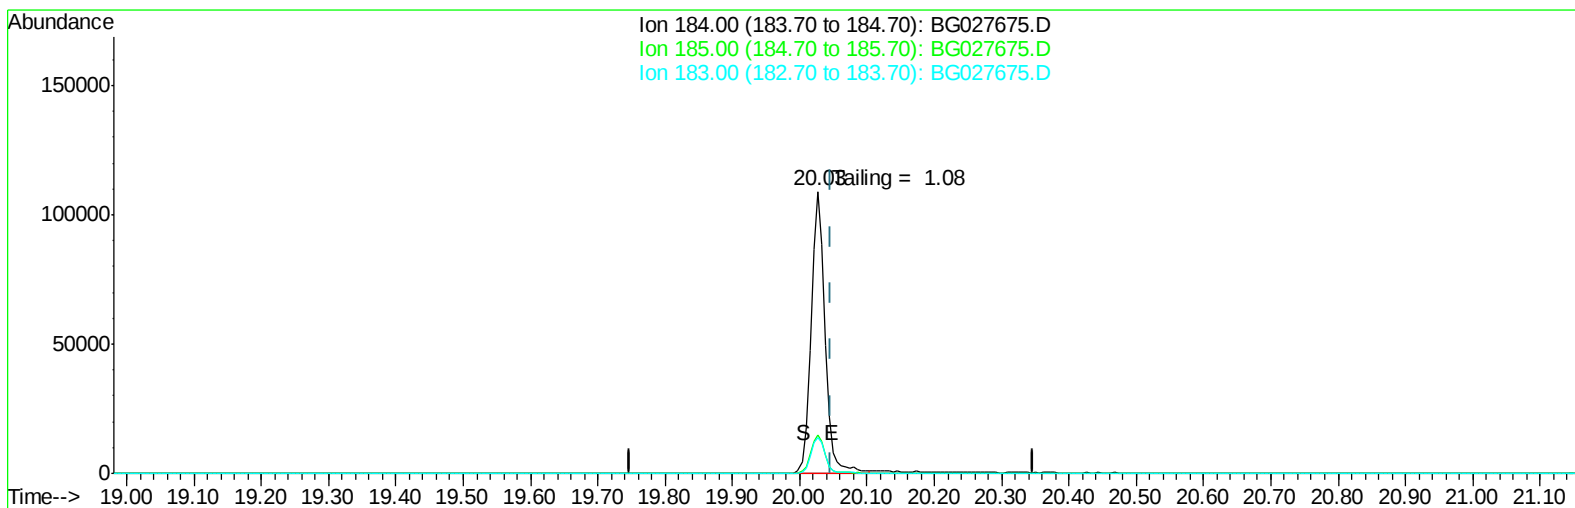

TIC: BG027675.D

(76) Benzidine



20.027min (-0.021) 0.00ng

response 162860

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.82
183.00	13.80	12.53
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062617\
Data File : BG027675.D
Acq On : 26 Jun 2017 15:07
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 09:09:05 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 18:52:15 2017
Response via : Initial Calibration

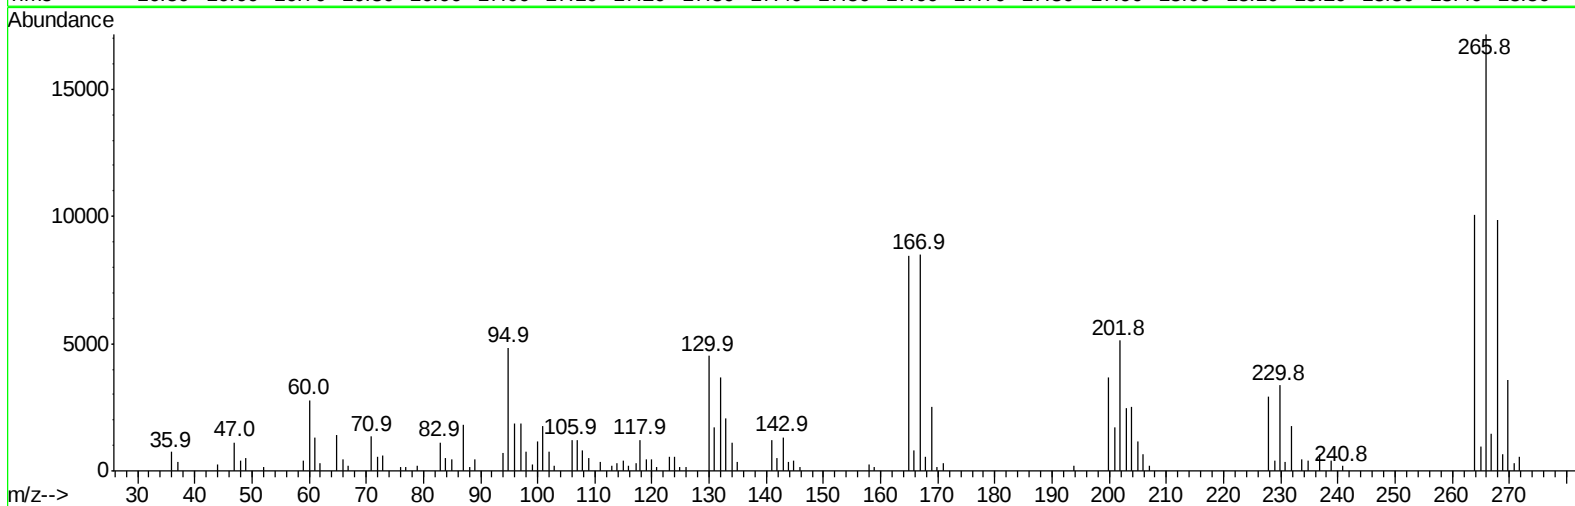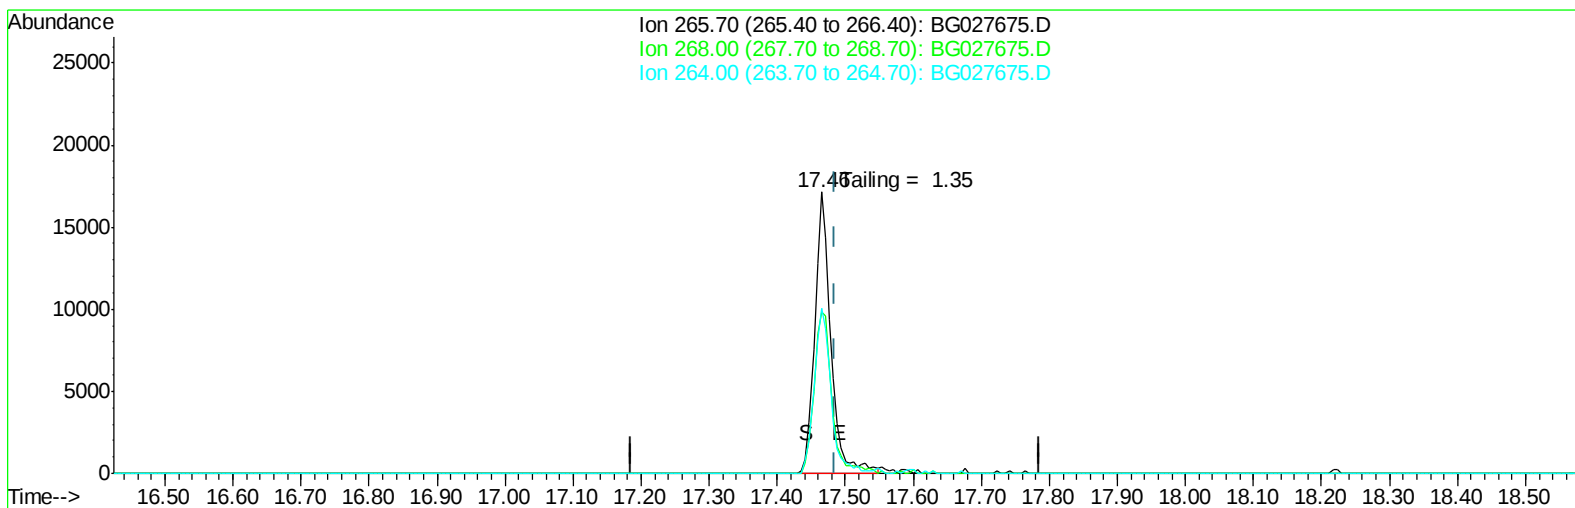

TIC: BG027675.D

(69) Pentachlorophenol (C)

17.465min (-0.021) 0.00ng

response 28626

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	57.39
264.00	62.60	58.73
0.00	0.00	0.00