


Data Path : Z:\HPCHEM1\BNA G\Data\BG062617\
 Data File : BG027675.D
 Acq On : 26 Jun 2017 15:07
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 21 18:52:15 2017

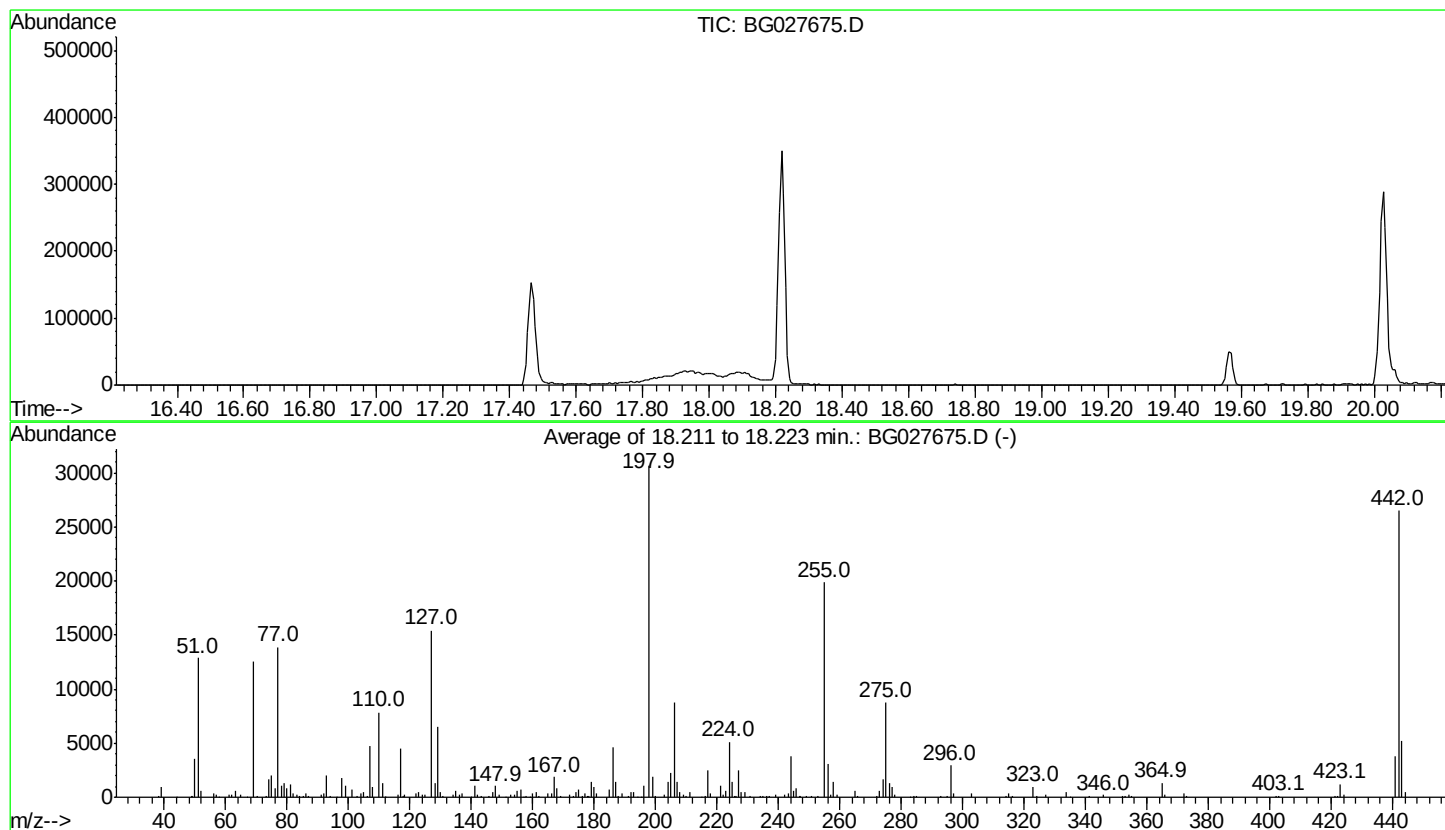

AutoFind: Scans 2438, 2439, 2440; Background Corrected with Scan 2432

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	12909	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.8	12510	PASS
70	69	0.00	2	1.2	154	PASS
127	198	10	80	50.3	15425	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	30680	PASS
199	198	5	9	6.3	1945	PASS
275	198	10	60	28.5	8758	PASS
365	198	1	100	4.3	1310	PASS
441	442	0.01	24	14.3	3791	PASS
442	198	50	100	86.3	26488	PASS
443	442	15	24	19.7	5230	PASS