



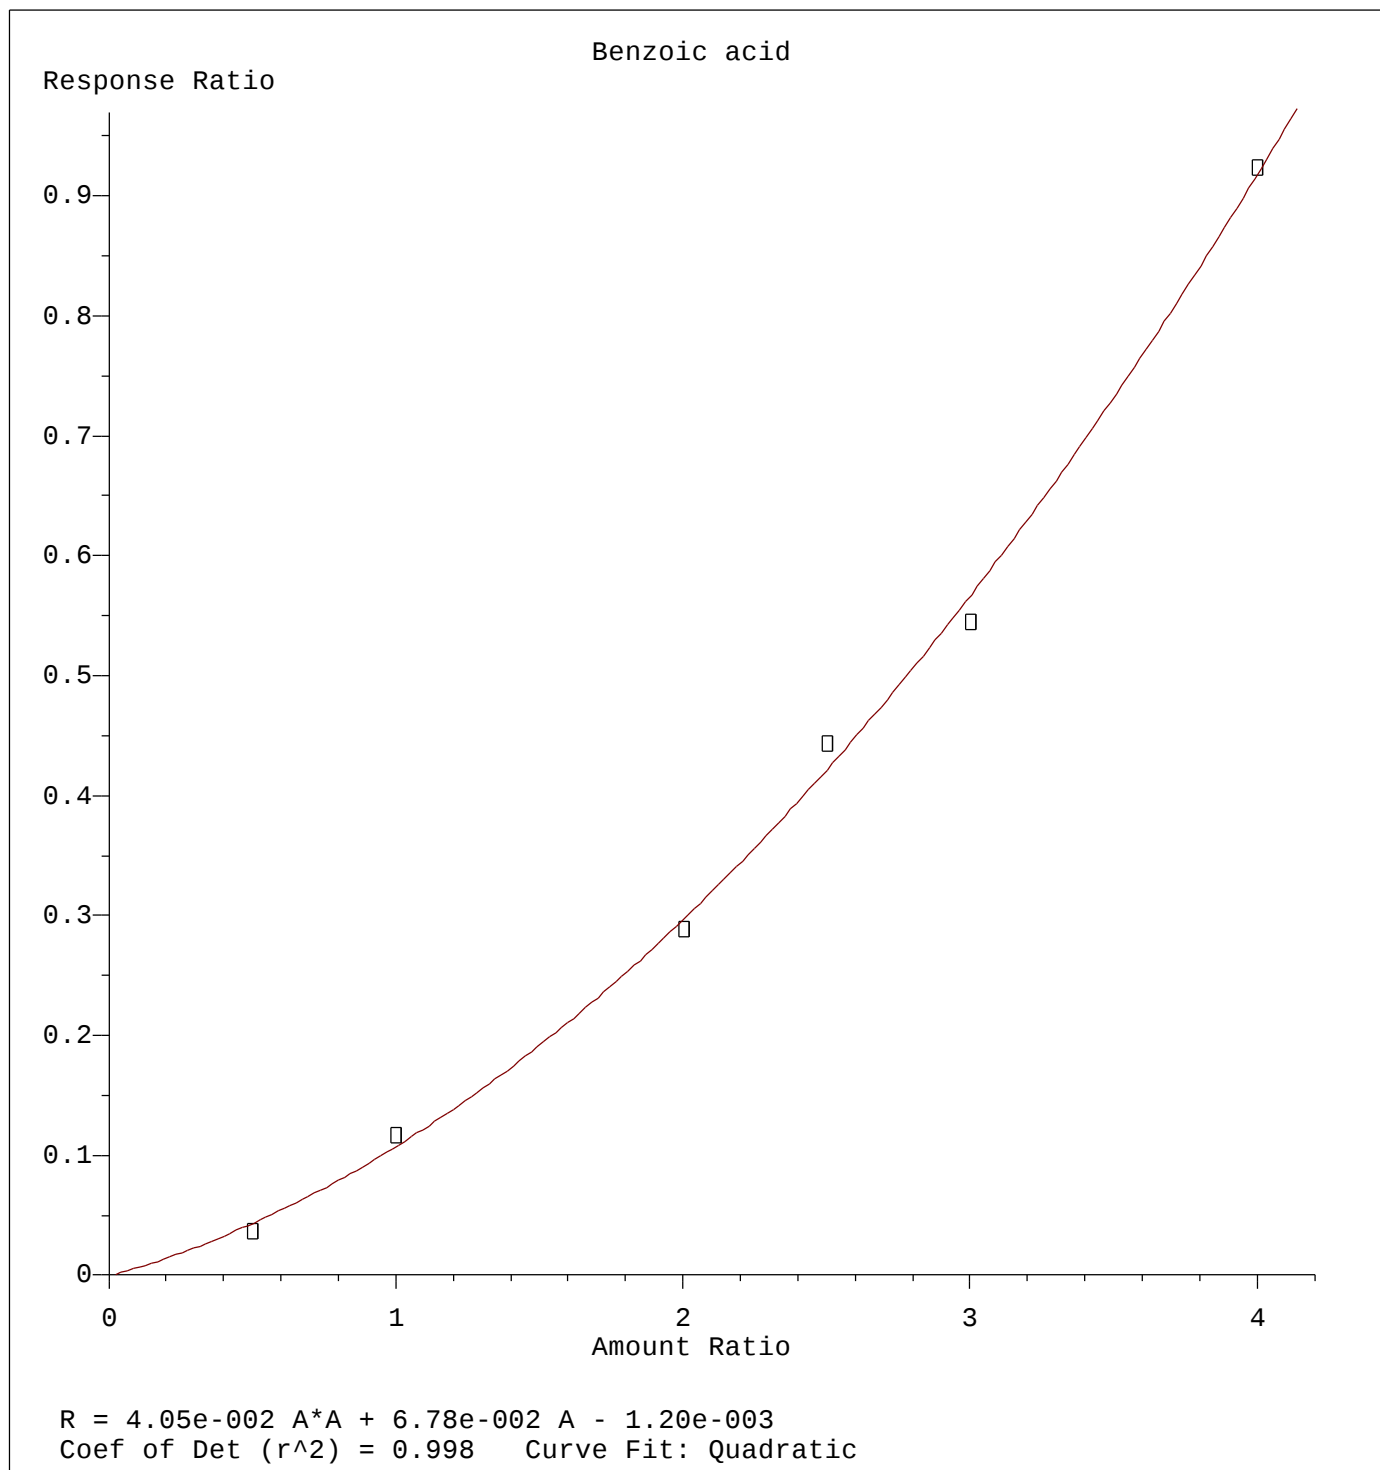

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG062619.M
Calibration Table Last Updated: Thu Jun 27 13:25:55 2019

Hexachlorocyclopentadiene

Response Ratio

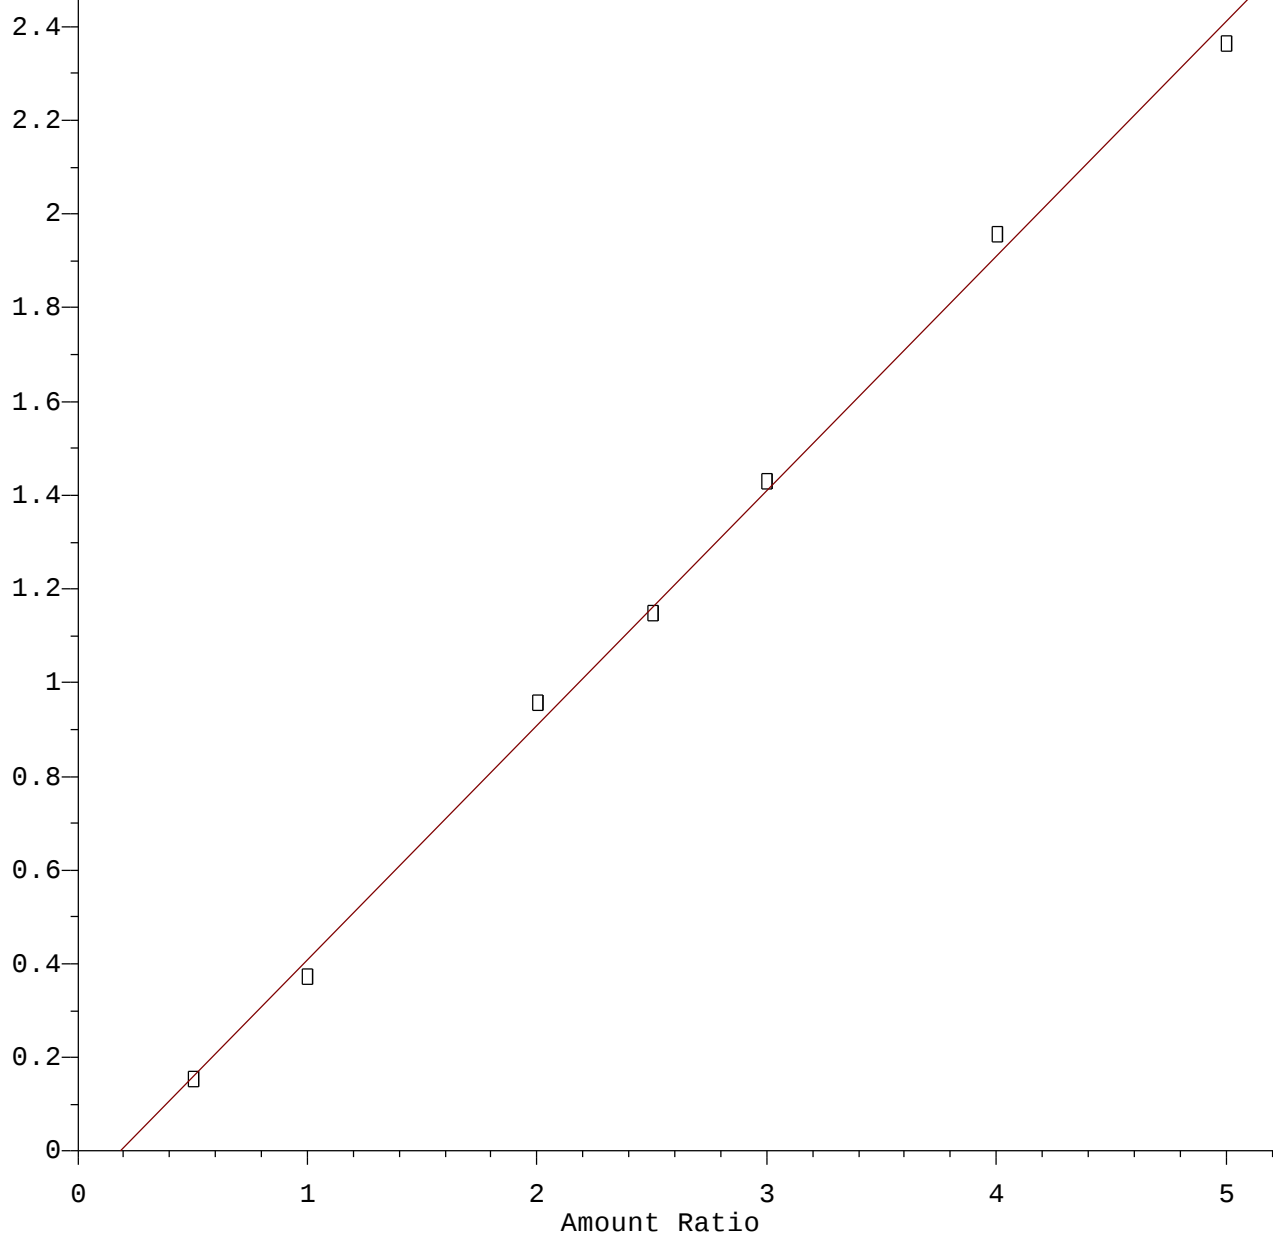


Resp Ratio = $5.01 \times 10^{-1} \times \text{Amt} - 9.13 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG062619.M
Calibration Table Last Updated: Thu Jun 27 13:25:55 2019

2,4-Dinitrophenol

Response Ratio

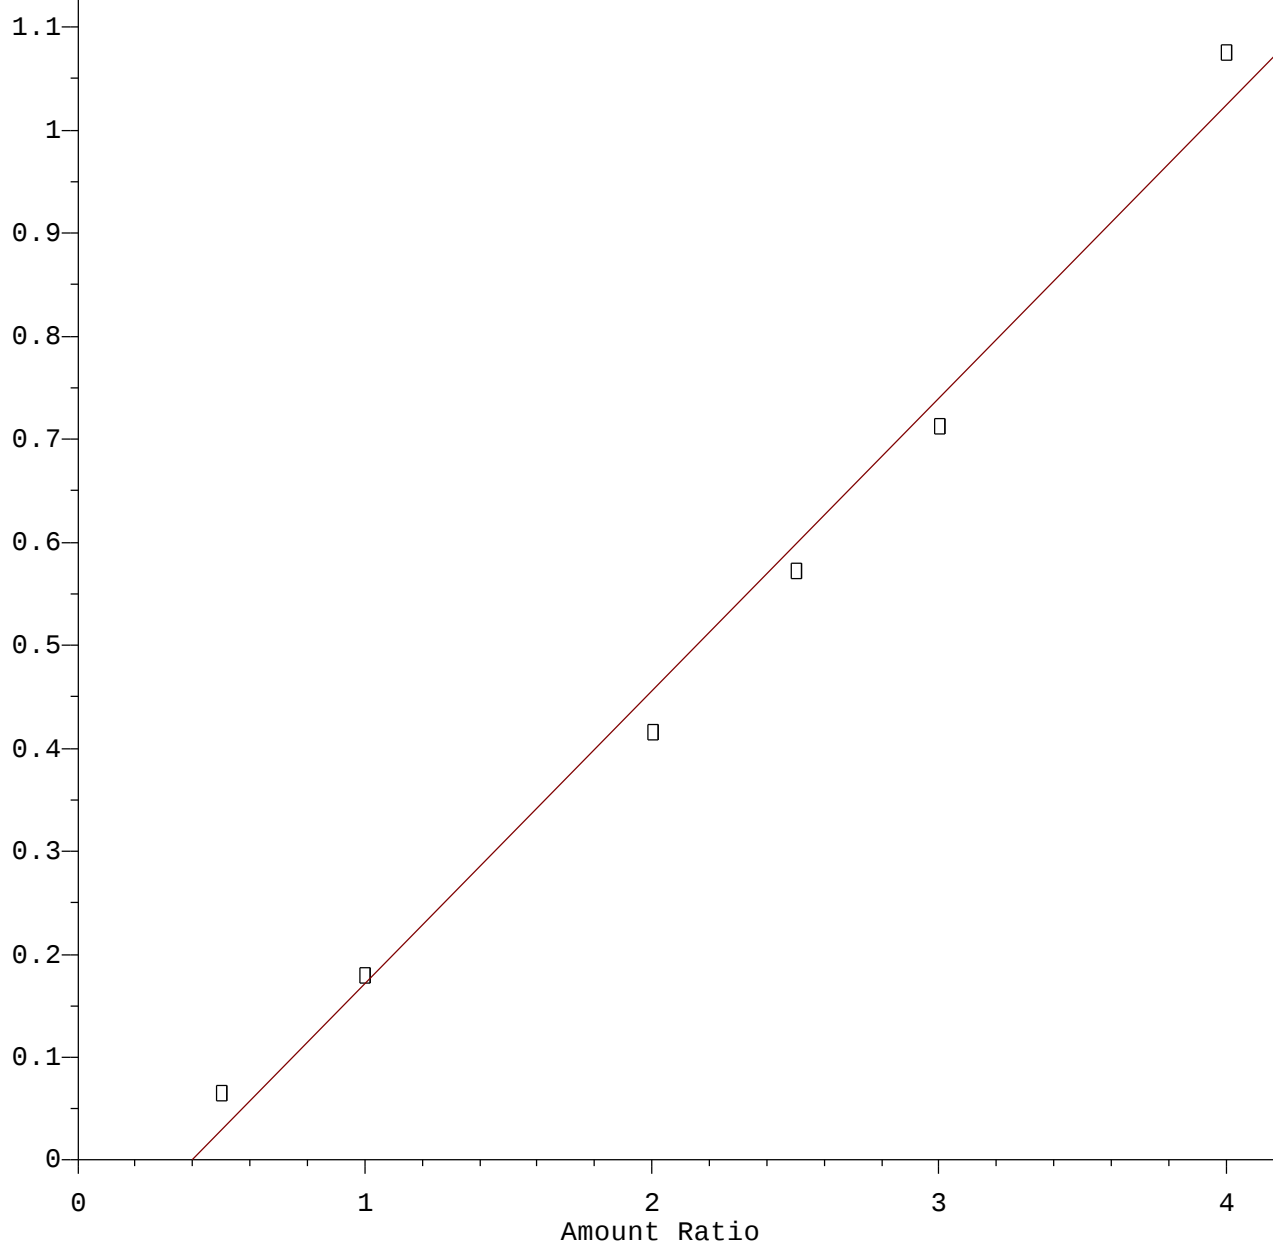

Resp Ratio = $2.84 \times 10^{-1} \times \text{Amt} - 1.13 \times 10^{-1}$
Coef of Det (r^2) = 0.990 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG062619.M
Calibration Table Last Updated: Thu Jun 27 13:25:55 2019