
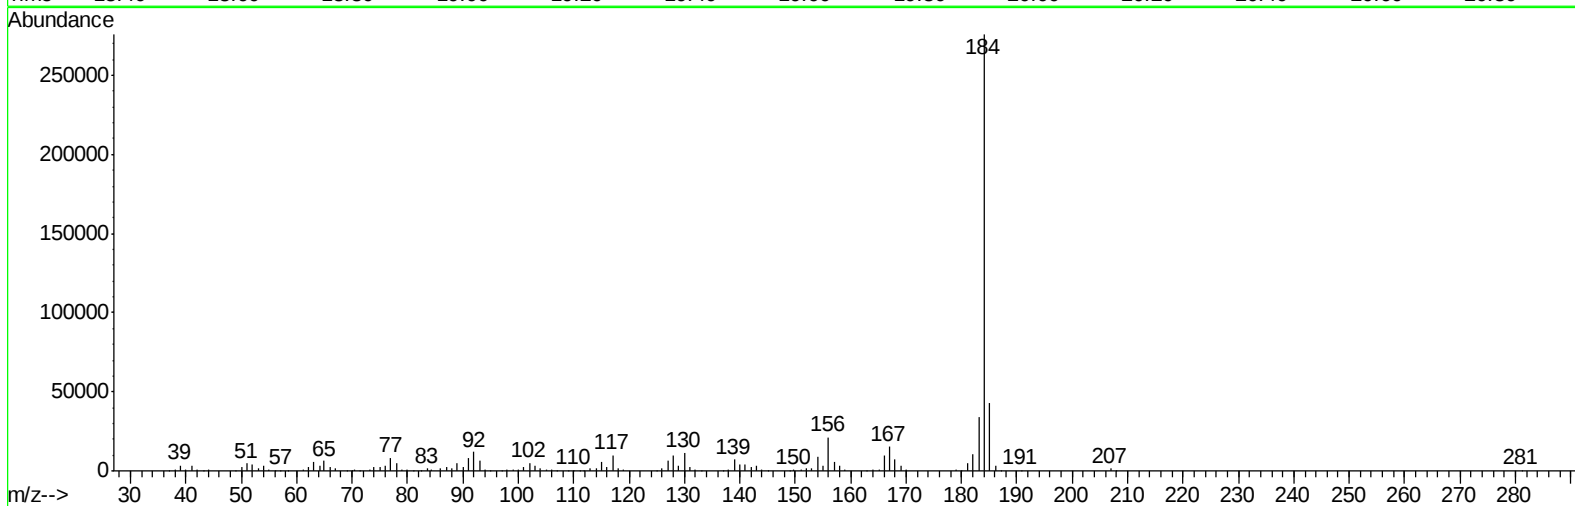


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062619\
Data File : BG041461.D
Acq On : 26 Jun 2019 8:52
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 04:37:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 26 15:47:16 2019
Response via : Initial Calibration

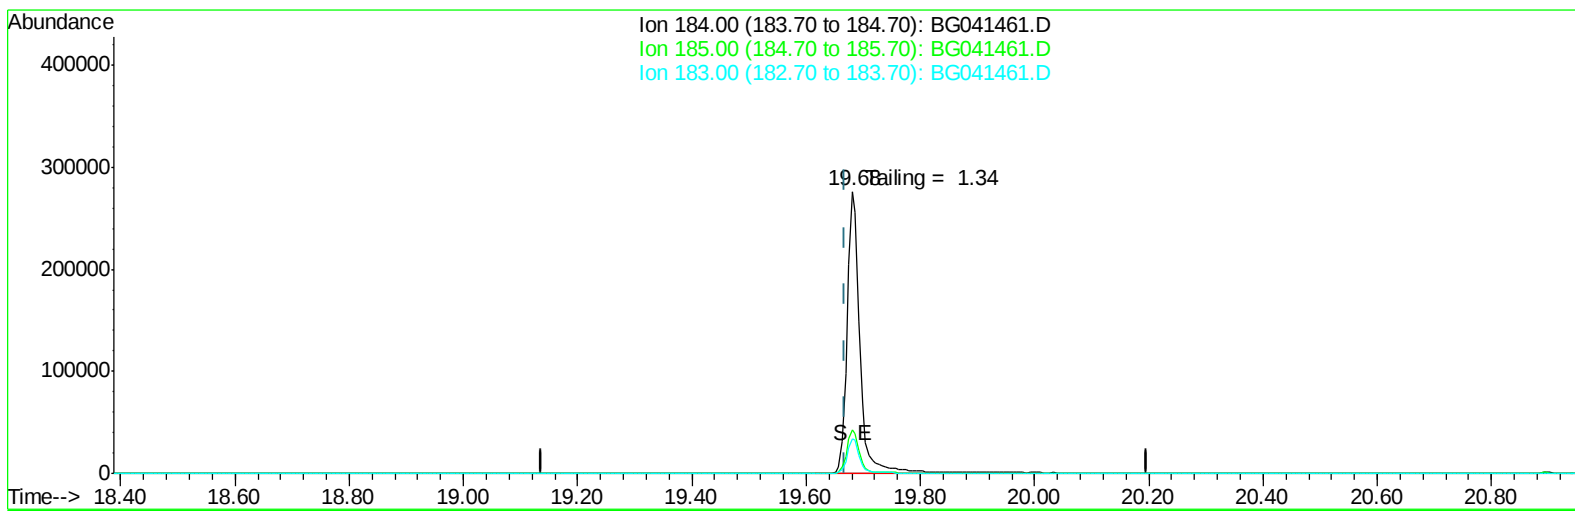

TIC: BG041461.D

(77) Benzidine

19.680min (+0.013) 0.00ng

response 434115

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.61
183.00	11.30	12.34
0.00	0.00	0.00

