


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062619\
 Data File : BG041461.D
 Acq On : 26 Jun 2019 8:52
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG062619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 27 13:25:55 2019

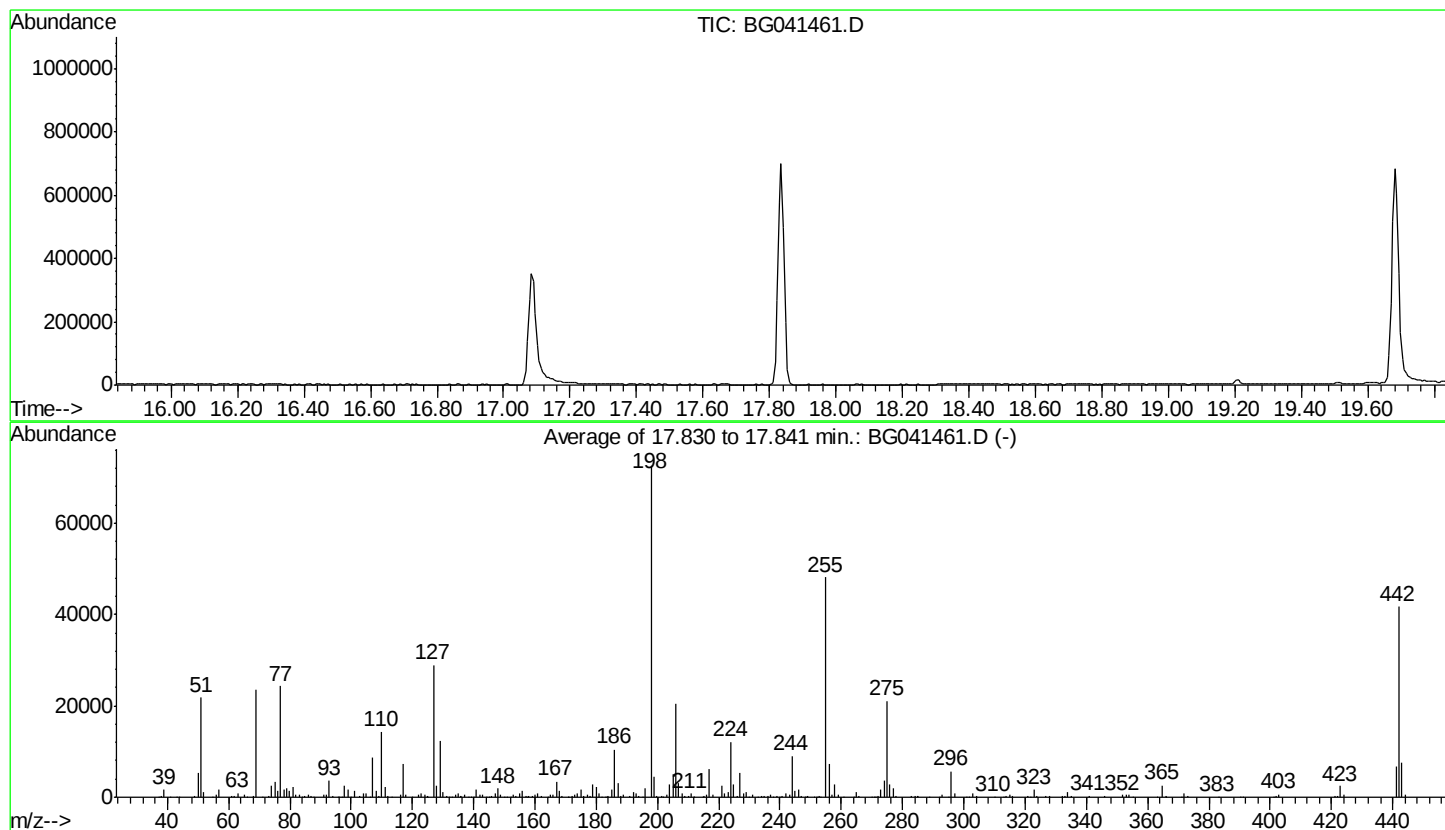

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	21748	PASS
68	69	0.00	2	1.4	320	PASS
69	198	0.00	100	32.6	23646	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.9	28930	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72562	PASS
199	198	5	9	6.2	4519	PASS
275	198	10	60	29.1	21098	PASS
365	198	1	100	3.5	2548	PASS
441	198	0.01	100	9.1	6600	PASS
442	198	50	100	57.4	41677	PASS
443	442	15	24	18.2	7598	PASS