
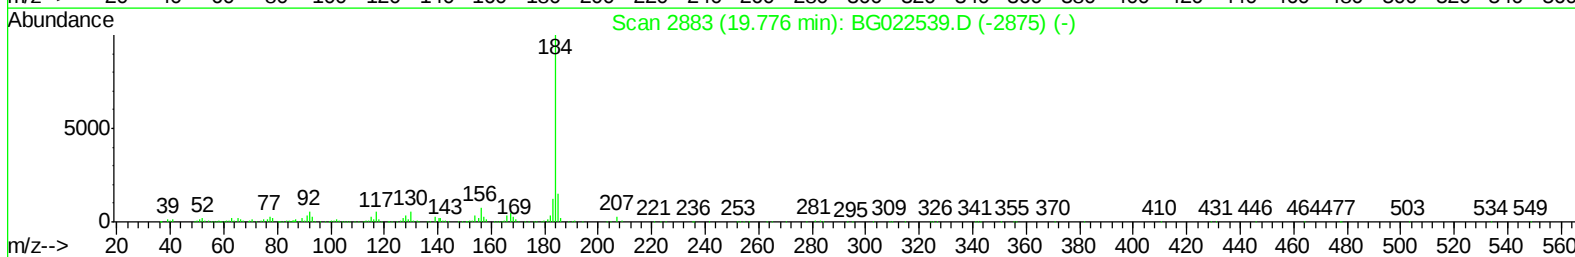
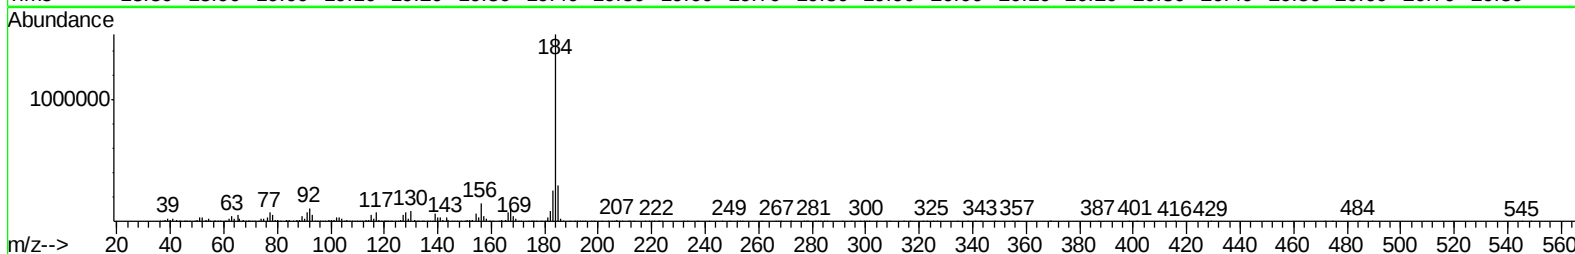


Data Path : Z:\HPCHEM1\BNA_G\Data\BG062716\
 Data File : BG022633.D
 Acq On : 27 Jun 2016 8:22
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 09:04:18 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 20:14:59 2016
 Response via : Initial Calibration

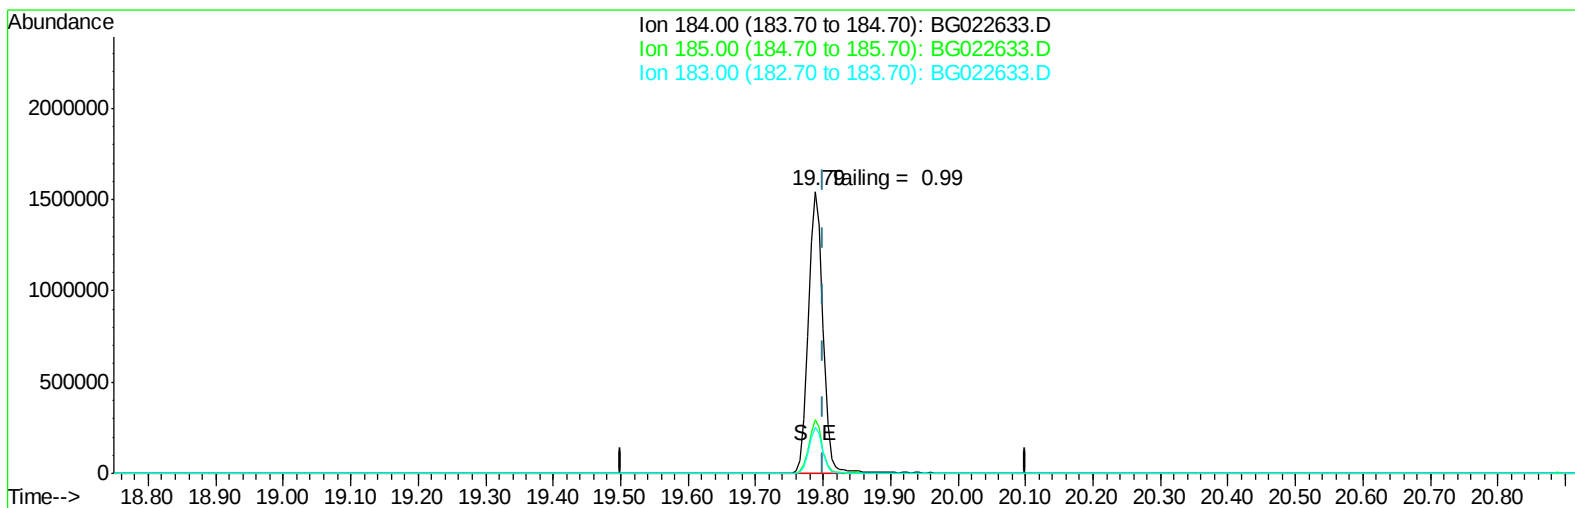

TIC: BG022633.D

(76) Benzidine




19.789min (-0.012) 129270.37ng

response 2341081

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	19.28#
183.00	13.40	16.41#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG062716\
Data File : BG022633.D
Acq On : 27 Jun 2016 8:22
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 09:04:18 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

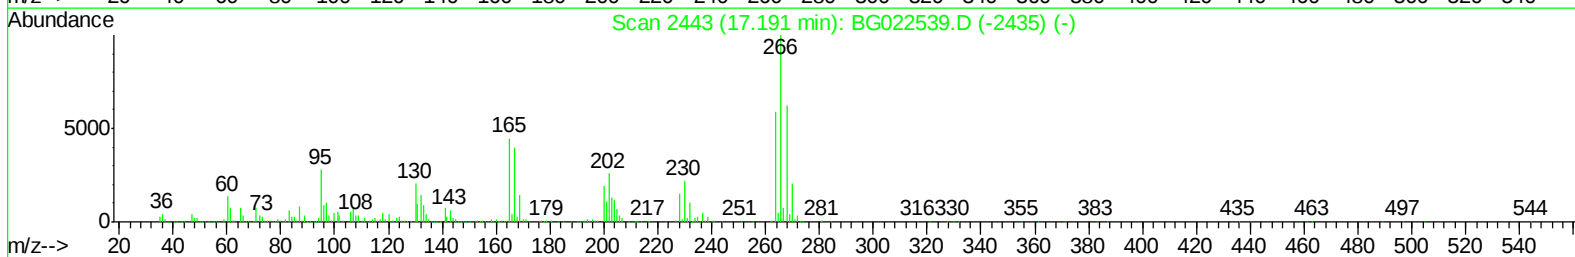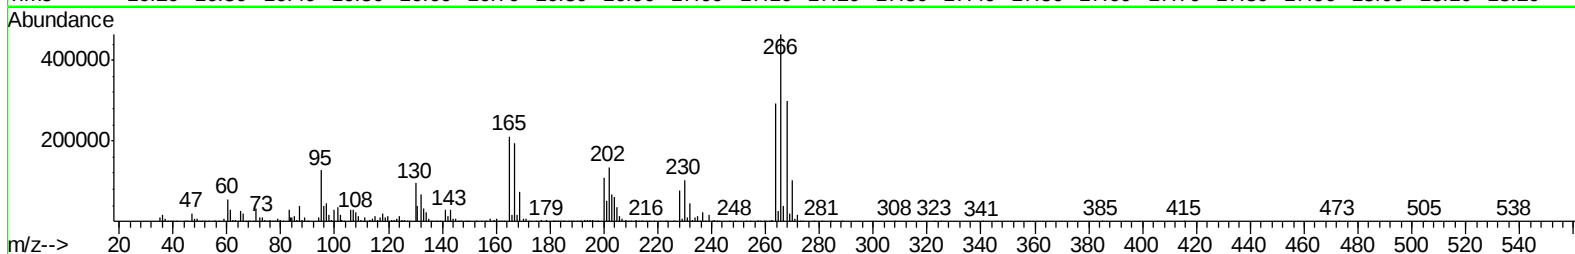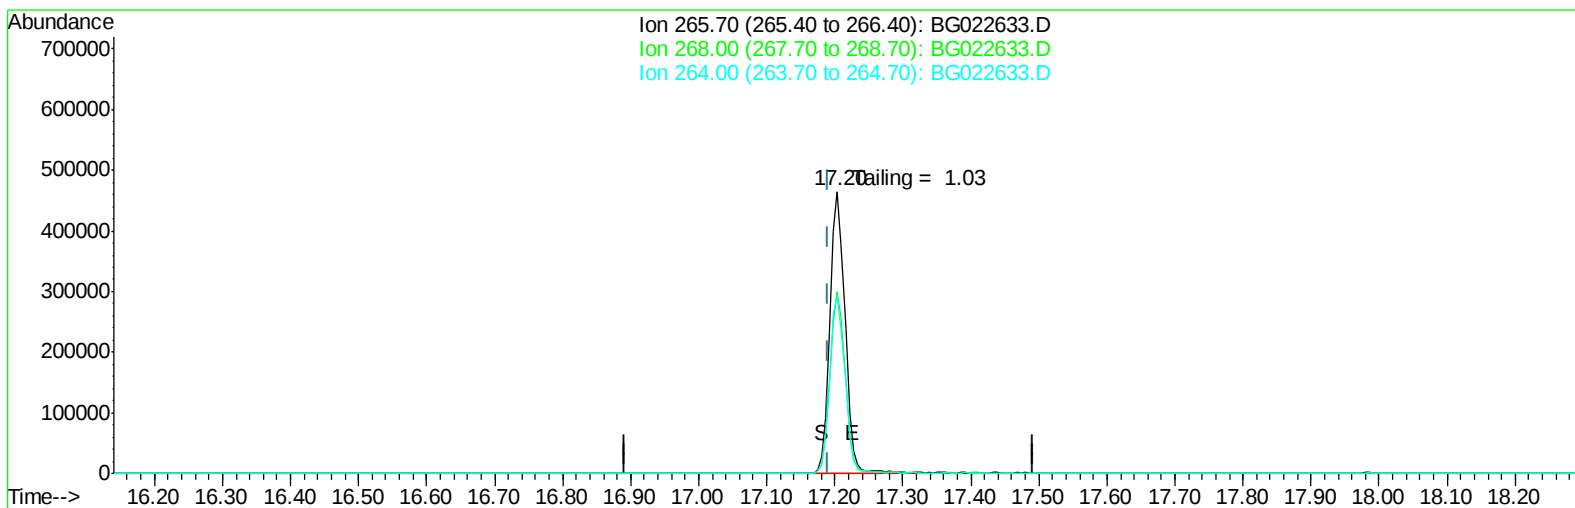

TIC: BG022633.D

(69) Pentachlorophenol (C)

17.204min (+0.012) 73047.68ng

response 714402

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	64.54
264.00	63.20	63.37
0.00	0.00	0.00