
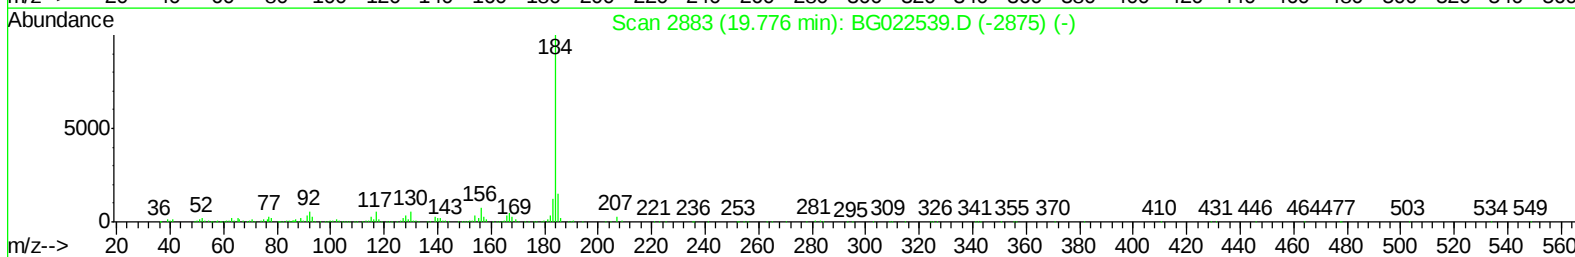
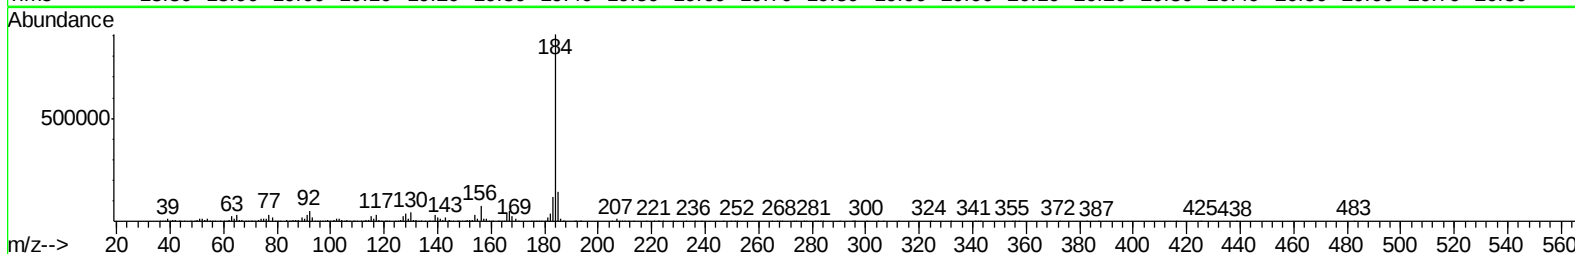


Data Path : Z:\HPCHEM1\BNA_G\Data\BG062716\
Data File : BG022650.D
Acq On : 27 Jun 2016 19:58
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 09:07:14 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

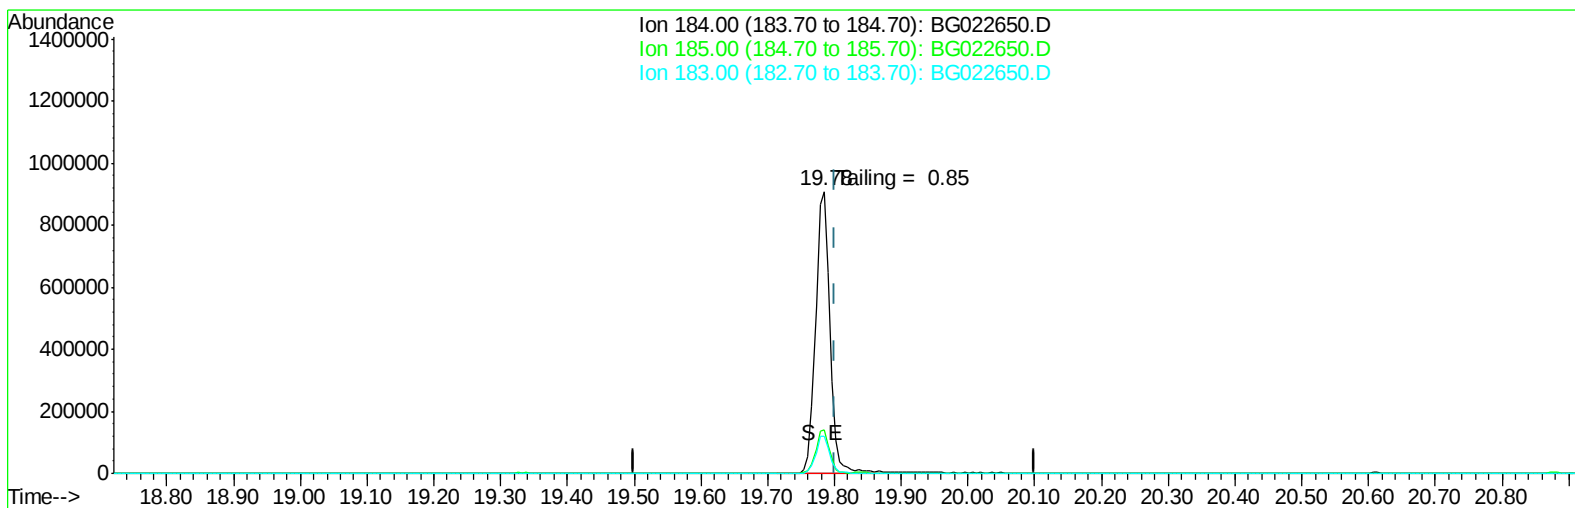

TIC: BG022650.D

(76) Benzidine




19.784min (-0.017) 260436.98ng

response 1350345

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.64
183.00	13.40	13.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG062716\
Data File : BG022650.D
Acq On : 27 Jun 2016 19:58
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 09:07:14 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

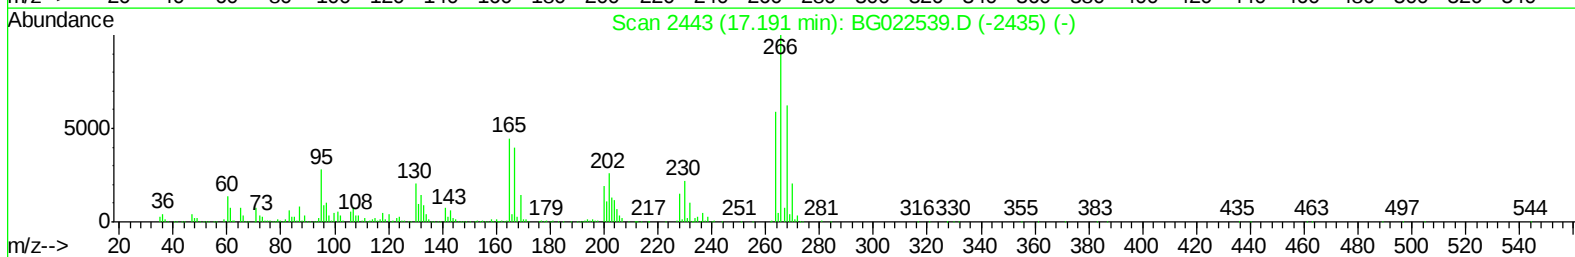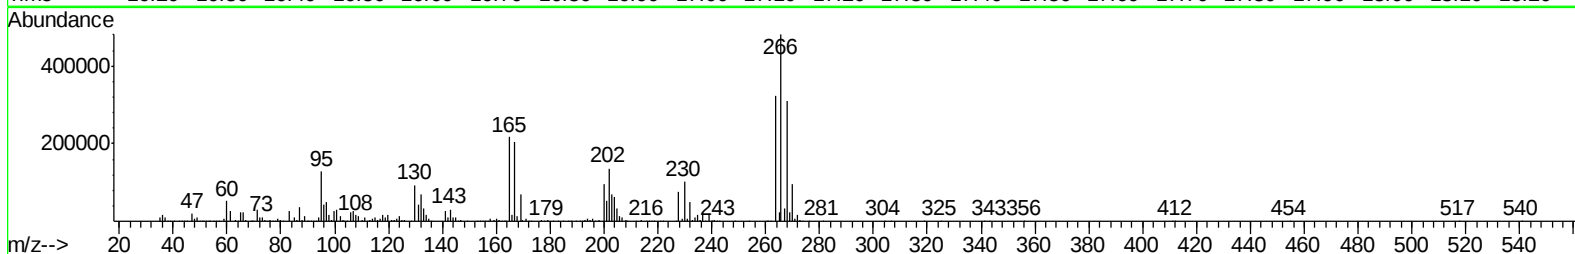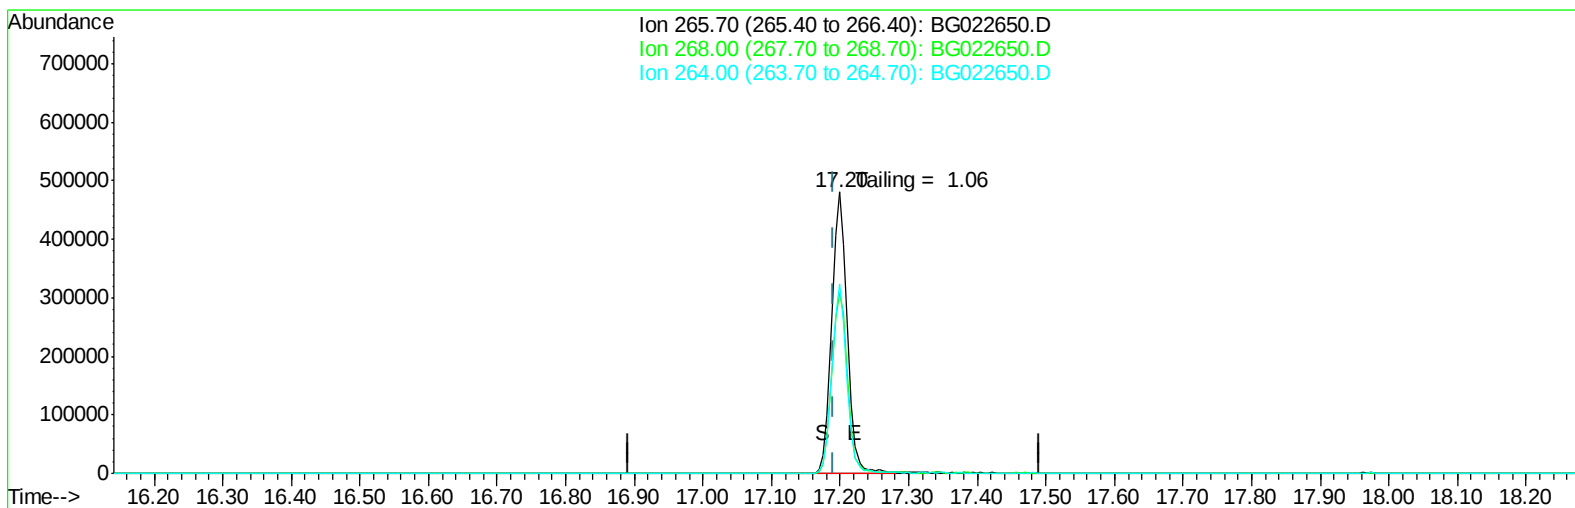

TIC: BG022650.D

(69) Pentachlorophenol (C)

17.199min (+0.007) 1129242.31ng

response 746211

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	64.31
264.00	63.20	67.06
0.00	0.00	0.00