


Data Path : Z:\HPCHEM1\BNA G\DATA\BG062716\
 Data File : BG022650.D
 Acq On : 27 Jun 2016 19:58
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 24 20:14:59 2016

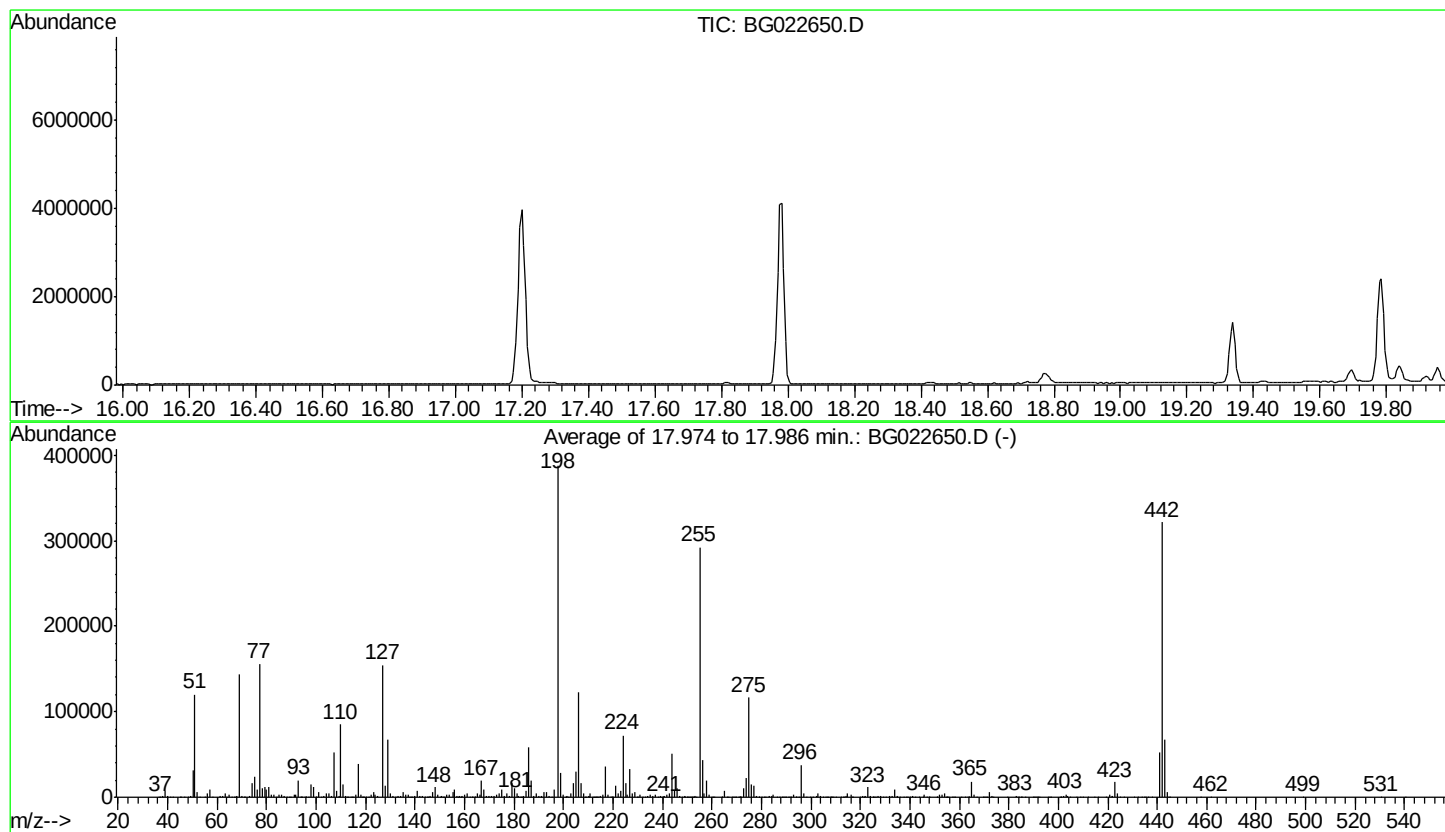

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	120093	PASS
68	69	0.00	2	1.4	2063	PASS
69	198	0.00	100	37.0	143450	PASS
70	69	0.00	2	0.8	1183	PASS
127	198	10	80	39.9	154680	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	387626	PASS
199	198	5	9	7.3	28282	PASS
275	198	10	60	30.1	116685	PASS
365	198	1	100	4.7	18263	PASS
441	442	0.01	24	16.3	52400	PASS
442	198	50	100	83.0	321664	PASS
443	442	15	24	20.9	67322	PASS