
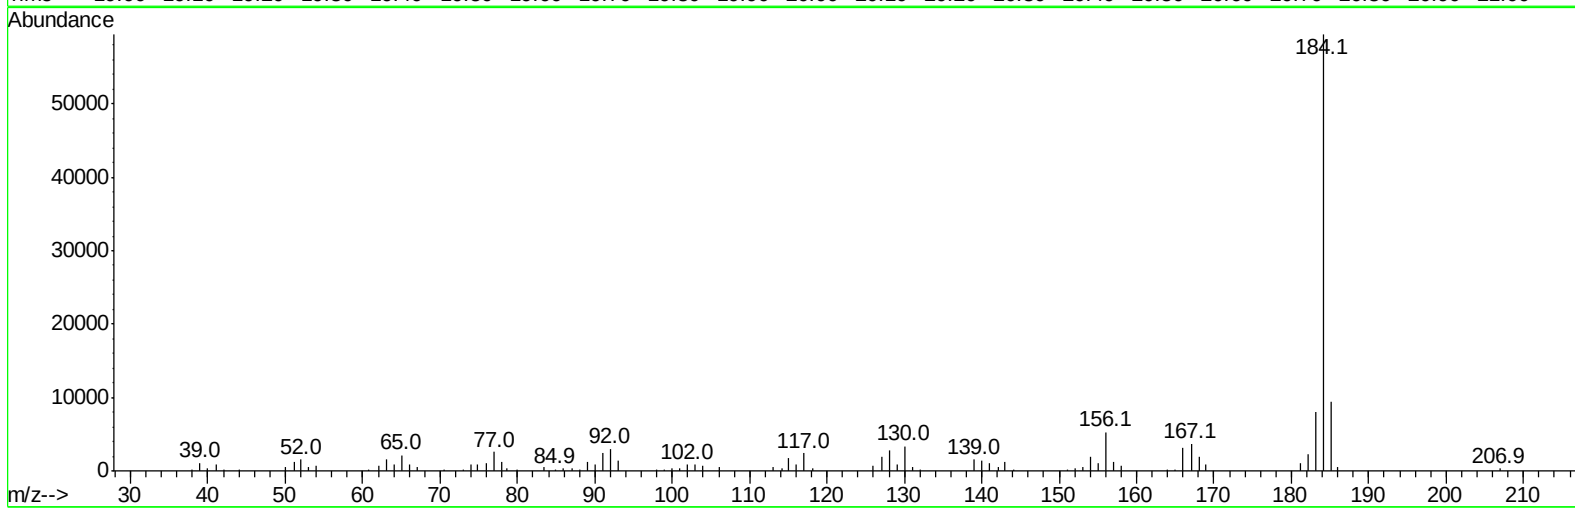


Data Path : Z:\HPCHEM1\BNA G\DATA\BG062717\
Data File : BG027693.D
Acq On : 27 Jun 2017 8:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 02:55:10 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 18:52:15 2017
Response via : Initial Calibration

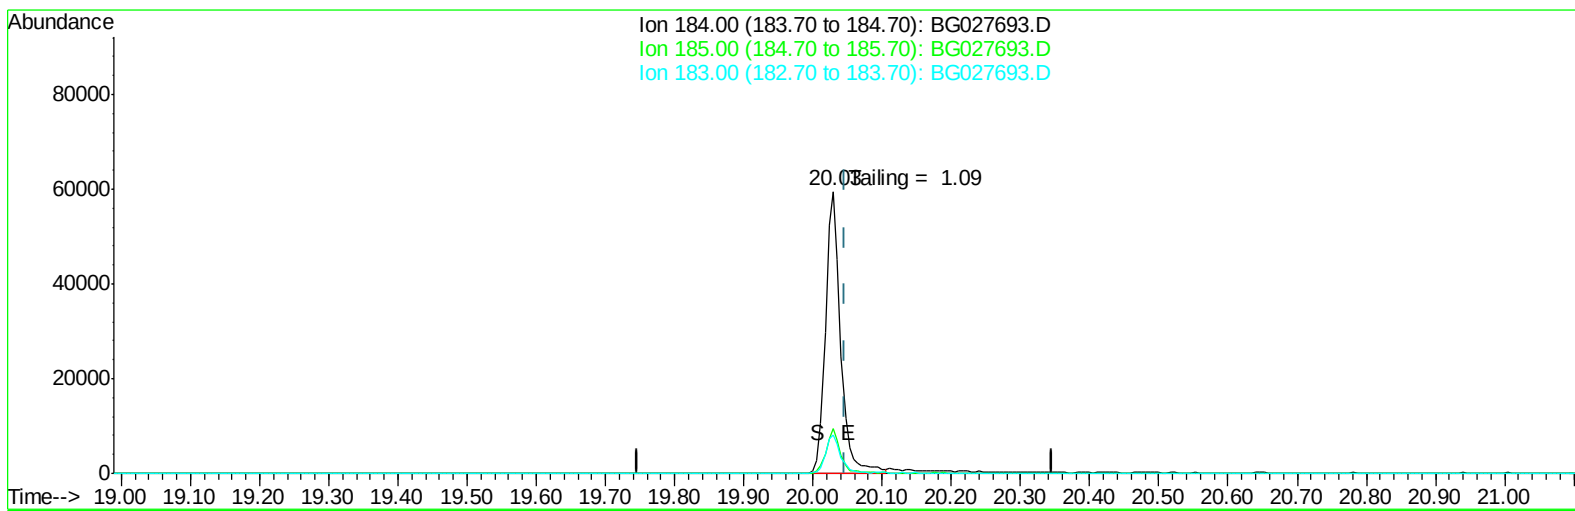

TIC: BG027693.D

(76) Benzidine



20.029min (-0.018) 64679.19ng

response 90484

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.84
183.00	13.80	13.54
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062717\
Data File : BG027693.D
Acq On : 27 Jun 2017 8:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 02:55:10 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 18:52:15 2017
Response via : Initial Calibration

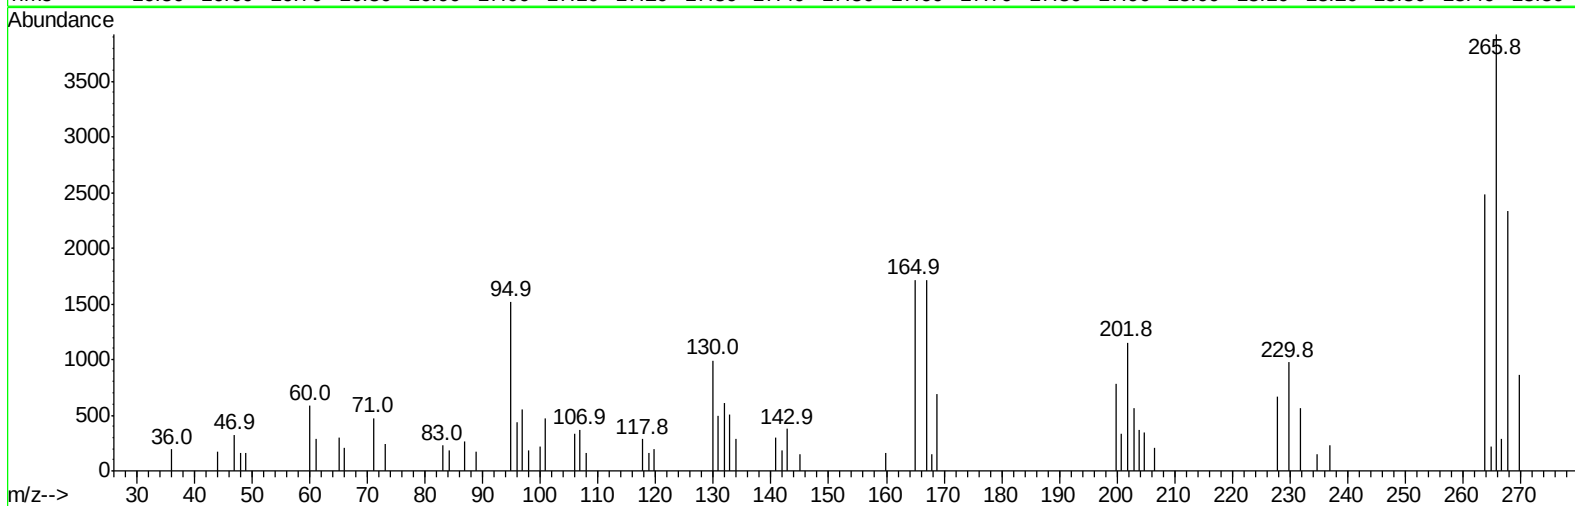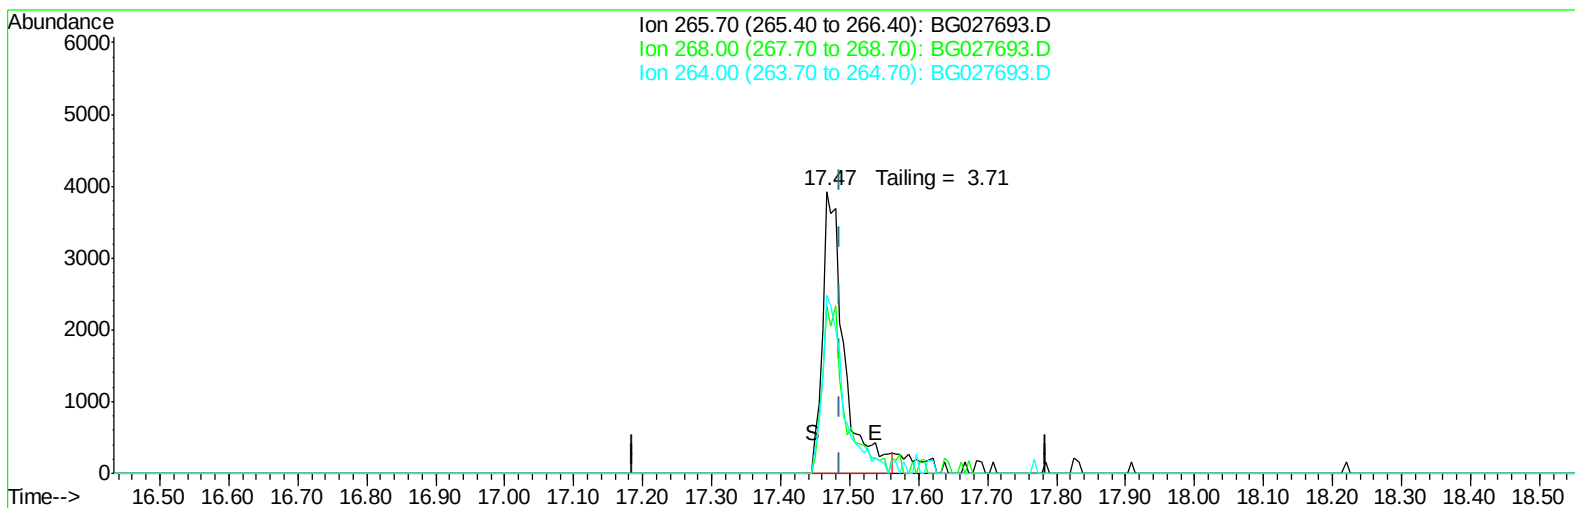

TIC: BG027693.D

(69) Pentachlorophenol (C)

17.467min (-0.018) 0.00ng

response 8471

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	59.59
264.00	62.60	63.36
0.00	0.00	0.00